

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032419\
 Data File : P0054539.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 13:17
 Operator : SM/SJ
 Sample : K1963-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BP-EB02-20190314

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 05:26:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 05:05:57 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.308	3.627	625912	601794	17.915	18.161
2) SA Decachlor...	9.931	8.611	730963	515927	15.545	15.518

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032419\
Data File : P0054539.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 13:17
Operator : SM/SJ
Sample : K1963-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BP-EB02-20190314

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 05:26:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032319.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 05:05:57 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

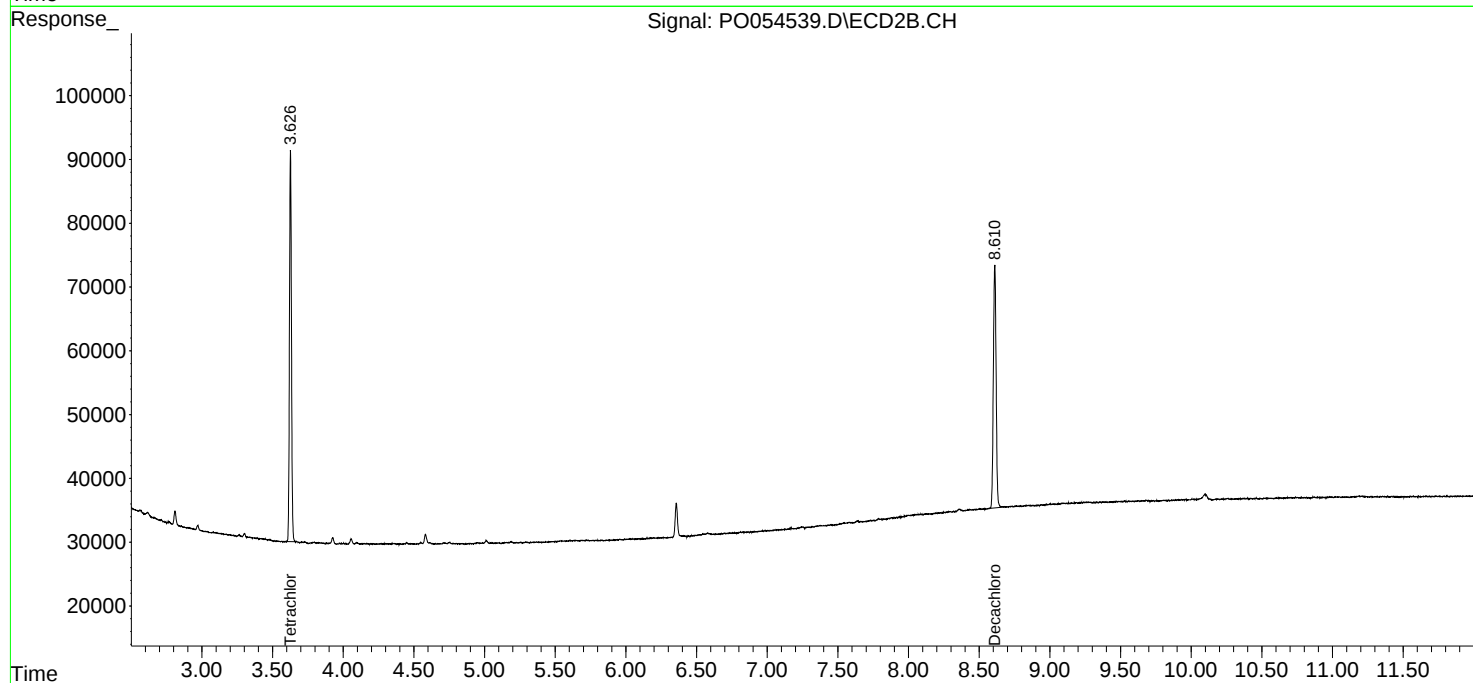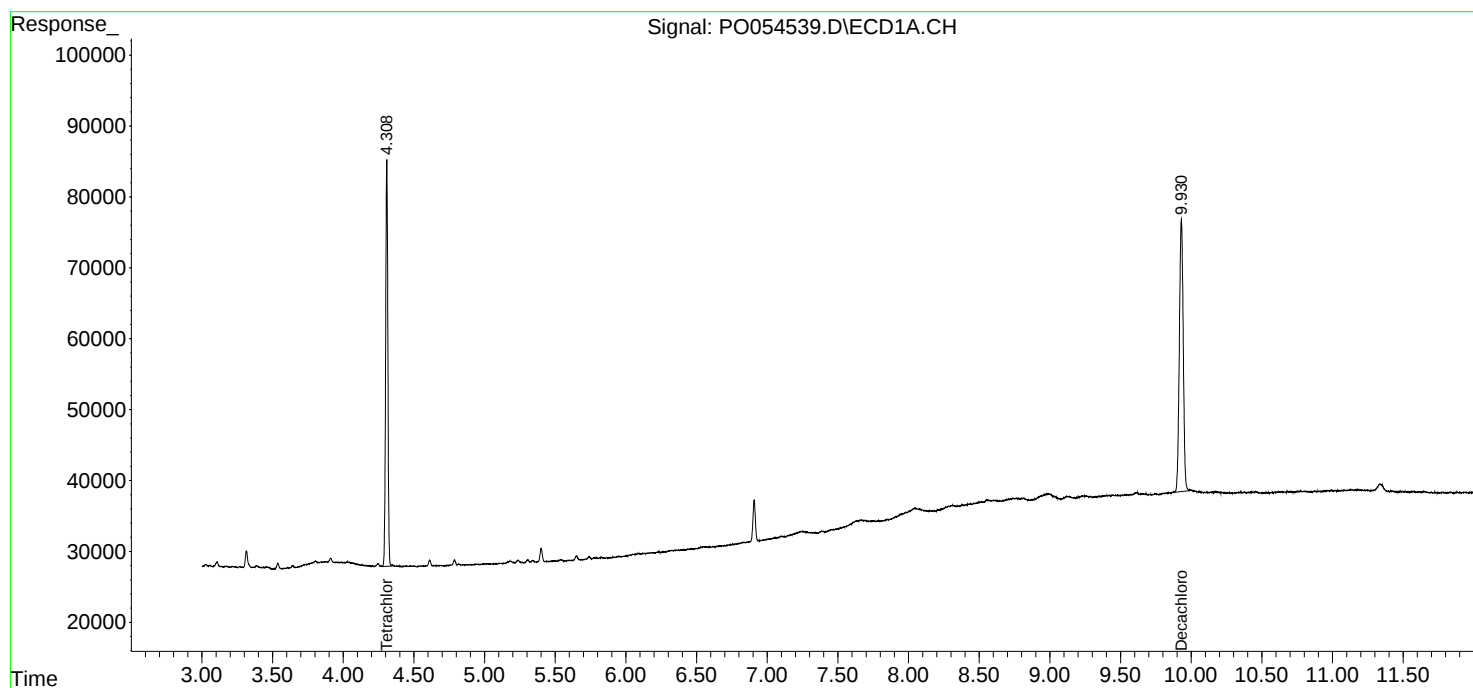


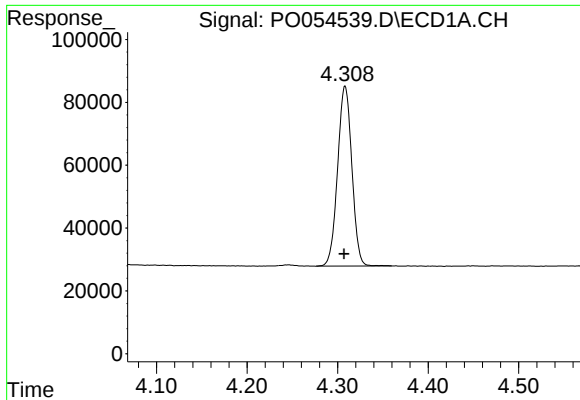

#1 Tetrachloro-m-xylene


R.T.: 4.308 min
Delta R.T.: 0.001 min
Response: 625912
Conc: 17.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
BP-EB02-20190314

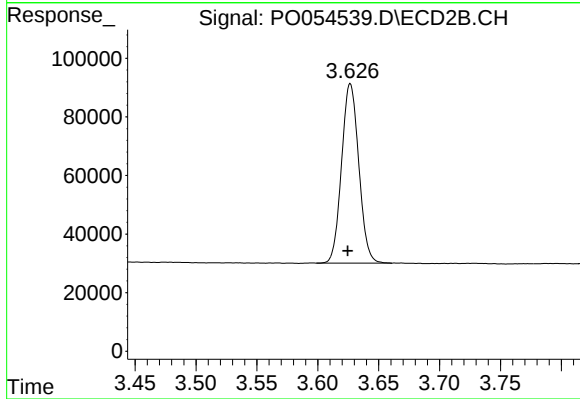


#1 Tetrachloro-m-xylene

R.T.: 3.627 min
Delta R.T.: 0.002 min
Response: 601794
Conc: 18.16 ng/ml

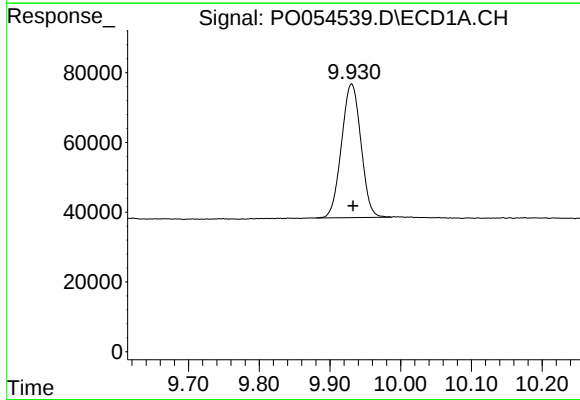

#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.002 min
Response: 730963
Conc: 15.55 ng/ml

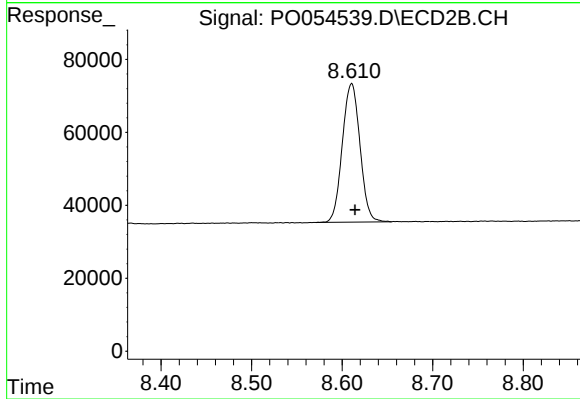

#2 Decachlorobiphenyl

R.T.: 8.611 min
Delta R.T.: -0.004 min
Response: 515927
Conc: 15.52 ng/ml