

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032419\
 Data File : P0054546.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 15:16
 Operator : SM/SJ
 Sample : K1900-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BPS1-TT-MW309D-20190313

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 05:30:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 05:05:57 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.308	3.627	718480	688314	20.564	20.772
2) SA Decachlor...	9.930	8.611	859930	600415	18.288	18.059

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032419\
Data File : P0054546.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 15:16
Operator : SM/SJ
Sample : K1900-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BPS1-TT-MW309D-20190313

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 05:30:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032319.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 05:05:57 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

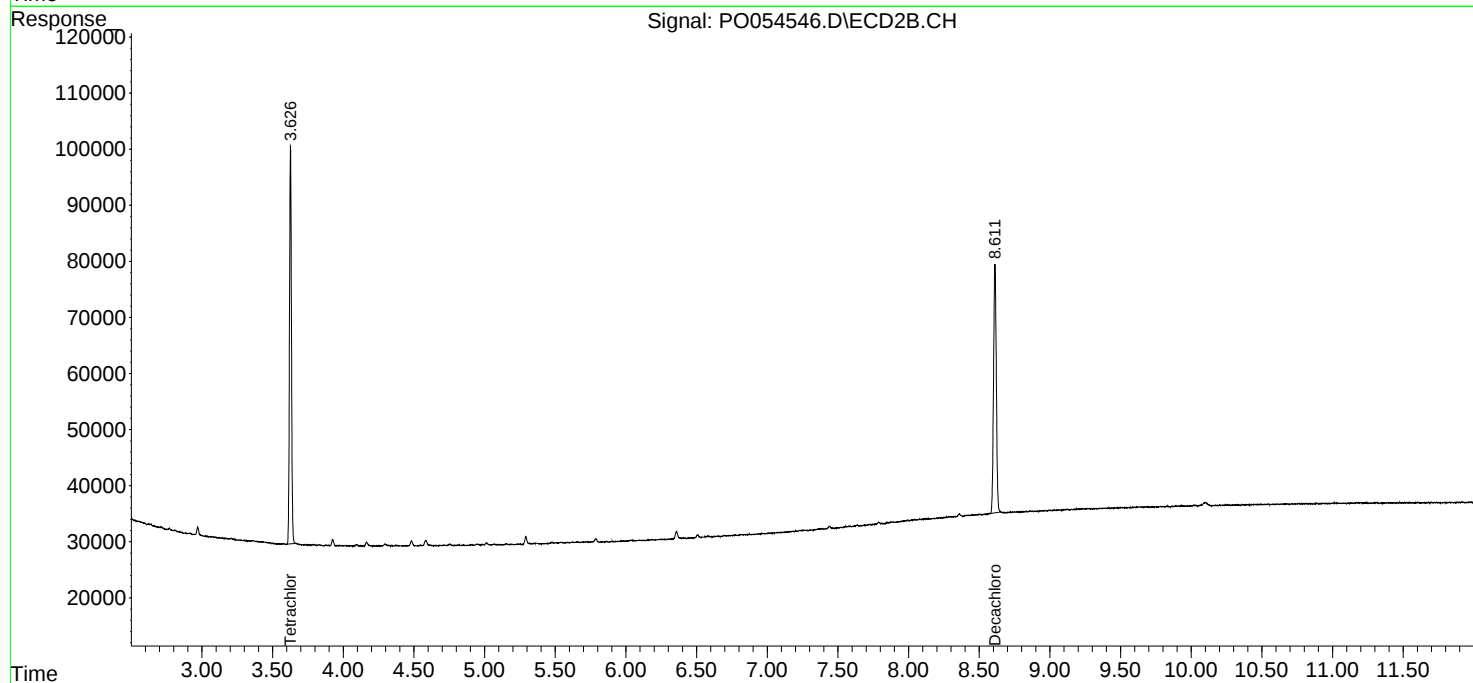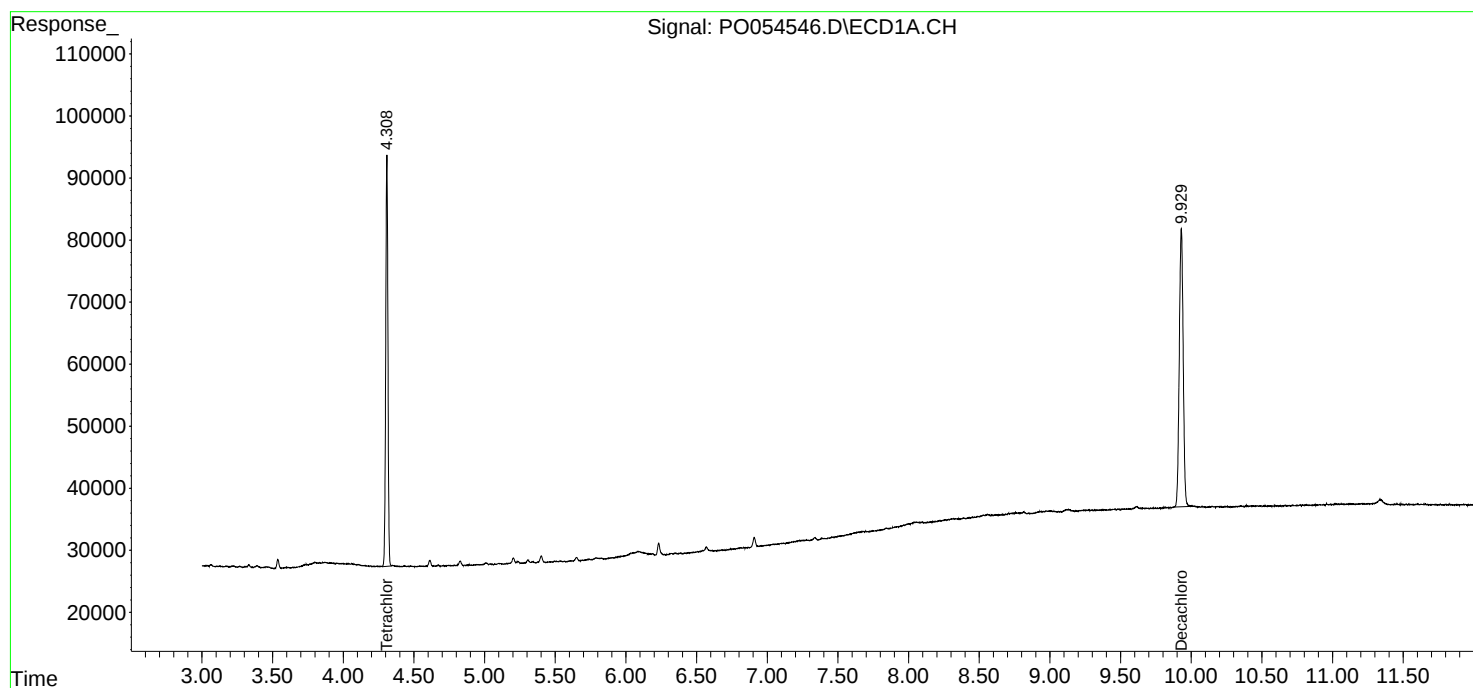


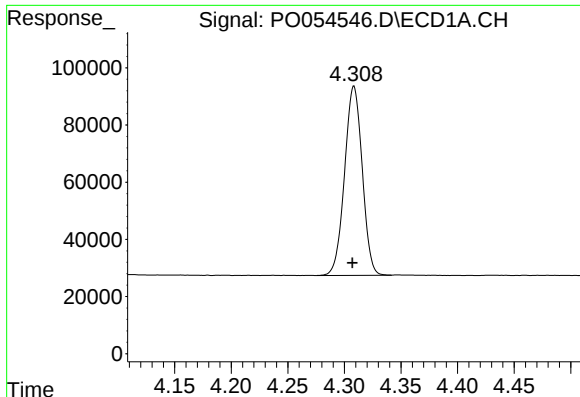

#1 Tetrachloro-m-xylene


R.T.: 4.308 min
Delta R.T.: 0.001 min
Response: 718480
Conc: 20.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-TT-MW309D-20190313

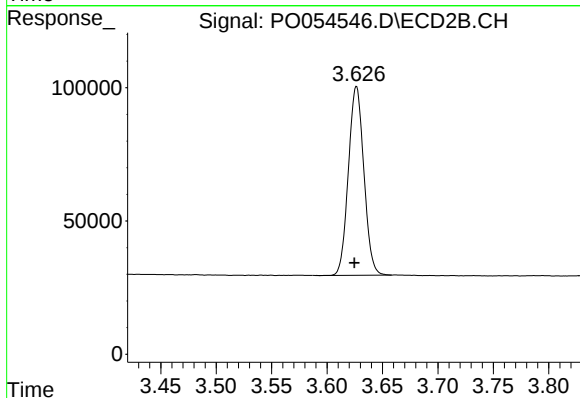


#1 Tetrachloro-m-xylene

R.T.: 3.627 min
Delta R.T.: 0.002 min
Response: 688314
Conc: 20.77 ng/ml

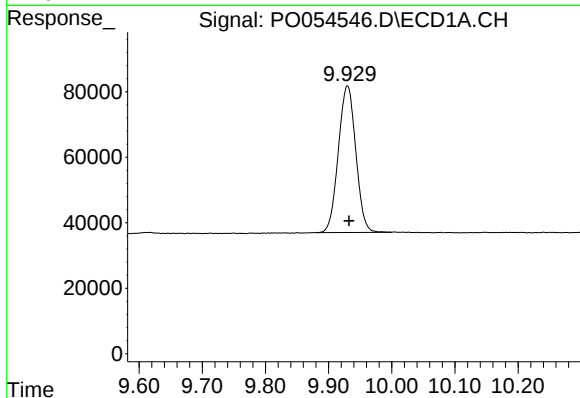

#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: -0.003 min
Response: 859930
Conc: 18.29 ng/ml

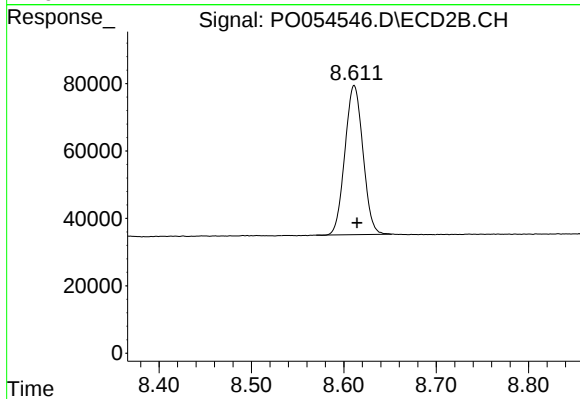

#2 Decachlorobiphenyl

R.T.: 8.611 min
Delta R.T.: -0.003 min
Response: 600415
Conc: 18.06 ng/ml