

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032419\
 Data File : P0054564.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 20:21
 Operator : SM/SJ
 Sample : K2033-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 032019-LIFT-F-D-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 05:42:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 05:05:57 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.308	3.626	747779	685439	21.403	20.685
2) SA Decachlor...	9.932	8.610	779863	549407	16.585	16.525

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032419\
Data File : PO054564.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 20:21
Operator : SM/SJ
Sample : K2033-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
032019-LIFT-F-D-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 05:42:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032319.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 05:05:57 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

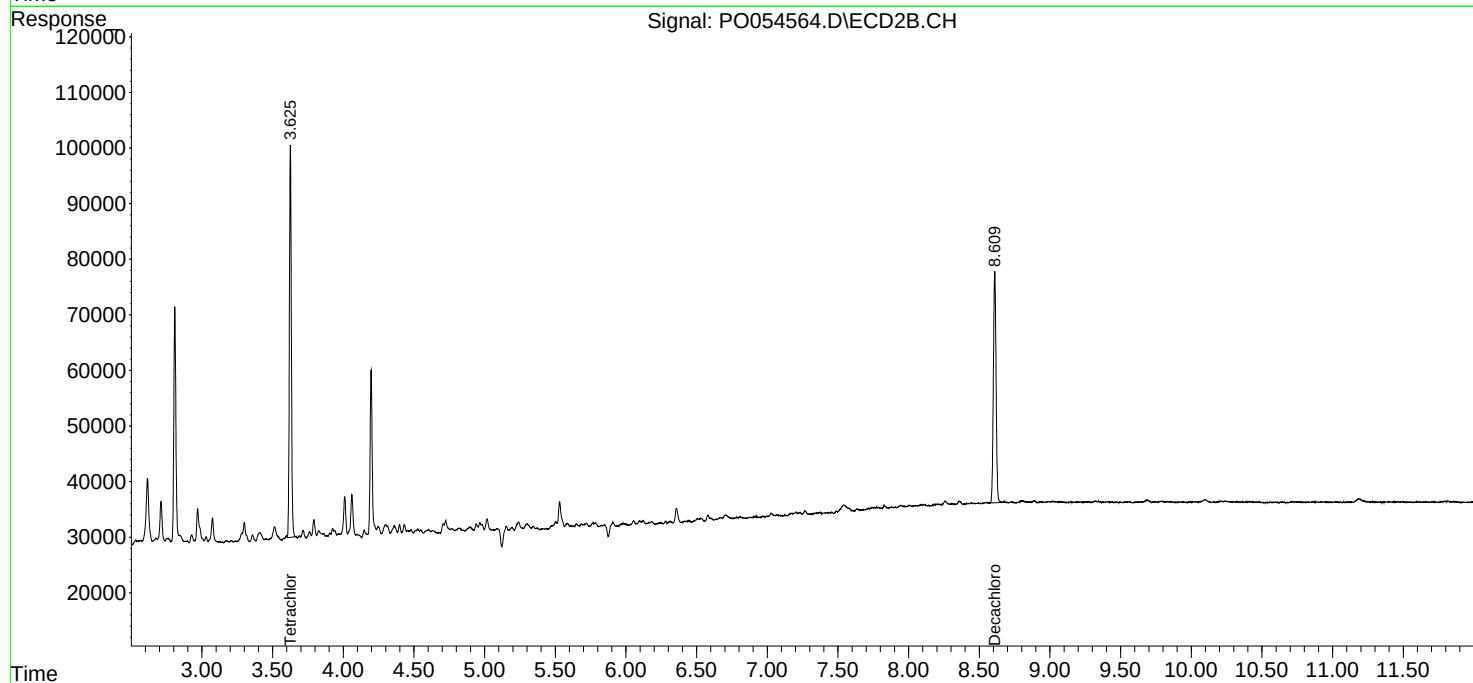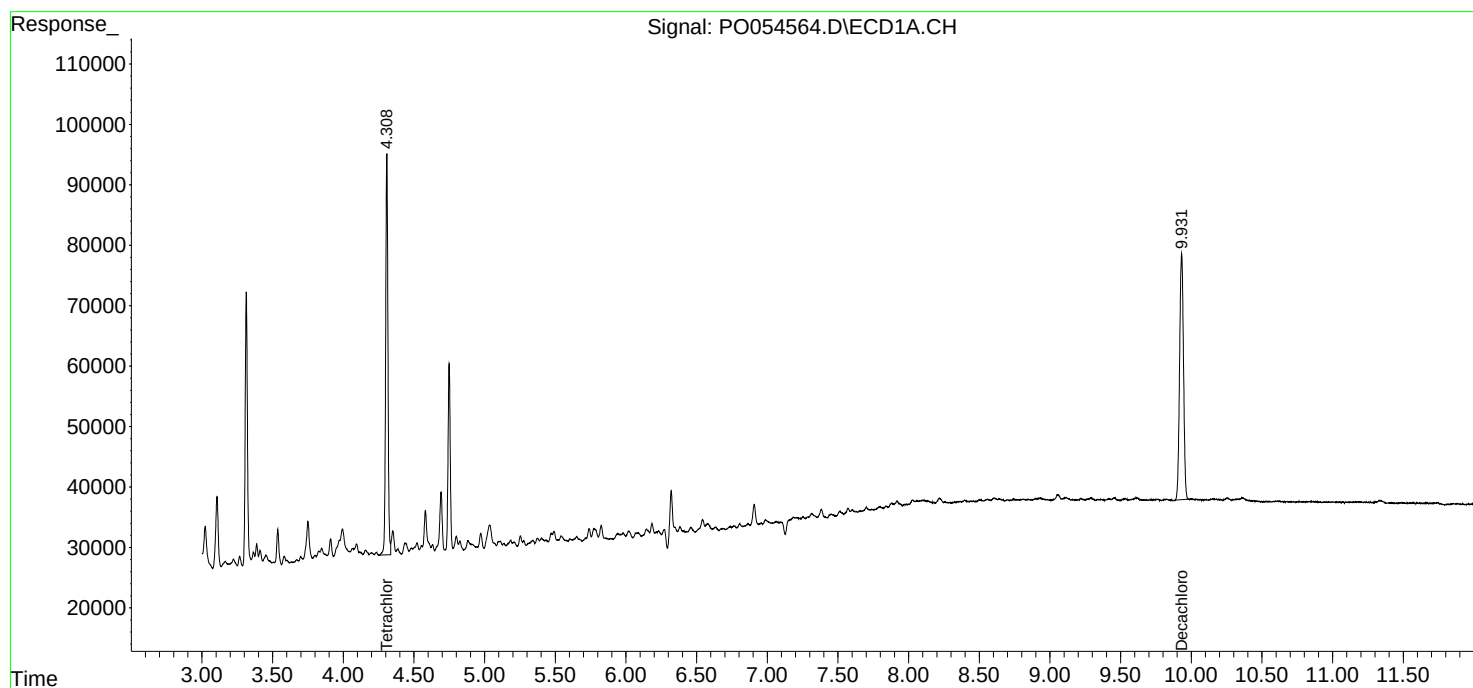


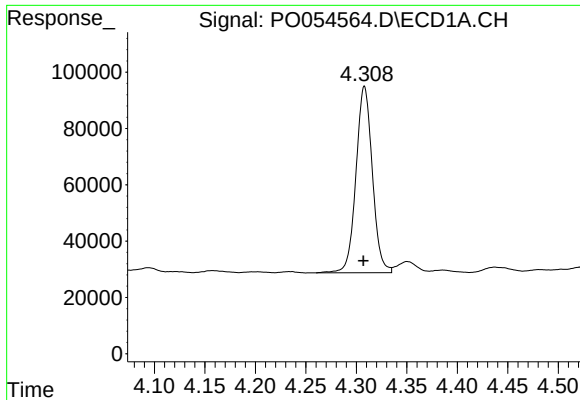

#1 Tetrachloro-m-xylene


R.T.: 4.308 min
Delta R.T.: 0.001 min
Response: 747779
Conc: 21.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
032019-LIFT-F-D-B

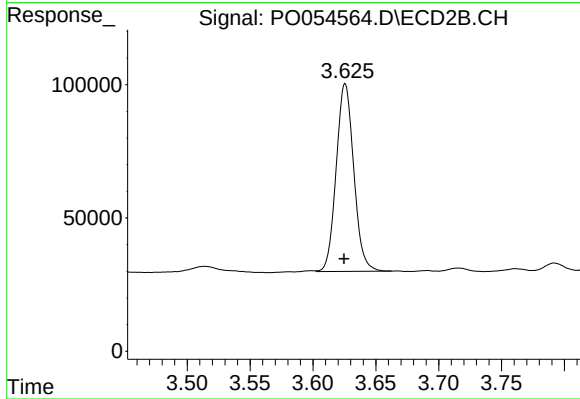


#1 Tetrachloro-m-xylene

R.T.: 3.626 min
Delta R.T.: 0.000 min
Response: 685439
Conc: 20.69 ng/ml

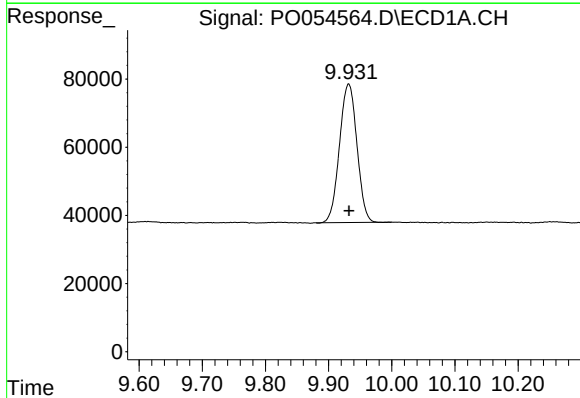

#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: 0.000 min
Response: 779863
Conc: 16.58 ng/ml

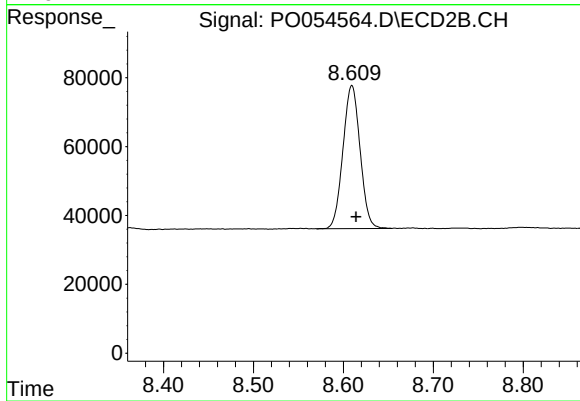

#2 Decachlorobiphenyl

R.T.: 8.610 min
Delta R.T.: -0.005 min
Response: 549407
Conc: 16.53 ng/ml