

Data Path : P:\HPCHEM1\ECD 0\Data\P0032618\
 Data File : P0043303.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2018 12:08
 Operator : SM/UA
 Sample : J1748-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-05-032218-D

Manual Integrations
 APPROVED

ugo
 3/28/2018 12:00:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:47:58 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 23 05:22:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.079	3.334	4025443	5922462	18.997	20.234
2) SA Decachlor...	9.428	8.098	1822644	2285229	7.505	6.390m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032618\
Data File : P0043303.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2018 12:08
Operator : SM/UA
Sample : J1748-13
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-05-032218-D


Manual Integrations
APPROVED

ugo
3/28/2018 12:00:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:47:58 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

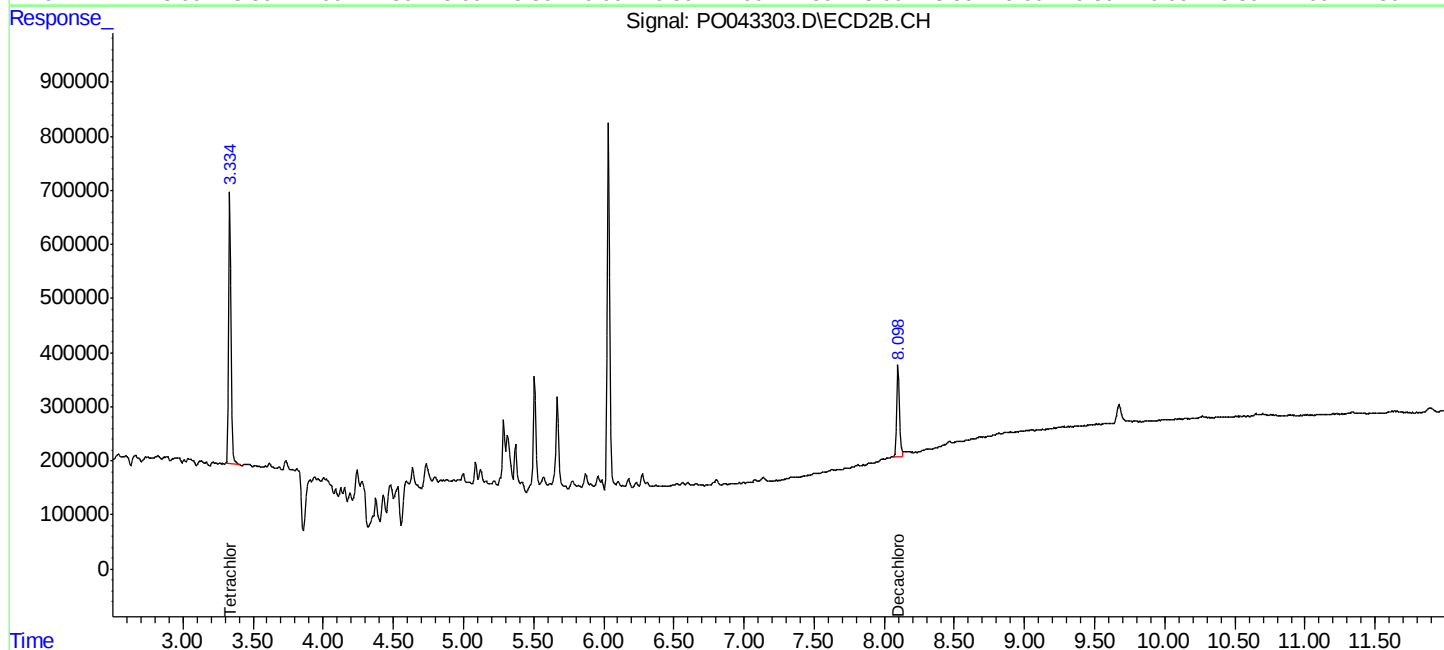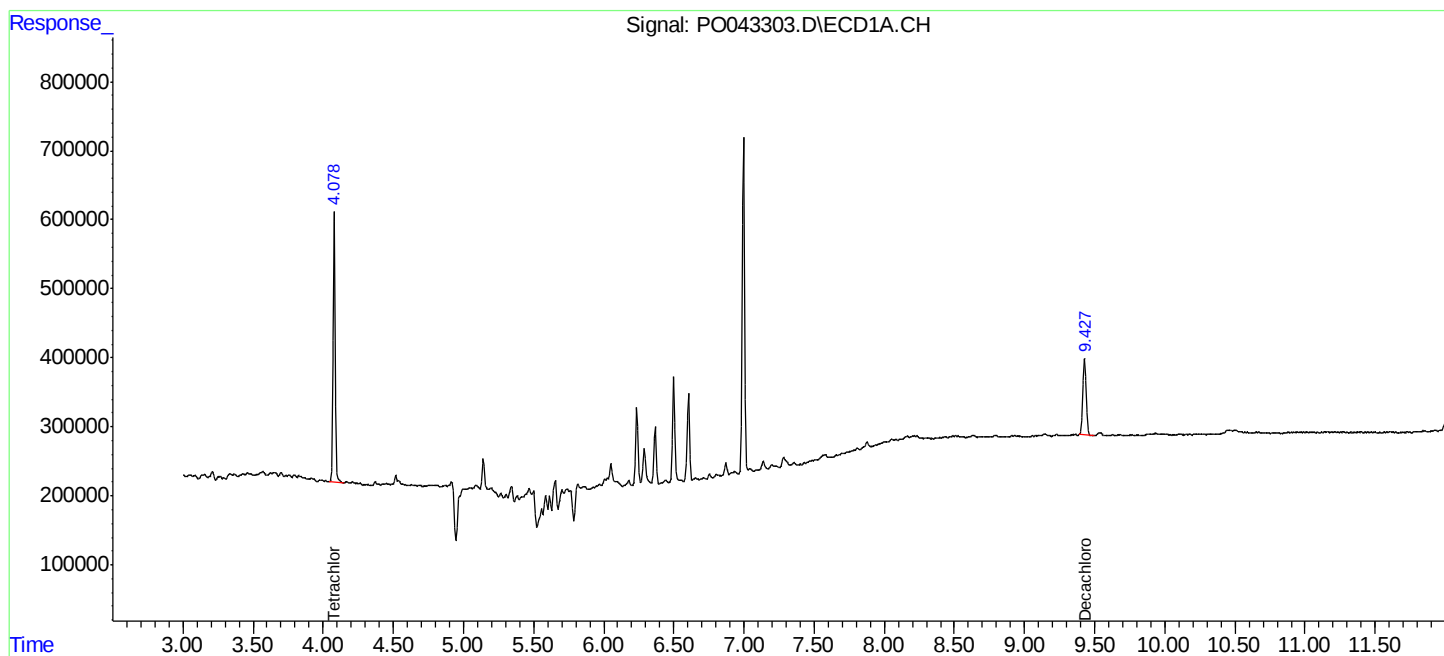

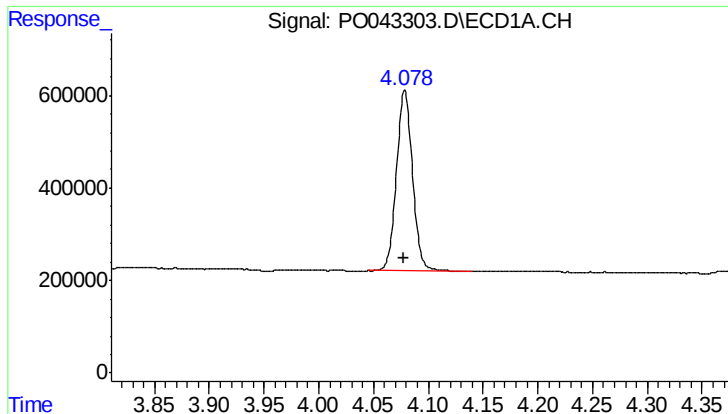


#1 Tetrachloro-m-xylene

R.T.: 4.079 min
Delta R.T.: 0.000 min
Response: 4025443
Conc: 19.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-05-032218-D


Manual Integrations
APPROVED

ugo
3/28/2018 12:00:20 PM

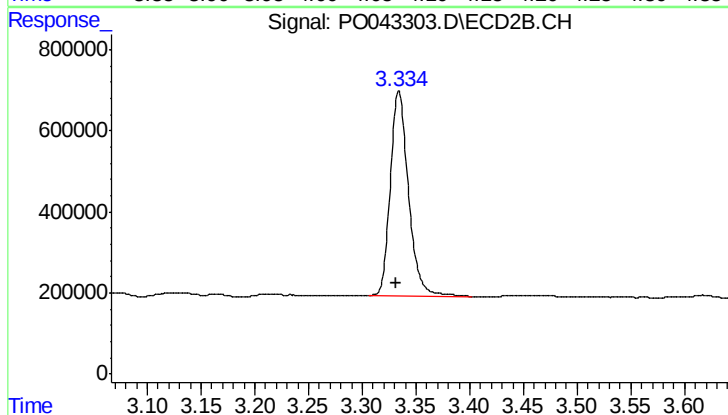


#1 Tetrachloro-m-xylene

R.T.: 3.334 min
Delta R.T.: 0.002 min
Response: 5922462
Conc: 20.23 ng/ml

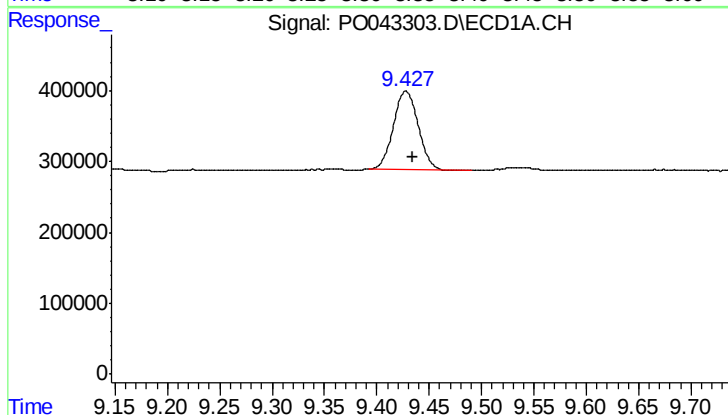

#2 Decachlorobiphenyl

R.T.: 9.428 min
Delta R.T.: -0.007 min
Response: 1822644
Conc: 7.50 ng/ml

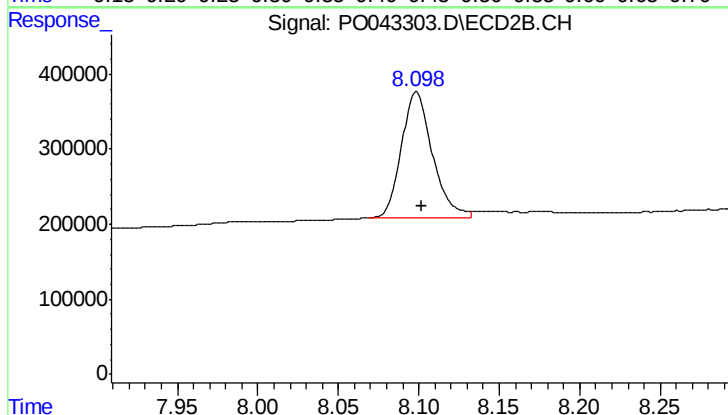

#2 Decachlorobiphenyl

R.T.: 8.098 min
Delta R.T.: -0.004 min
Response: 2285229
Conc: 6.39 ng/ml m