

Data Path : P:\HPCHEM1\ECD 0\Data\P0032618\
 Data File : P0043308.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2018 13:39
 Operator : SM/UA
 Sample : J1748-13RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-05-032218-DRE

Manual Integrations
 APPROVED

ugo
 3/28/2018 12:00:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:58:55 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 23 05:22:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.078	3.334	4154122	6024552	19.605	20.583
2) SA Decachlor...	9.428	8.098	1999875	2121373	8.234m	5.932 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032618\
Data File : P0043308.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2018 13:39
Operator : SM/UA
Sample : J1748-13RE
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-05-032218-DRE


Manual Integrations
APPROVED

ugo
3/28/2018 12:00:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:58:55 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

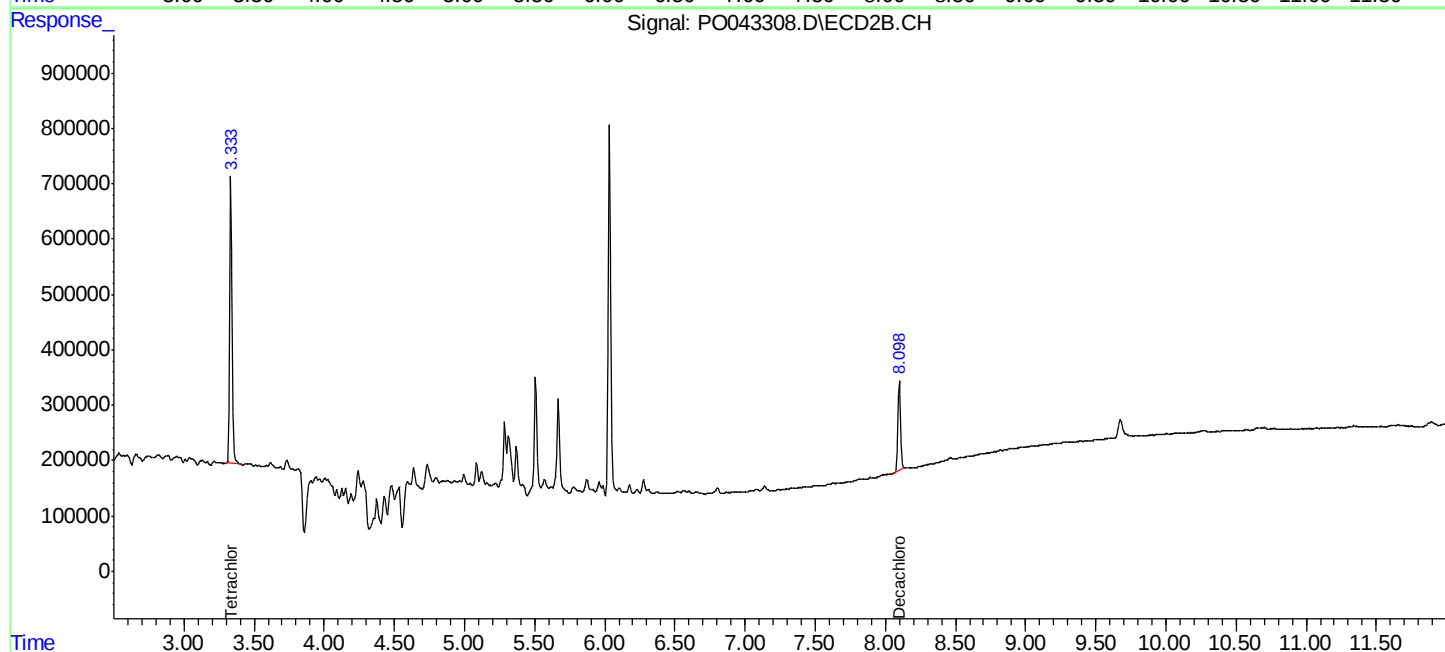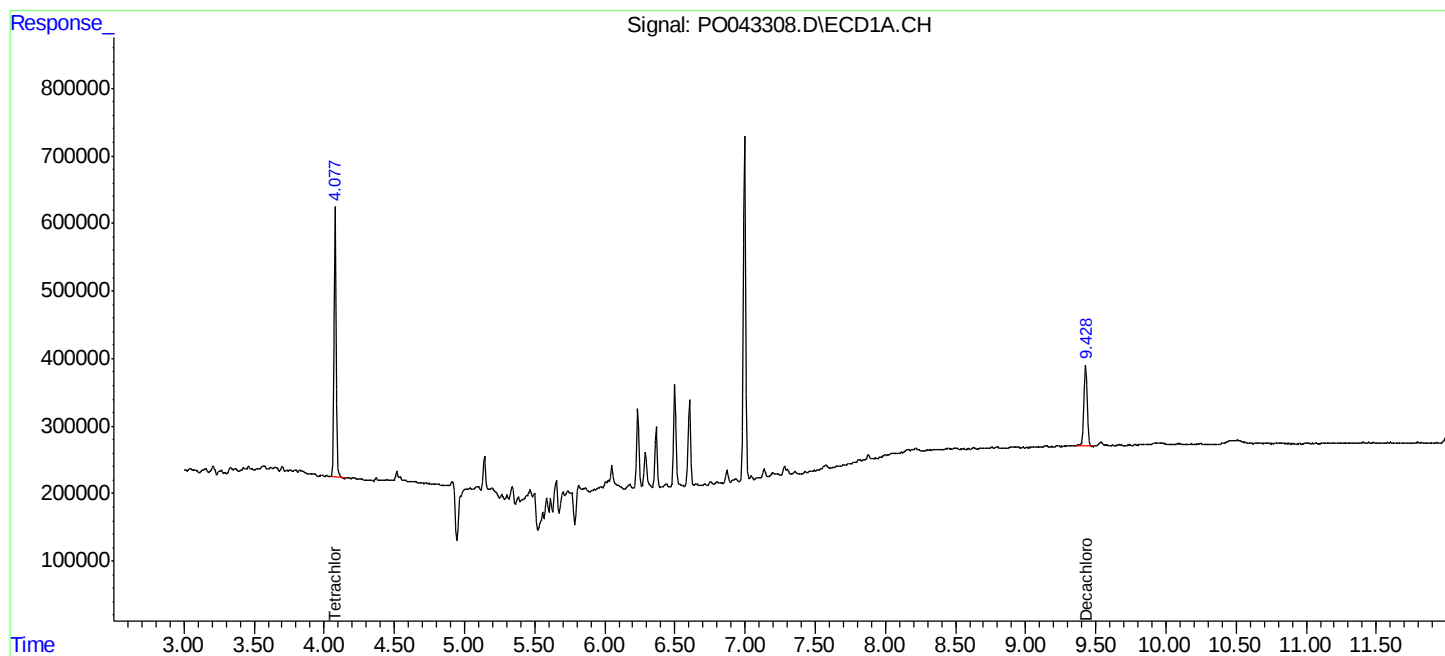

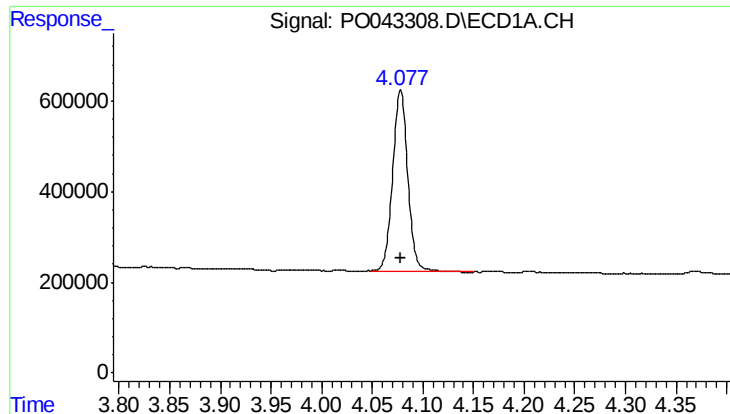


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 4154122
Conc: 19.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-05-032218-DRE


Manual Integrations
APPROVED

ugo
3/28/2018 12:00:40 PM

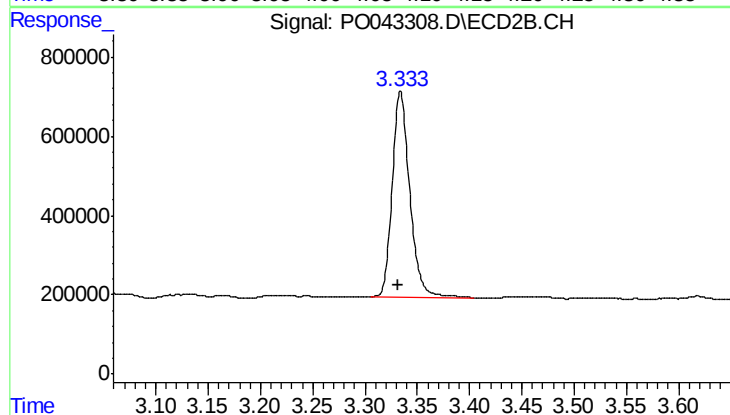


#1 Tetrachloro-m-xylene

R.T.: 3.334 min
Delta R.T.: 0.002 min
Response: 6024552
Conc: 20.58 ng/ml

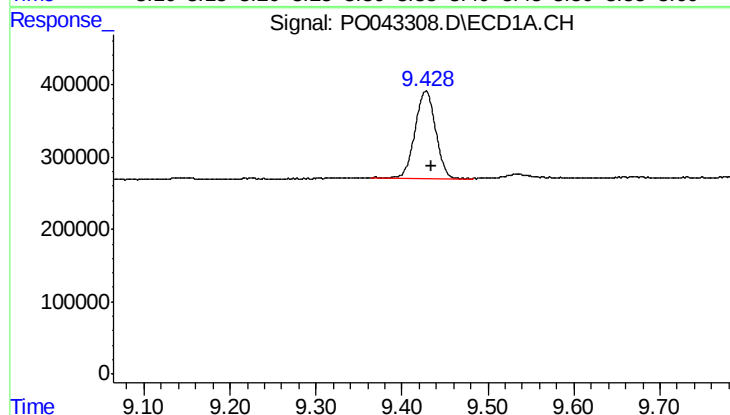

#2 Decachlorobiphenyl

R.T.: 9.428 min
Delta R.T.: -0.007 min
Response: 1999875
Conc: 8.23 ng/ml m

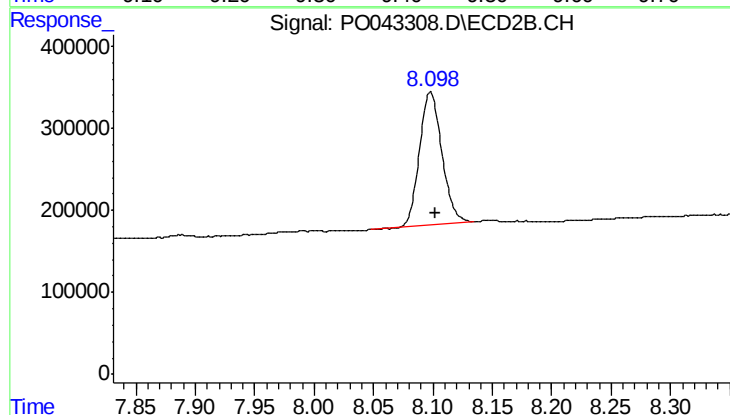

#2 Decachlorobiphenyl

R.T.: 8.098 min
Delta R.T.: -0.004 min
Response: 2121373
Conc: 5.93 ng/ml