

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032620\
 Data File : P0067458.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2020 17:53
 Operator : DD\AJ
 Sample : L2040-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 04:17:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.940	3.948	521626	753580	24.543	21.556
2)	SA Decachlor...	10.925	9.243	657366	787998	22.878	20.202
Target Compounds							
6)	L1 AR-1016-4	0.000	5.530	0	95586	N.D.	102.773 #
14)	L3 AR-1232-4	0.000	5.530	0	95586	N.D.	267.606 #
19)	L4 AR-1242-4	0.000	5.530	0	95586	N.D.	113.047 #
22)	L5 AR-1248-2	0.000	5.530	0	95586	N.D.	92.644 #
23)	L5 AR-1248-3	0.000	5.530	0	95586	N.D.	90.819 #
27)	L6 AR-1254-2	0.000	6.288	0	143734	N.D.	83.389 #
40)	L8 AR-1262-5	0.000	8.693	0	180973	N.D.	106.528 #
44)	L9 AR-1268-4	0.000	8.693	0	180973	N.D.	96.770 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032620\
Data File : P0067458.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2020 17:53
Operator : DD\AJ
Sample : L2040-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 04:17:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

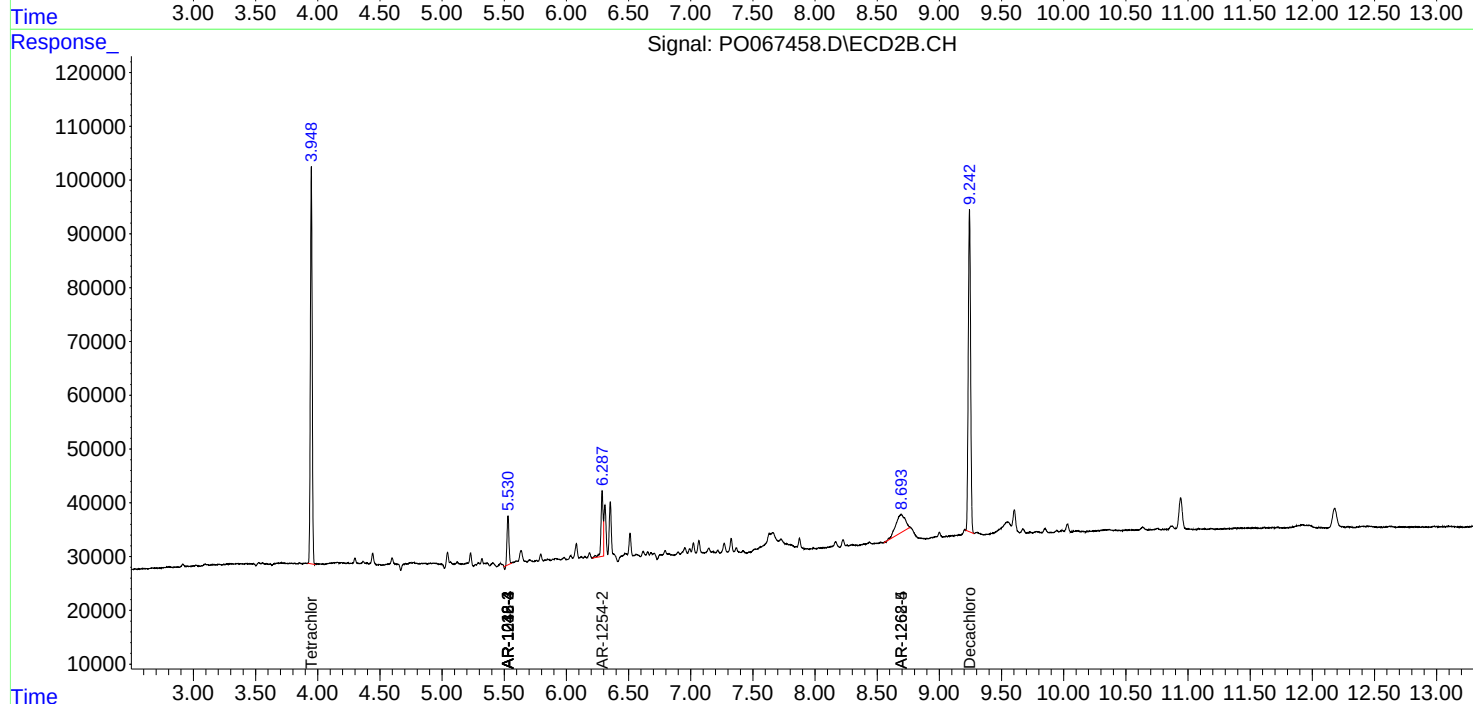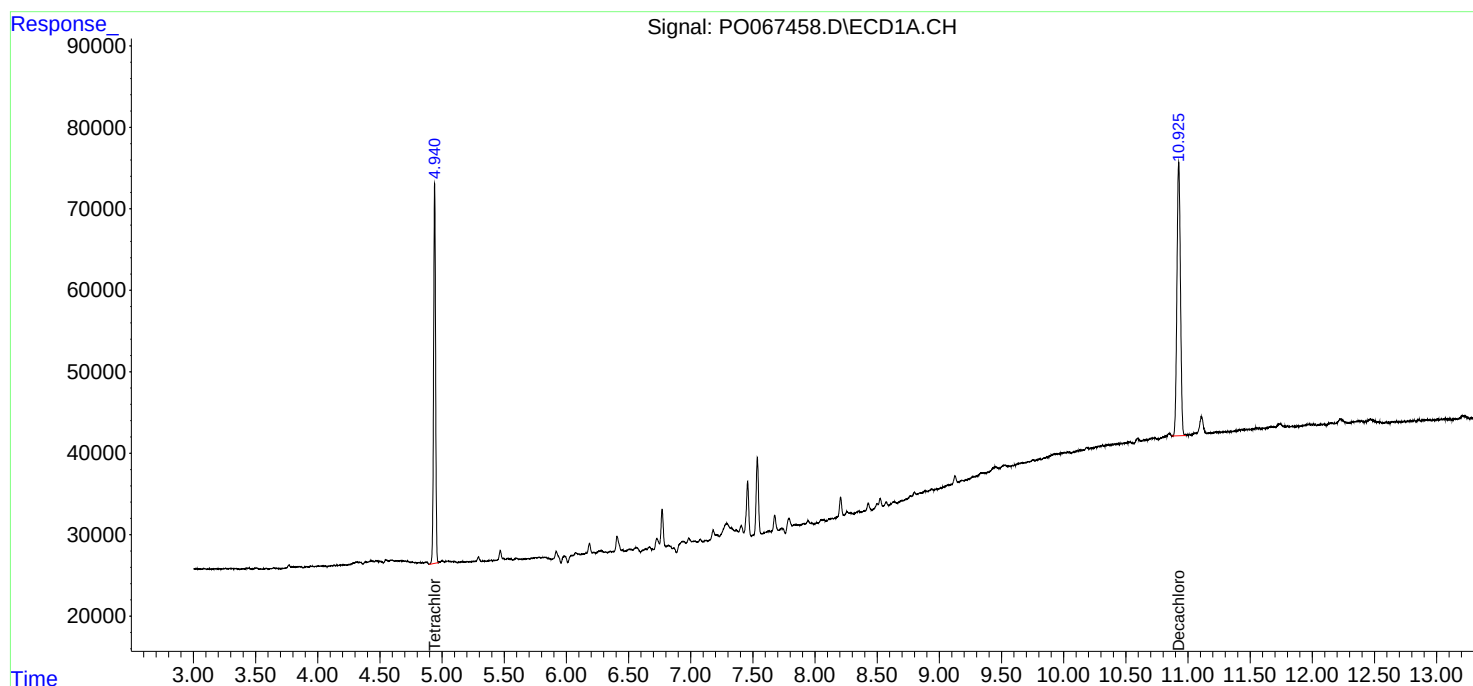


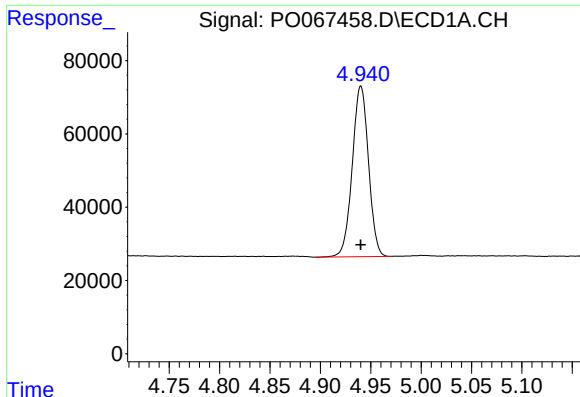

#1 Tetrachloro-m-xylene


R.T.: 4.940 min
Delta R.T.: 0.000 min
Response: 521626
Conc: 24.54 ng/ml

Instrument :
ECD_O
ClientSampleId :

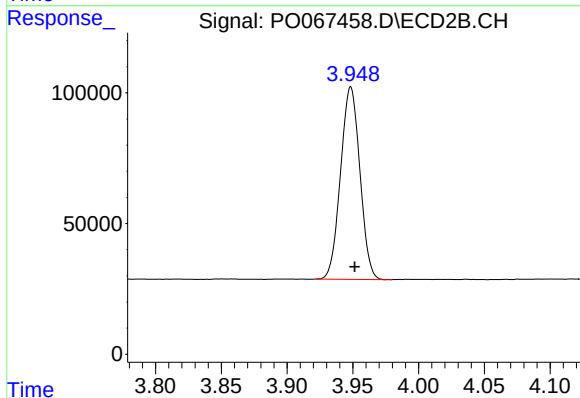


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.003 min
Response: 753580
Conc: 21.56 ng/ml

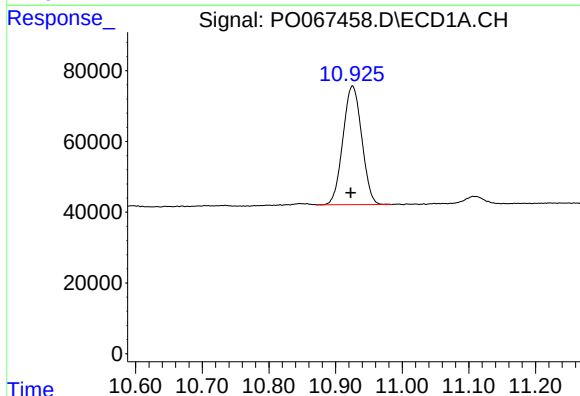


#2 Decachlorobiphenyl

R.T.: 10.925 min
Delta R.T.: 0.003 min
Response: 657366
Conc: 22.88 ng/ml

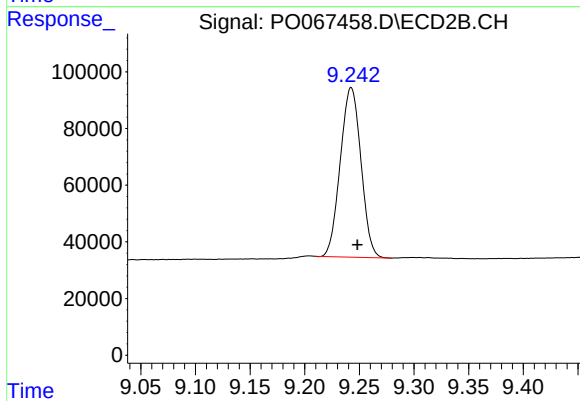

#2 Decachlorobiphenyl


R.T.: 9.243 min
Delta R.T.: -0.006 min
Response: 787998
Conc: 20.20 ng/ml

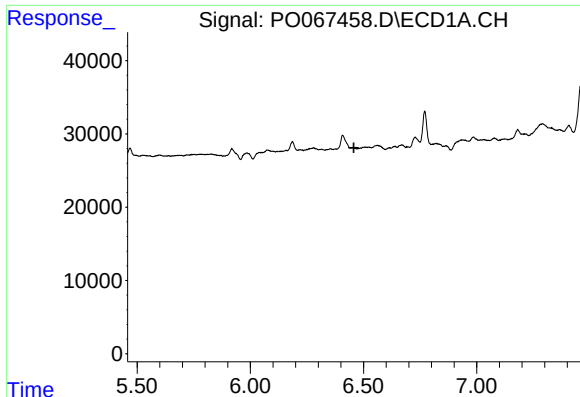

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

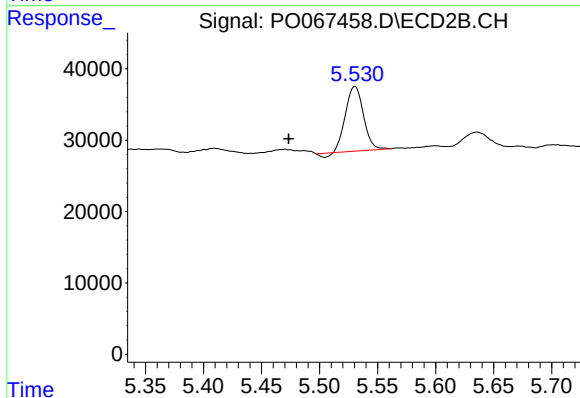


#6 AR-1016-4

R.T.: 5.530 min
Delta R.T.: 0.057 min
Response: 95586
Conc: 102.77 ng/ml

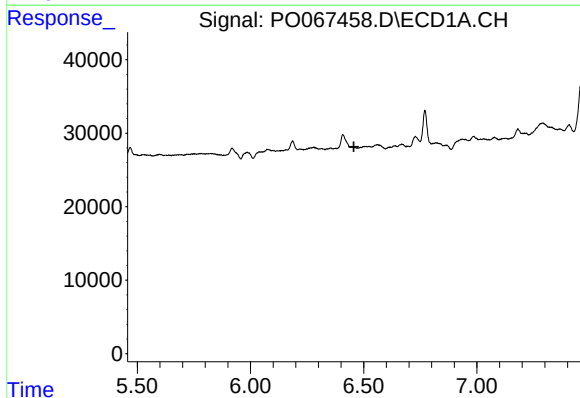


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

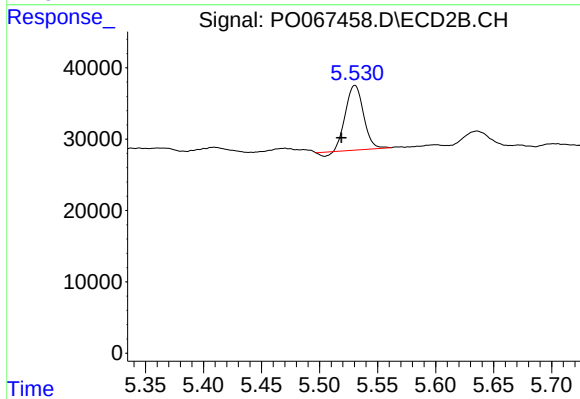

#14 AR-1232-4


R.T.: 5.530 min
Delta R.T.: 0.012 min
Response: 95586
Conc: 267.61 ng/ml

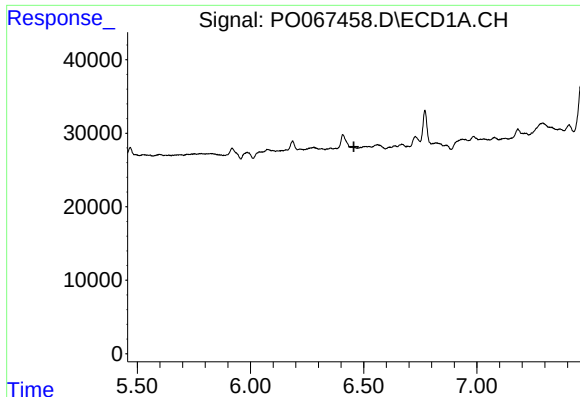

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

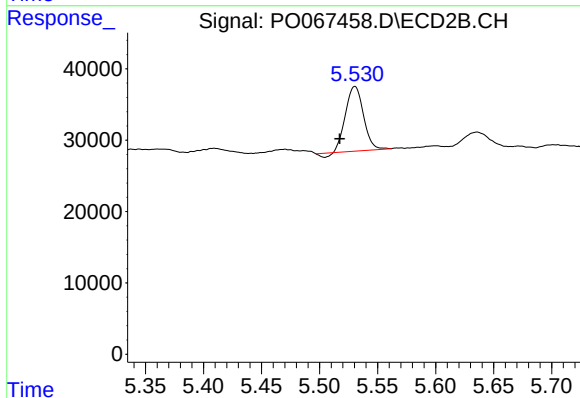


#19 AR-1242-4

R.T.: 5.530 min
Delta R.T.: 0.013 min
Response: 95586
Conc: 113.05 ng/ml

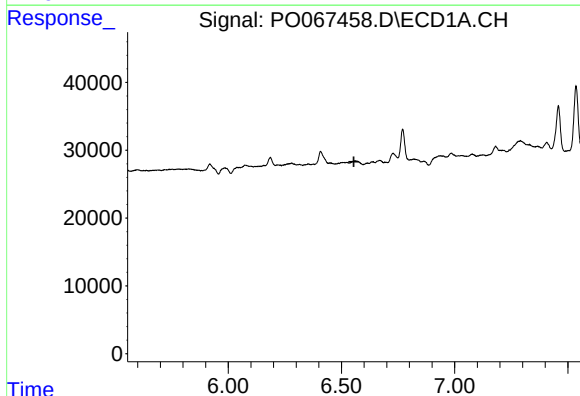


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 6.555 min
Response: 0
Conc: N.D.

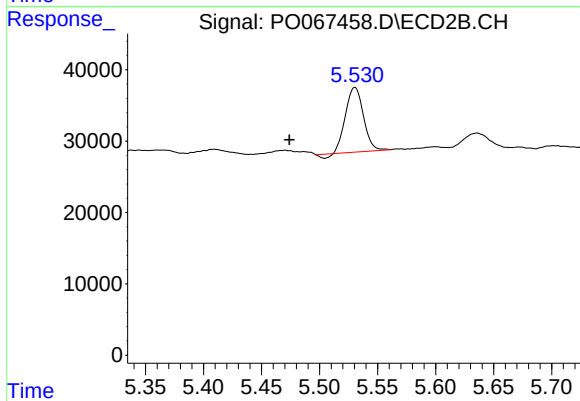

#22 AR-1248-2


R.T.: 5.530 min
Delta R.T.: 0.057 min
Response: 95586
Conc: 92.64 ng/ml

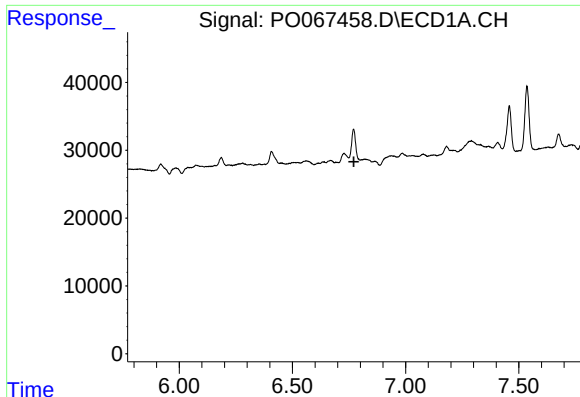

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.772 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

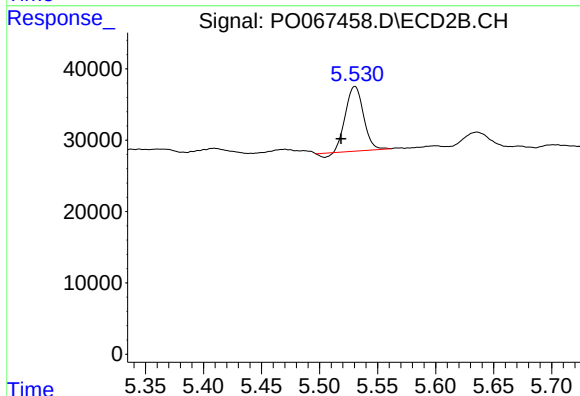


#23 AR-1248-3

R.T.: 5.530 min
Delta R.T.: 0.012 min
Response: 95586
Conc: 90.82 ng/ml

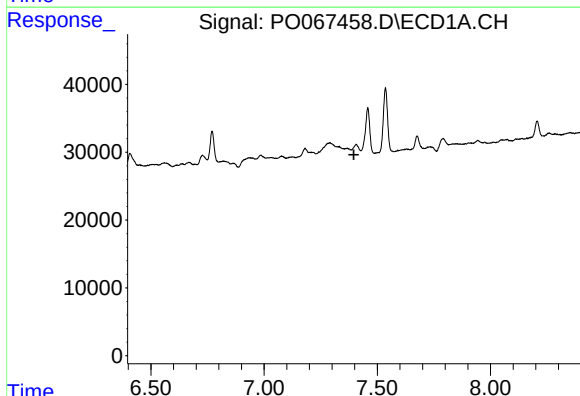


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 7.396 min
Response: 0
Conc: N.D.

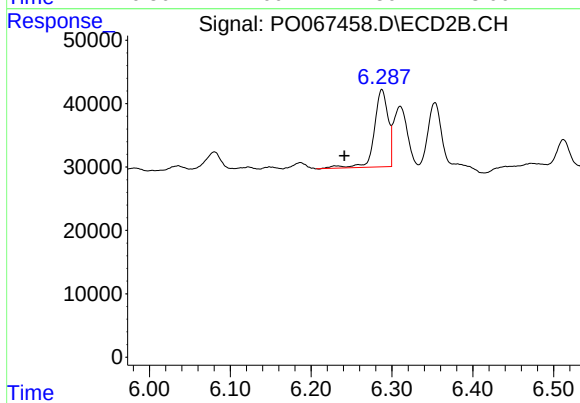

#27 AR-1254-2


R.T.: 6.288 min
Delta R.T.: 0.047 min
Response: 143734
Conc: 83.39 ng/ml

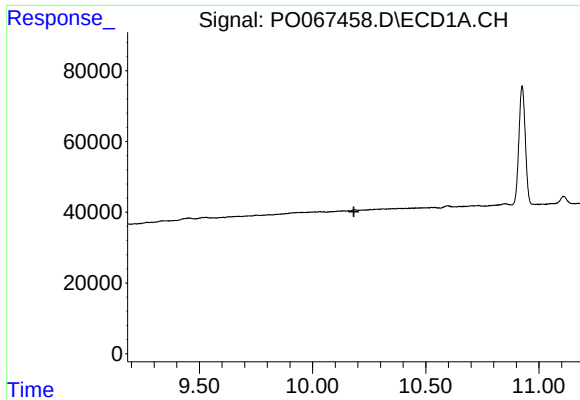

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 10.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

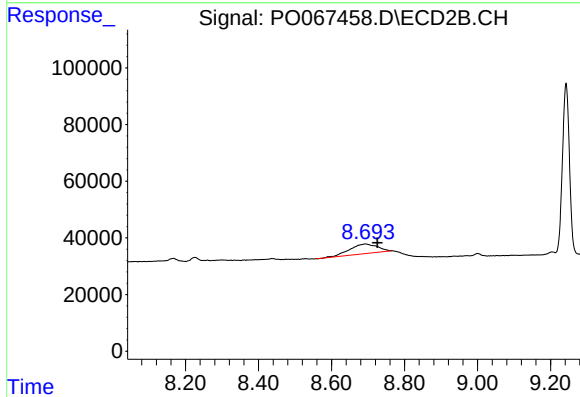


#40 AR-1262-5

R.T.: 8.693 min
Delta R.T.: -0.033 min
Response: 180973
Conc: 106.53 ng/ml

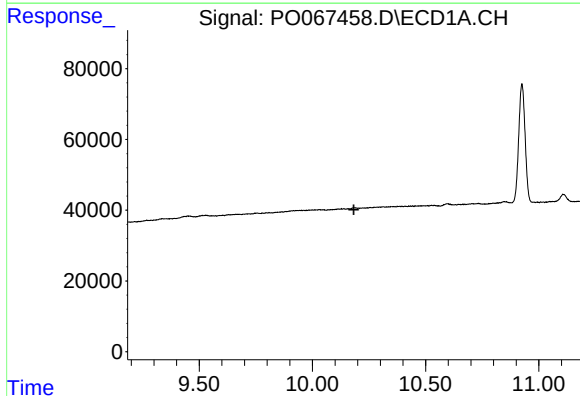

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 10.183 min
Response: 0
Conc: N.D.

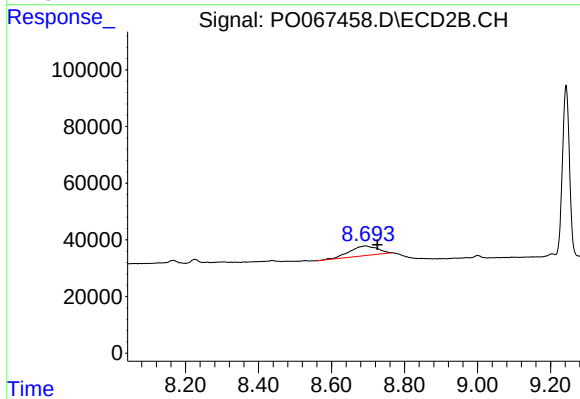

#44 AR-1268-4

R.T.: 8.693 min
Delta R.T.: -0.033 min
Response: 180973
Conc: 96.77 ng/ml