

Data Path : P:\HPCHEM1\ECD 0\Data\P0032718\
 Data File : P0043314.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2018 9:15
 Operator : SM/UA
 Sample : J2070-01 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 A461238

Manual Integrations
 APPROVED

ugo
 3/29/2018 5:47:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 11:53:03 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 23 05:22:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.078	3.330	275822	169003	1.302	0.577 #
2) SA Decachlor...	9.429	8.098	422173	327093	1.738m	0.915m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032718\
Data File : P0043314.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2018 9:15
Operator : SM/UA
Sample : J2070-01 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
A461238


Manual Integrations
APPROVED

ugo
3/29/2018 5:47:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 11:53:03 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

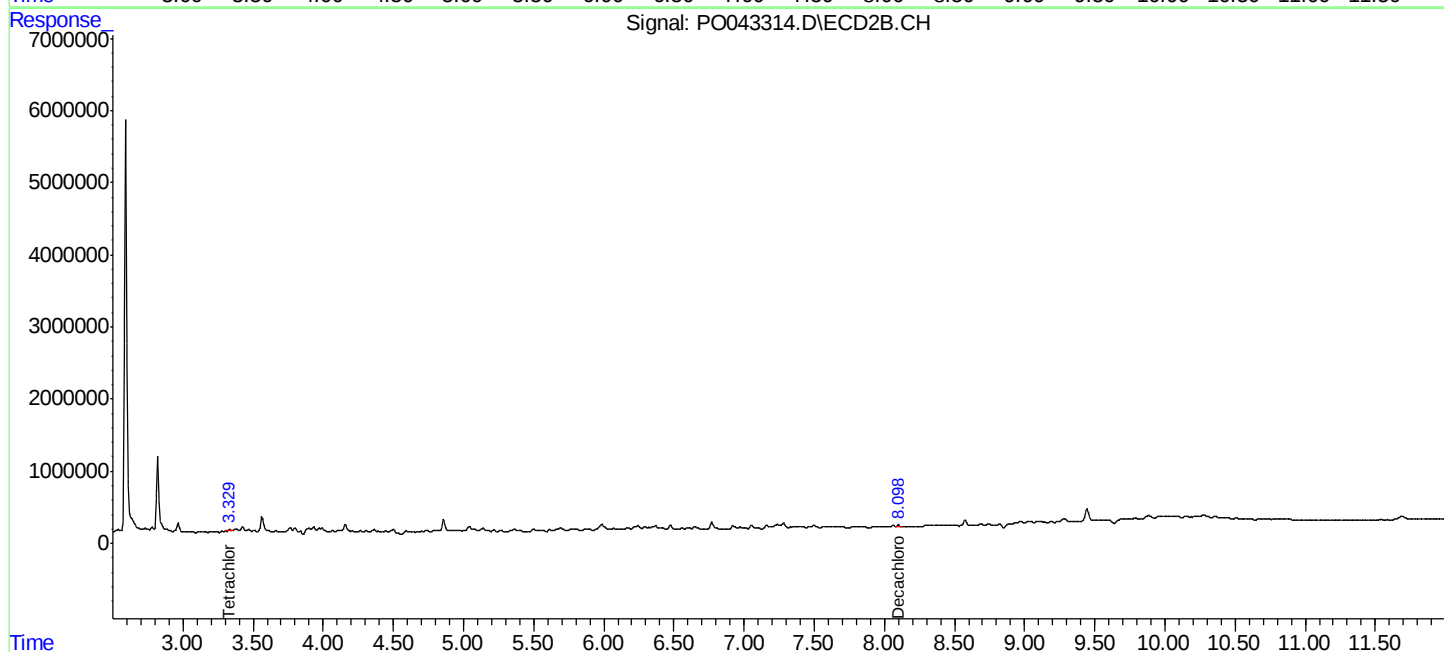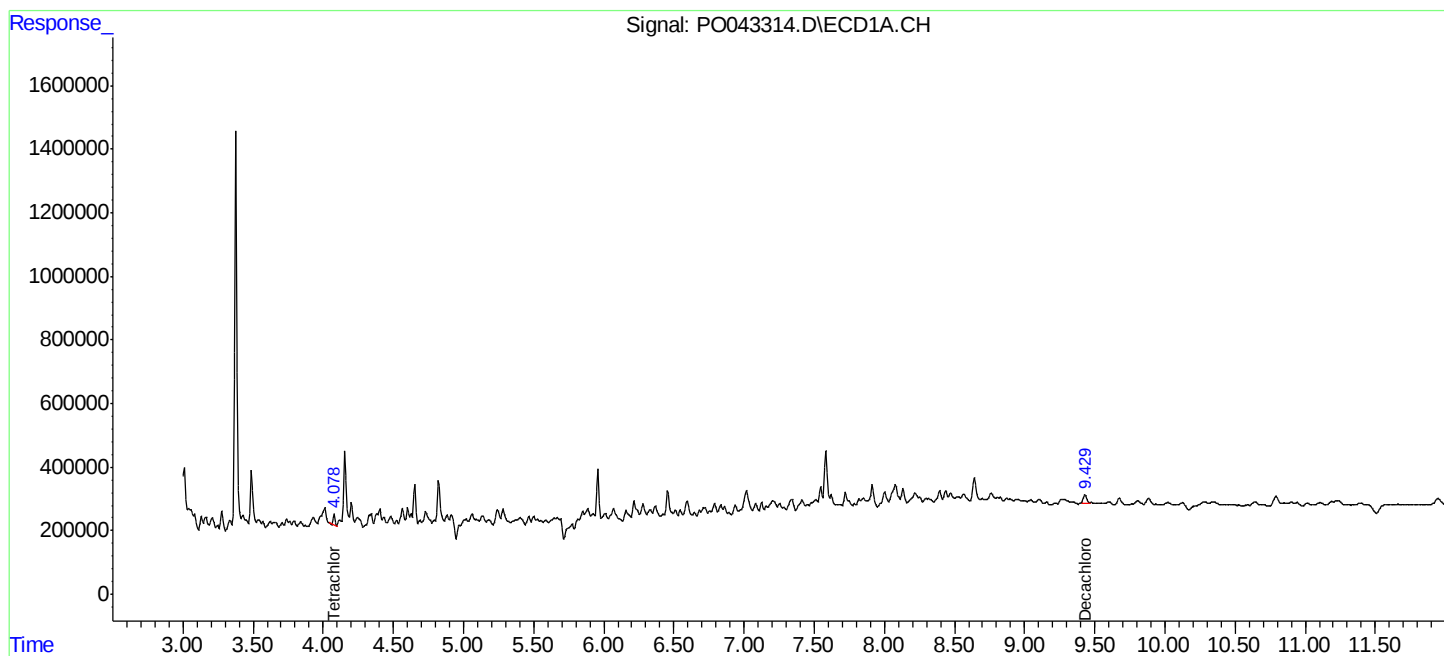

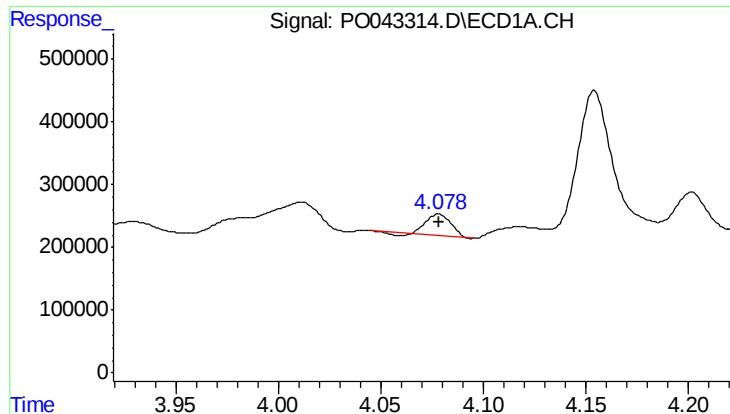


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 275822
Conc: 1.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
A461238


Manual Integrations
APPROVED

ugo
3/29/2018 5:47:55 PM

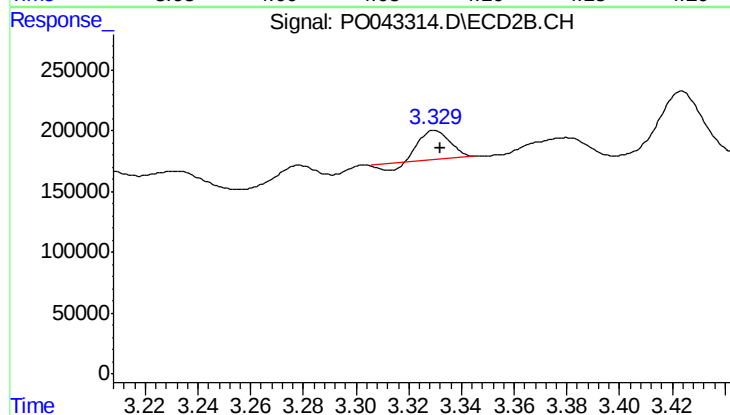


#1 Tetrachloro-m-xylene

R.T.: 3.330 min
Delta R.T.: -0.002 min
Response: 169003
Conc: 0.58 ng/ml

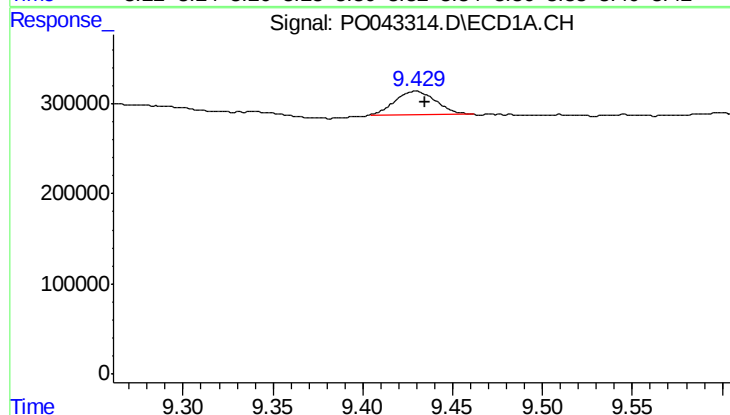

#2 Decachlorobiphenyl

R.T.: 9.429 min
Delta R.T.: -0.006 min
Response: 422173
Conc: 1.74 ng/ml m

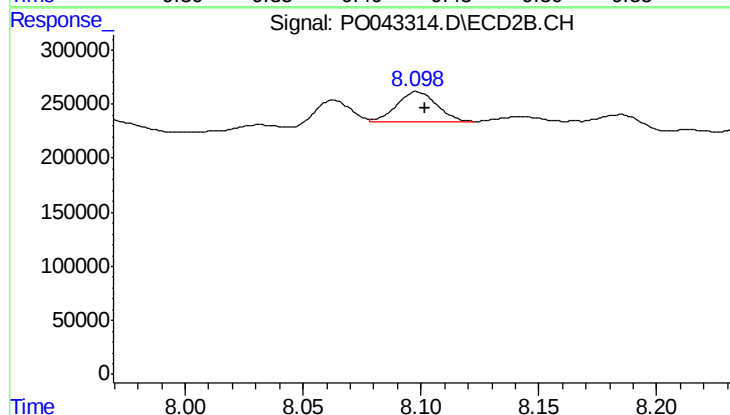

#2 Decachlorobiphenyl

R.T.: 8.098 min
Delta R.T.: -0.004 min
Response: 327093
Conc: 0.91 ng/ml m