

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032719\
 Data File : P0054678.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 20:09
 Operator : SM/SJ
 Sample : K2103-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SHORE-RD-CLVRT-STLD-3H-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 00:55:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.303	3.619	501361	452425	14.446	14.177
2)	SA Decachlor...	9.919	8.598	673200	490130	13.656	15.390
Target Compounds							
5)	L1 AR-1016-3	0.000	4.915	0	16278	N.D.	13.473 #
6)	L1 AR-1016-4	0.000	4.915	0	16278	N.D.	16.109 #
7)	L1 AR-1016-5	0.000	5.210	0	8490	N.D.	6.513 #
13)	L3 AR-1232-3	0.000	4.915	0	16278	N.D.	33.594 #
14)	L3 AR-1232-4	0.000	4.915	0	16278	N.D.	37.047 #
15)	L3 AR-1232-5	0.000	5.210	0	8490	N.D.	17.455 #
18)	L4 AR-1242-3	0.000	4.915	0	16278	N.D.	17.183 #
19)	L4 AR-1242-4	0.000	4.915	0	16278	N.D.	17.032 #
22)	L5 AR-1248-2	0.000	4.915	0	16278	N.D.	13.469 #
23)	L5 AR-1248-3	0.000	4.915	0	16278	N.D.	13.046 #
24)	L5 AR-1248-4	0.000	5.210	0	8490	N.D.	5.574 #
31)	L7 AR-1260-1	0.000	6.179	0	764	N.D.	0.333 #
33)	L7 AR-1260-3	0.000	6.568	0	153	N.D.	0.059 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032719\
Data File : P0054678.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 20:09
Operator : SM/SJ
Sample : K2103-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-3H-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 00:55:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

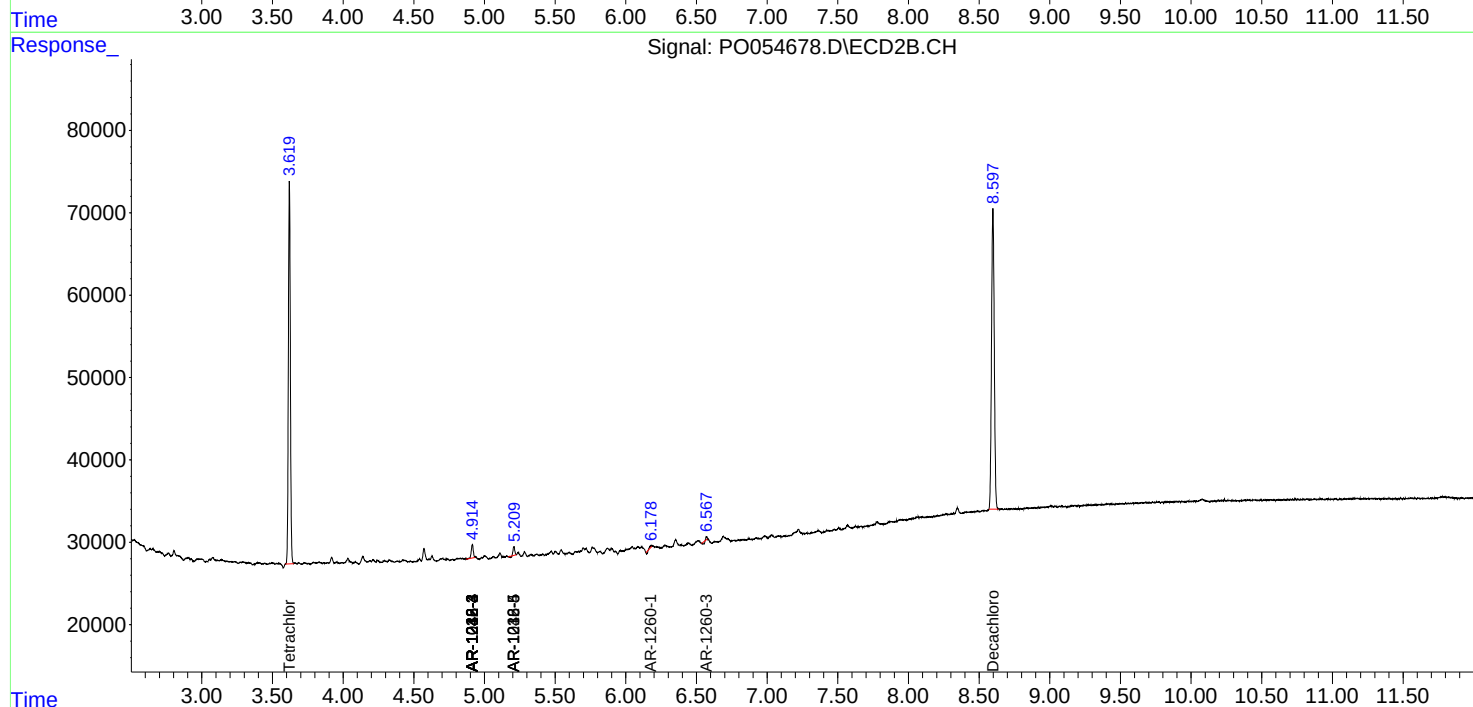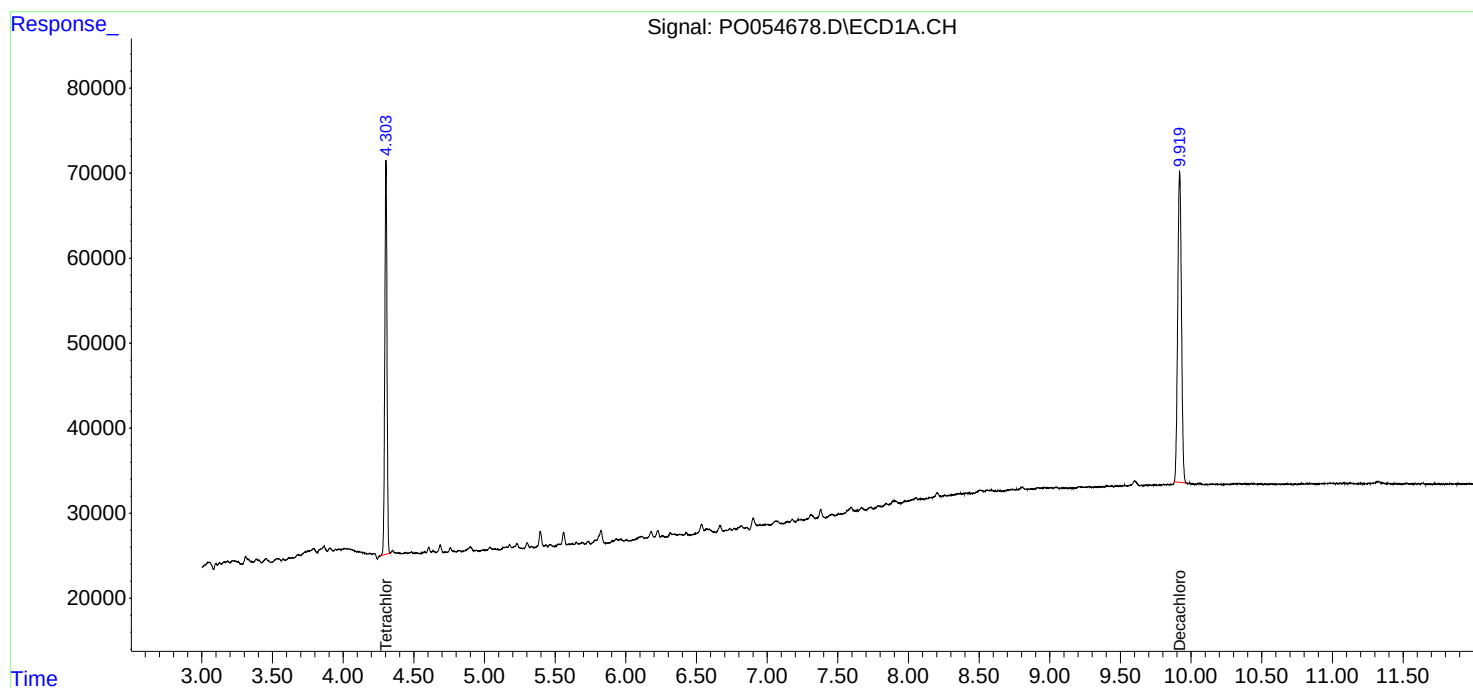


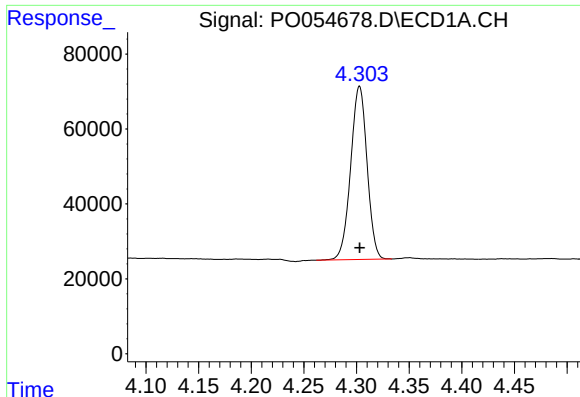

#1 Tetrachloro-m-xylene


R.T.: 4.303 min
Delta R.T.: 0.000 min
Response: 501361
Conc: 14.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-3H-A

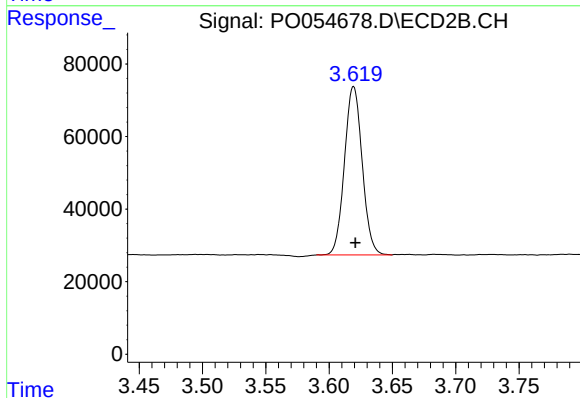


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.001 min
Response: 452425
Conc: 14.18 ng/ml

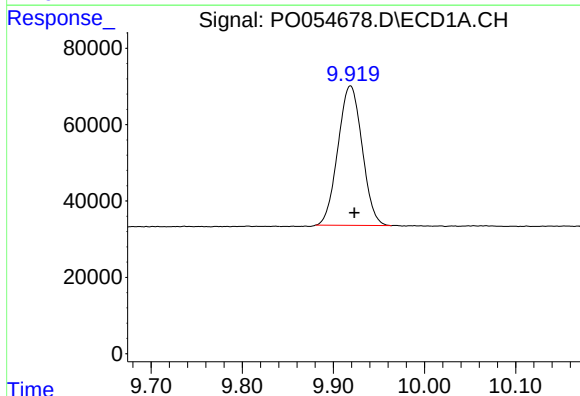


#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.004 min
Response: 673200
Conc: 13.66 ng/ml

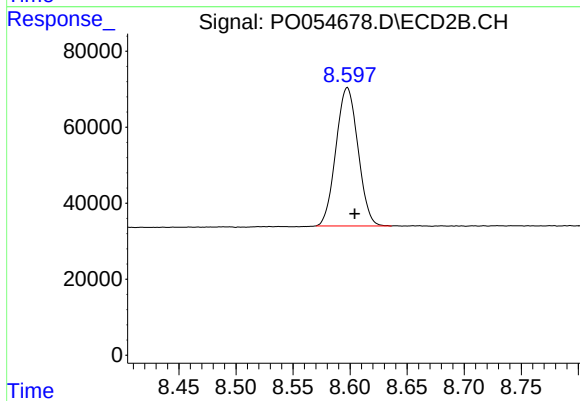

#2 Decachlorobiphenyl


R.T.: 8.598 min
Delta R.T.: -0.006 min
Response: 490130
Conc: 15.39 ng/ml

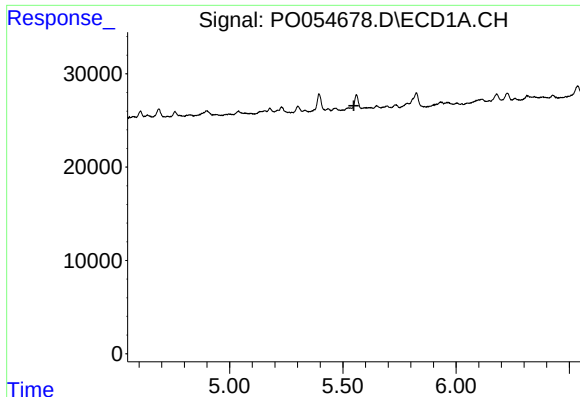

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-3H-A

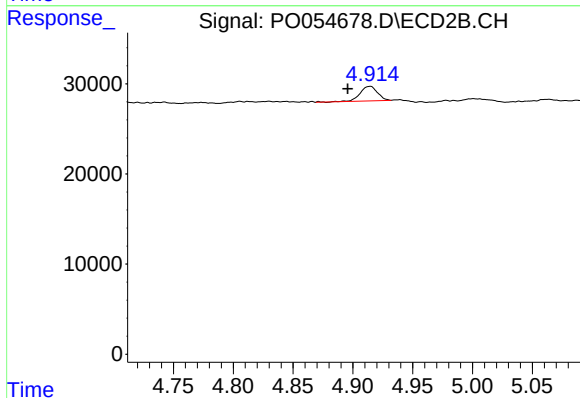


#5 AR-1016-3

R.T.: 4.915 min
Delta R.T.: 0.019 min
Response: 16278
Conc: 13.47 ng/ml

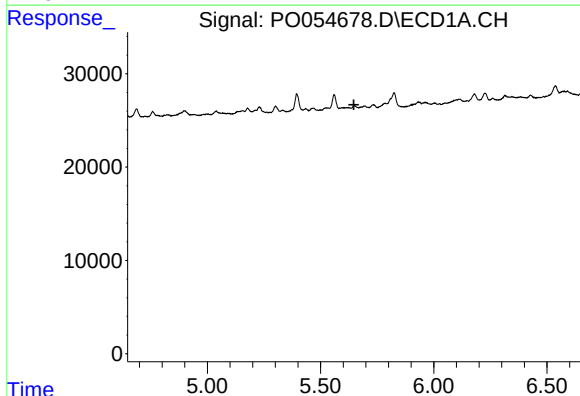


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.647 min
Response: 0
Conc: N.D.

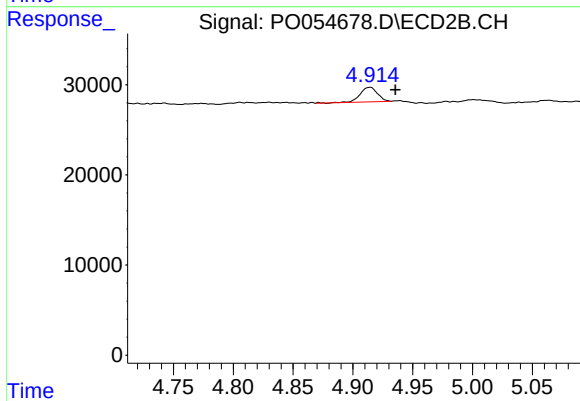

#6 AR-1016-4


R.T.: 4.915 min
Delta R.T.: -0.021 min
Response: 16278
Conc: 16.11 ng/ml

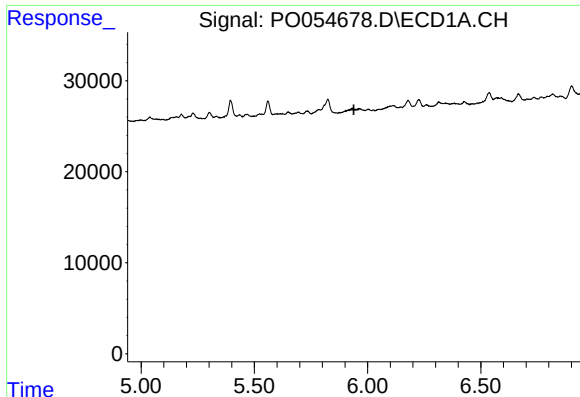

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-3H-A

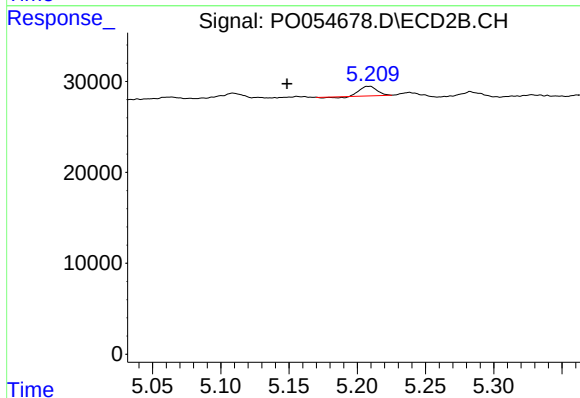


#7 AR-1016-5

R.T.: 5.210 min
Delta R.T.: 0.061 min
Response: 8490
Conc: 6.51 ng/ml

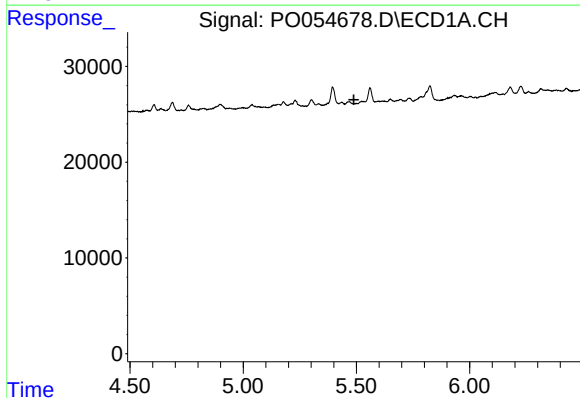


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T.: 5.488 min
Response: 0
Conc: N.D.

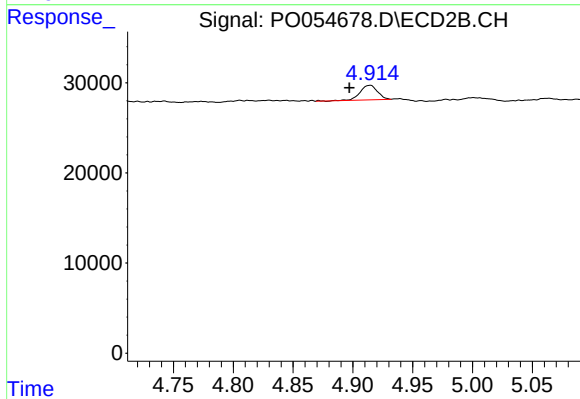

#13 AR-1232-3


R.T.: 4.915 min
Delta R.T.: 0.018 min
Response: 16278
Conc: 33.59 ng/ml

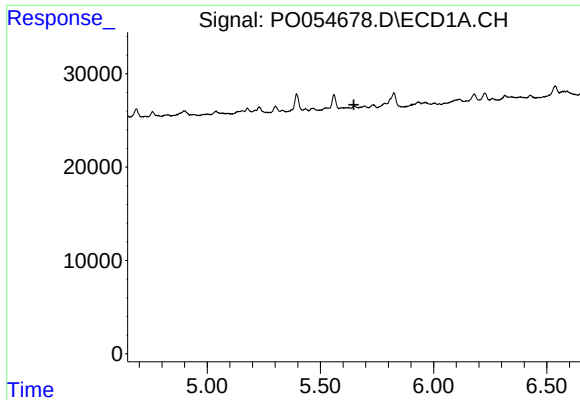

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 5.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-3H-A

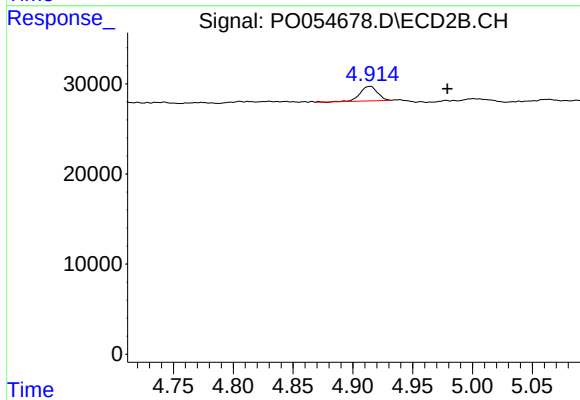


#14 AR-1232-4

R.T.: 4.915 min
Delta R.T.: -0.064 min
Response: 16278
Conc: 37.05 ng/ml

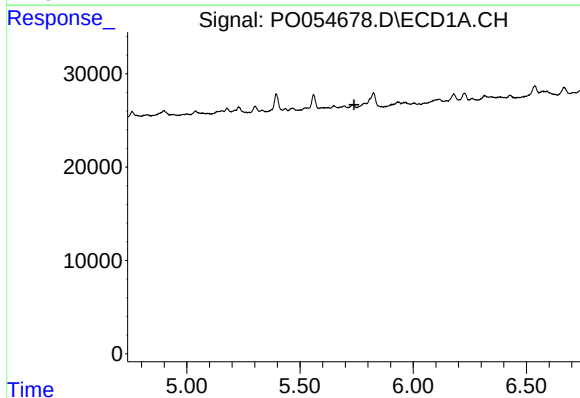


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.738 min
Response: 0
Conc: N.D.

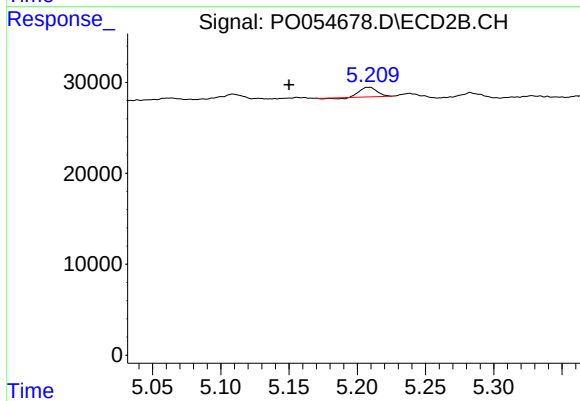

#15 AR-1232-5


R.T.: 5.210 min
Delta R.T.: 0.060 min
Response: 8490
Conc: 17.46 ng/ml

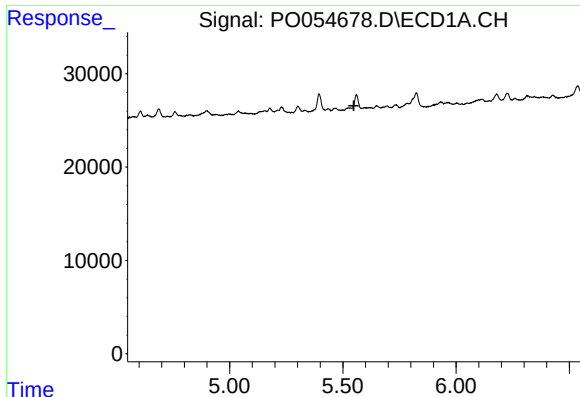

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-3H-A

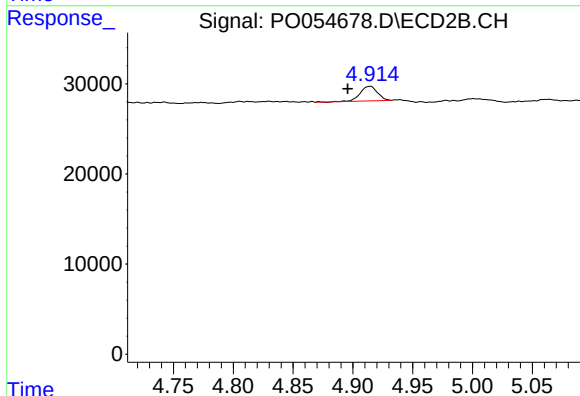


#18 AR-1242-3

R.T.: 4.915 min
Delta R.T.: 0.019 min
Response: 16278
Conc: 17.18 ng/ml

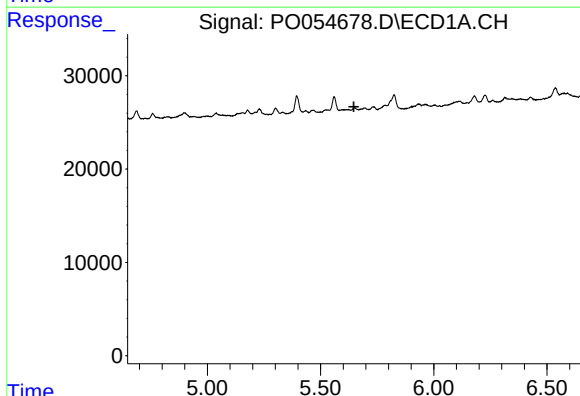


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 5.647 min
Response: 0
Conc: N.D.

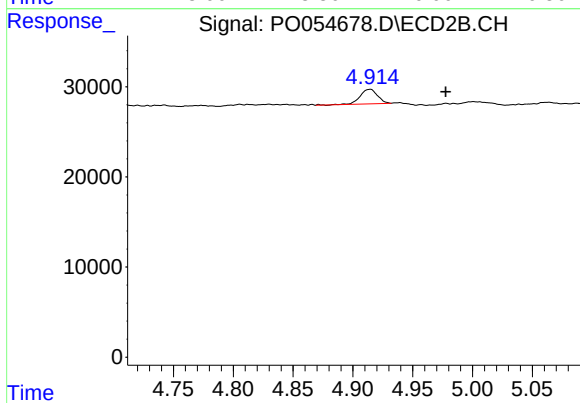

#19 AR-1242-4


R.T.: 4.915 min
Delta R.T.: -0.063 min
Response: 16278
Conc: 17.03 ng/ml

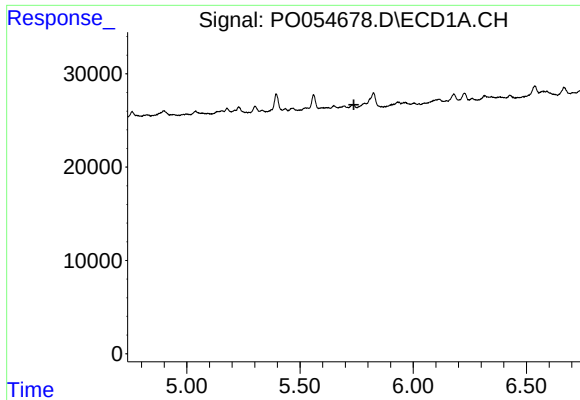

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 5.738 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-3H-A

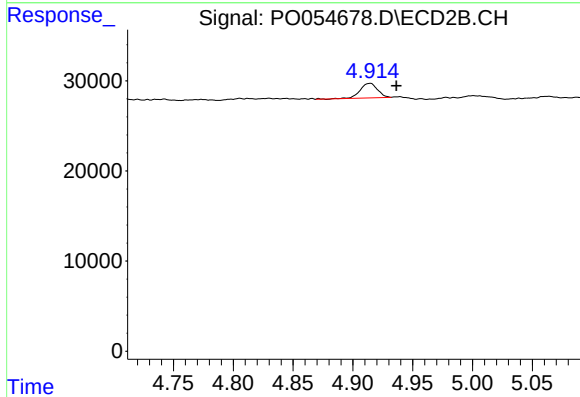


#22 AR-1248-2

R.T.: 4.915 min
Delta R.T.: -0.021 min
Response: 16278
Conc: 13.47 ng/ml

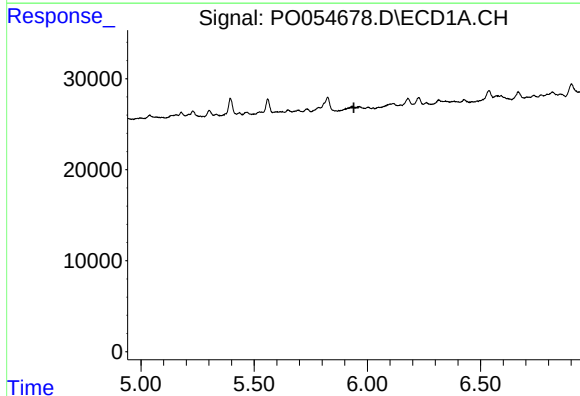


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

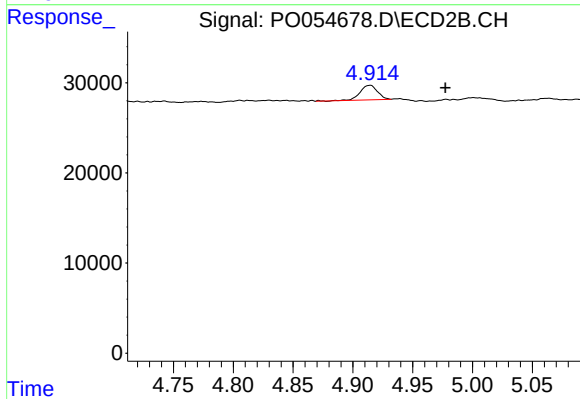

#23 AR-1248-3


R.T.: 4.915 min
Delta R.T.: -0.063 min
Response: 16278
Conc: 13.05 ng/ml

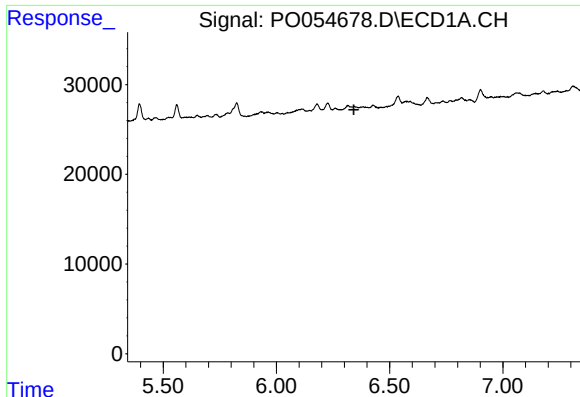

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-3H-A

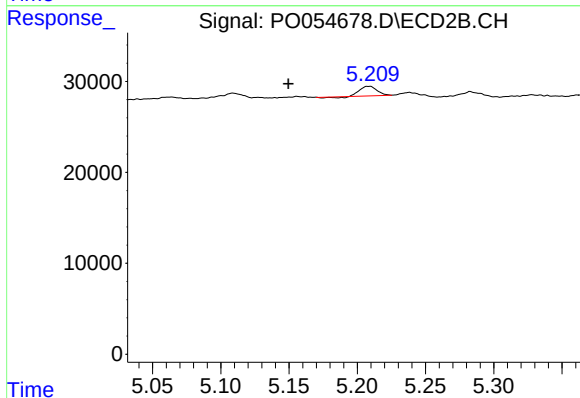


#24 AR-1248-4

R.T.: 5.210 min
Delta R.T.: 0.060 min
Response: 8490
Conc: 5.57 ng/ml

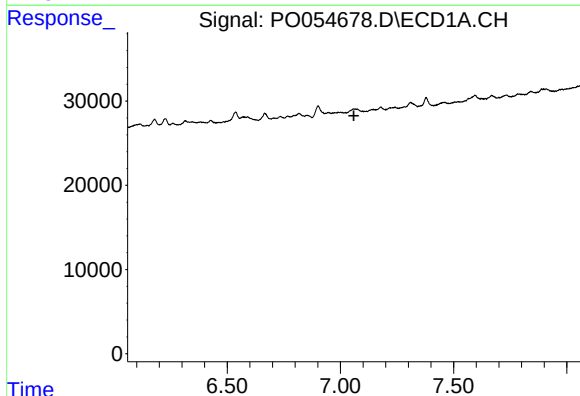


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 7.060 min
Response: 0
Conc: N.D.

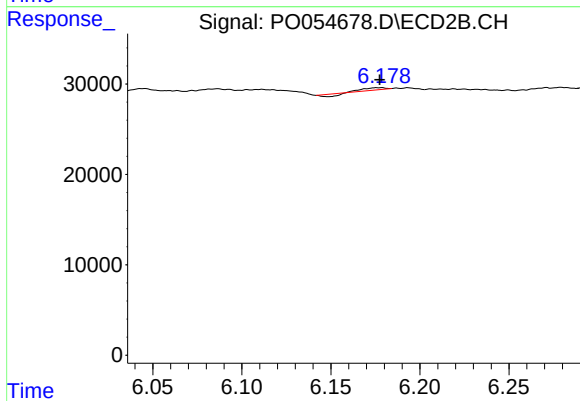

#31 AR-1260-1


R.T.: 6.179 min
Delta R.T.: 0.002 min
Response: 764
Conc: 0.33 ng/ml

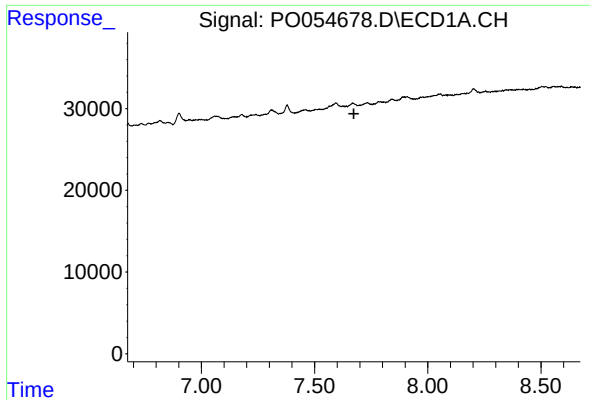

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-3H-A

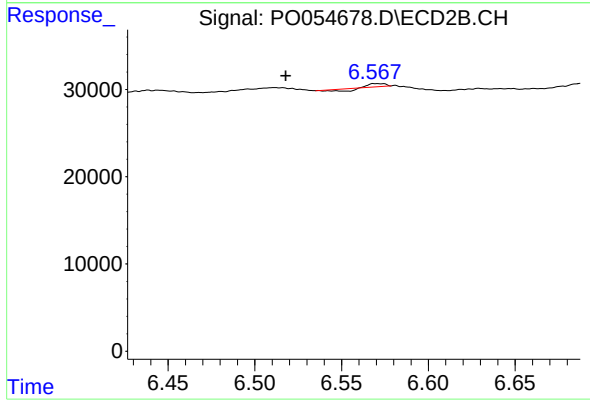

#33 AR-1260-3

R.T.: 6.568 min
Delta R.T.: 0.051 min
Response: 153
Conc: 0.06 ng/ml