

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032719\
 Data File : P0054680.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 20:43
 Operator : SM/SJ
 Sample : K2103-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH-C05-SETTLED-3H-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 00:56:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.303	3.620	517496	476300	14.911	14.925
2) SA Decachlor...	9.918	8.597	643953	462259	13.063	14.514
Target Compounds						
8) L2 AR-1221-1	0.000	3.893	0	22286	N.D.	57.322 #
9) L2 AR-1221-2	4.601	3.919	30837	9918	90.933	33.082 #
10) L2 AR-1221-3	0.000	4.049	0	45063	N.D.	48.887 #
11) L3 AR-1232-1	0.000	4.049	0	45063	N.D.	60.092 #
12) L3 AR-1232-2	5.235	0.000	20205	0	41.308	N.D. #
16) L4 AR-1242-1	5.395	0.000	22059	0	15.878	N.D. #
32) L7 AR-1260-2	0.000	6.348	0	7568	N.D.	2.749 #
33) L7 AR-1260-3	0.000	6.520	0	21900	N.D.	8.495 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032719\
Data File : P0054680.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 20:43
Operator : SM/SJ
Sample : K2103-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MH-C05-SETTLED-3H-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 00:56:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

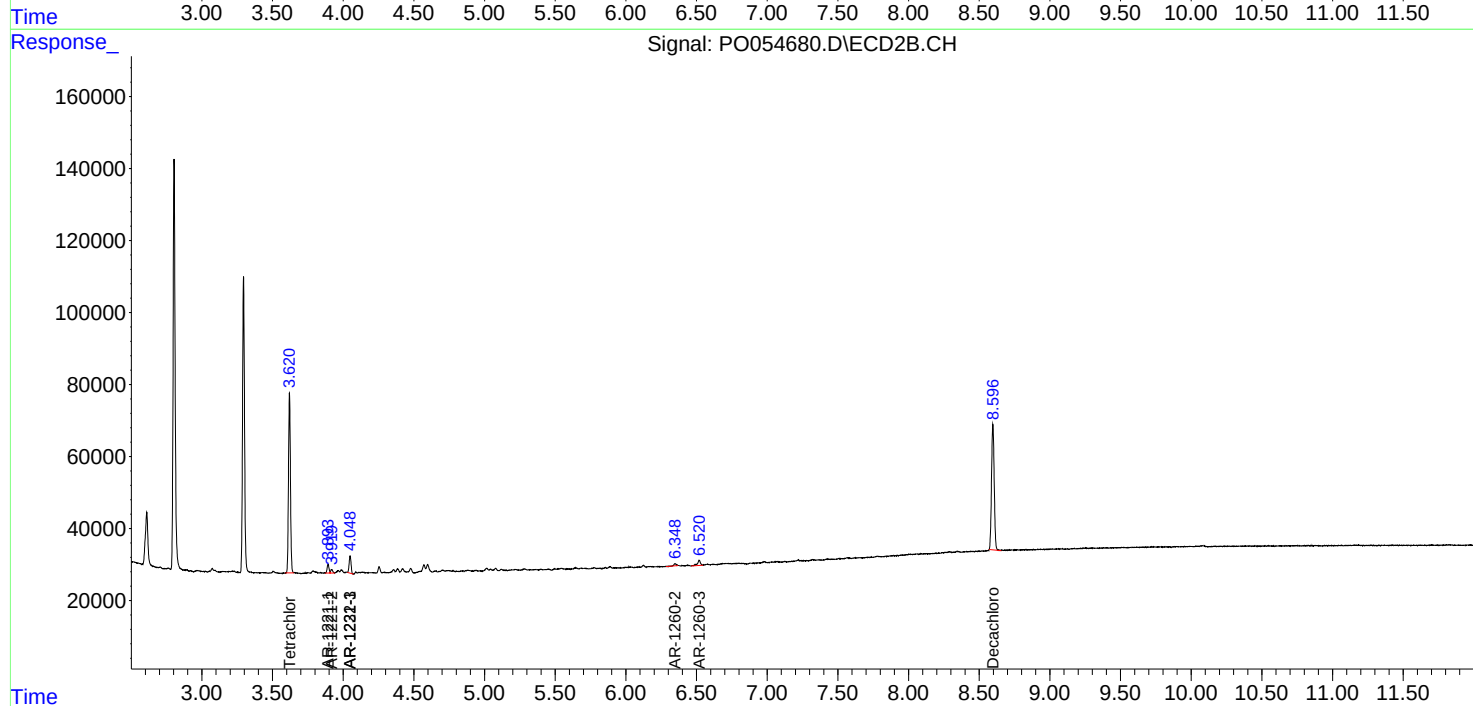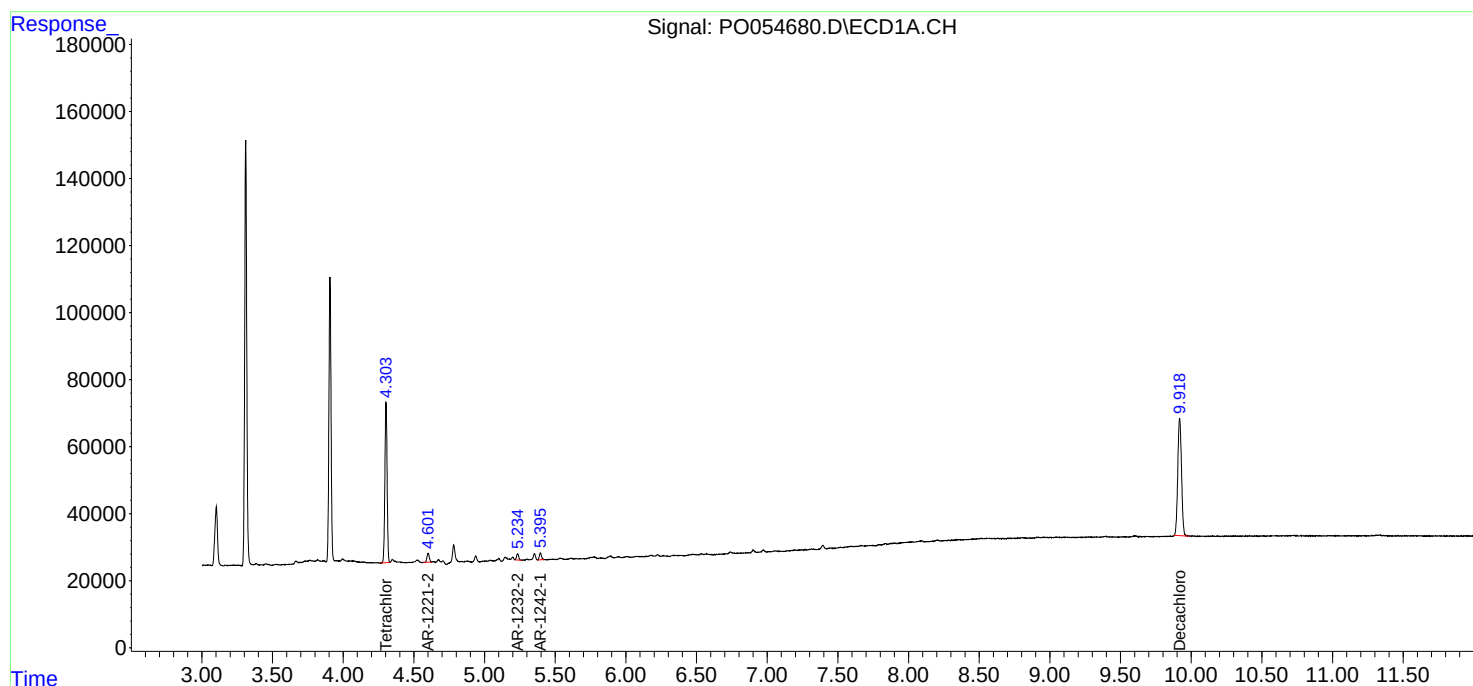


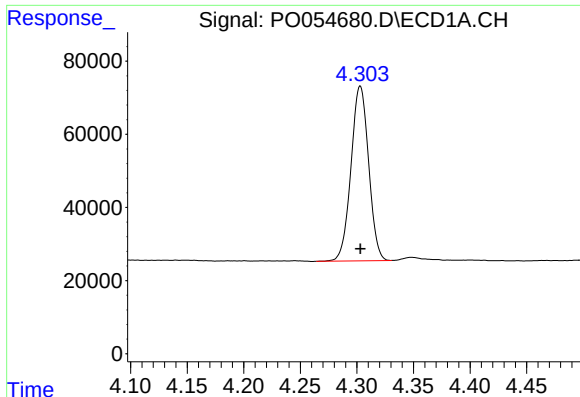

#1 Tetrachloro-m-xylene


R.T.: 4.303 min
Delta R.T.: 0.000 min
Response: 517496
Conc: 14.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-C05-SETTLED-3H-A

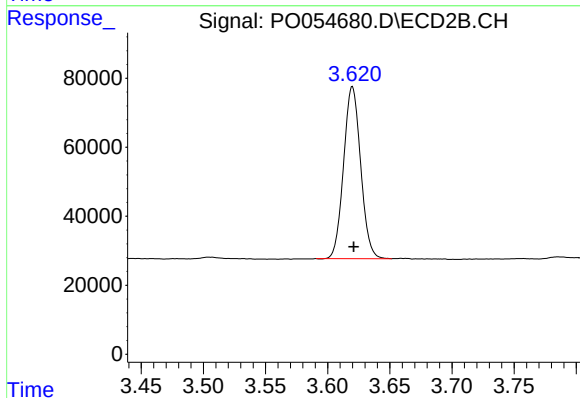


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: 0.000 min
Response: 476300
Conc: 14.93 ng/ml

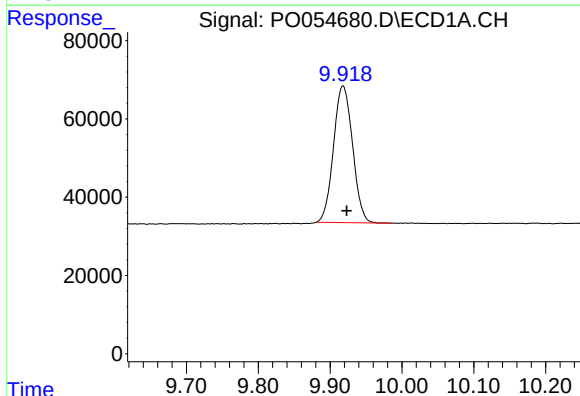


#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.005 min
Response: 643953
Conc: 13.06 ng/ml

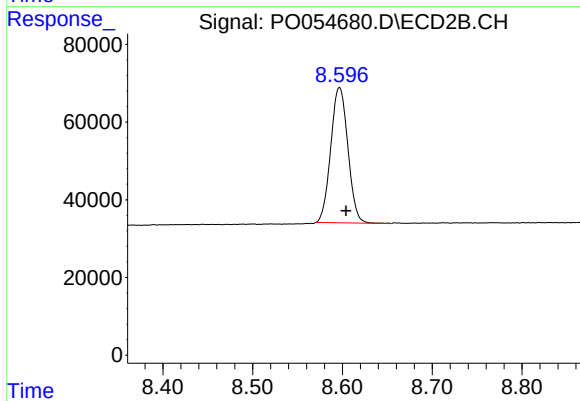

#2 Decachlorobiphenyl


R.T.: 8.597 min
Delta R.T.: -0.007 min
Response: 462259
Conc: 14.51 ng/ml

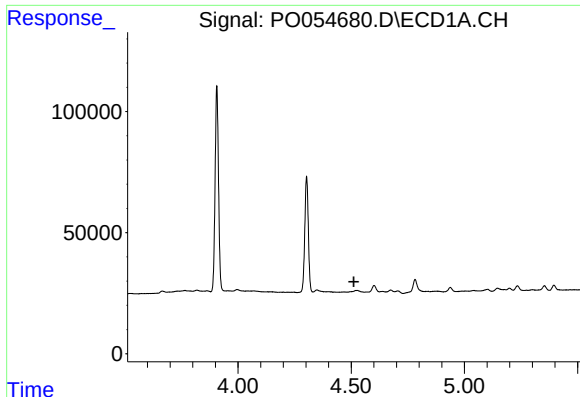

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.512 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MH-C05-SETTLED-3H-A

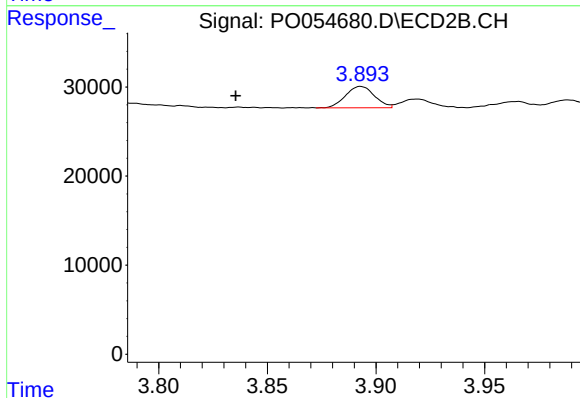


#8 AR-1221-1

R.T.: 3.893 min
Delta R.T.: 0.057 min
Response: 22286
Conc: 57.32 ng/ml

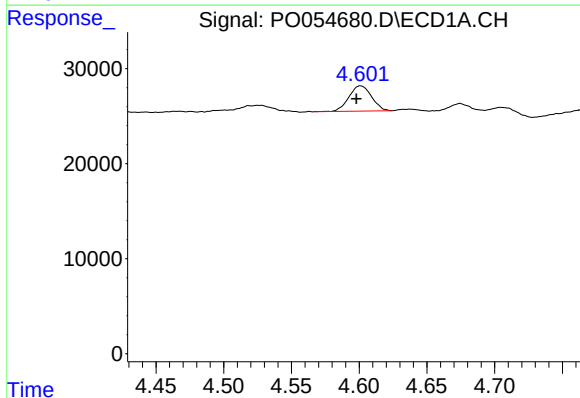


#9 AR-1221-2

R.T.: 4.601 min
Delta R.T.: 0.003 min
Response: 30837
Conc: 90.93 ng/ml

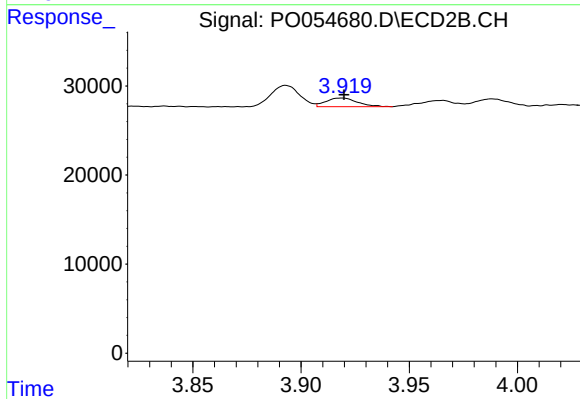

#9 AR-1221-2


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 9918
Conc: 33.08 ng/ml

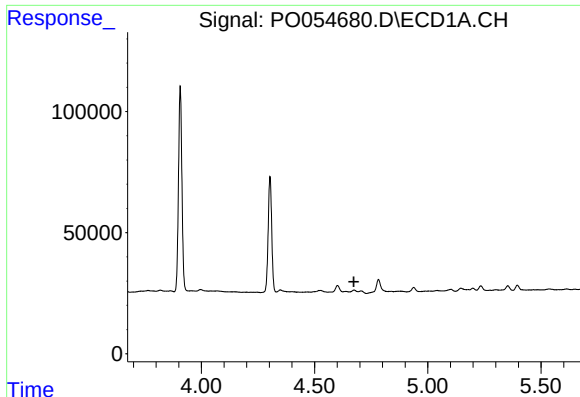

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MH-C05-SETTLED-3H-A

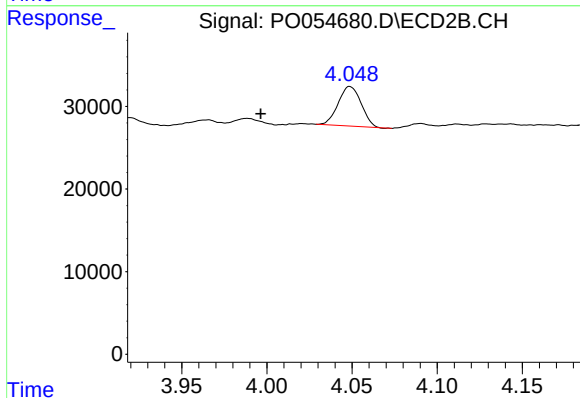


#10 AR-1221-3

R.T.: 4.049 min
Delta R.T.: 0.052 min
Response: 45063
Conc: 48.89 ng/ml

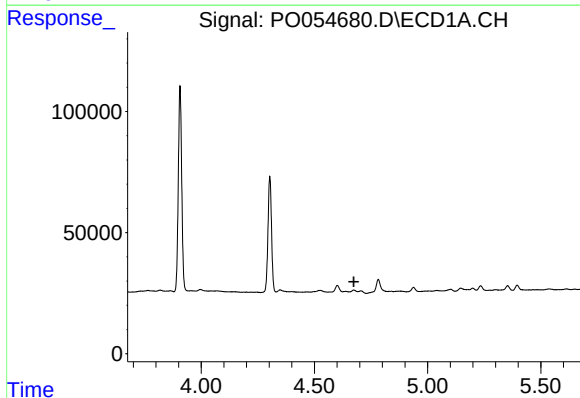


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 4.675 min
Response: 0
Conc: N.D.

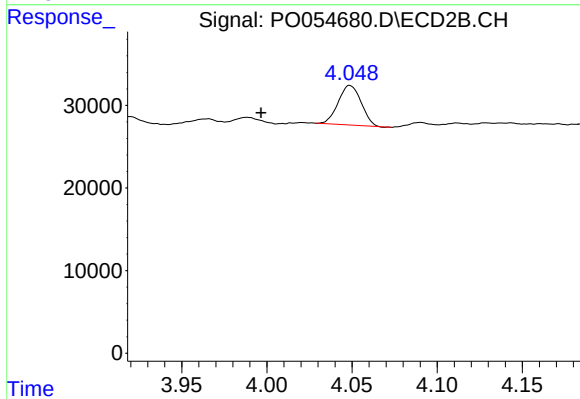

#11 AR-1232-1

R.T.: 4.049 min
Delta R.T.: 0.052 min
Response: 45063
Conc: 60.09 ng/ml

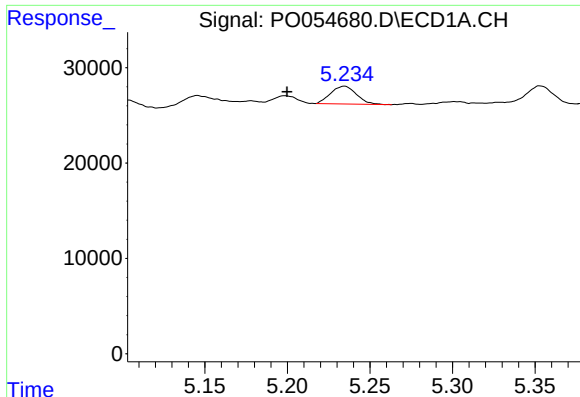

#12 AR-1232-2

R.T.: 5.235 min
Delta R.T.: 0.035 min
Response: 20205
Conc: 41.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-C05-SETTLED-3H-A

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.721 min
Response: 0
Conc: N.D.

#16 AR-1242-1

R.T.: 5.395 min
Delta R.T.: -0.070 min
Response: 22059
Conc: 15.88 ng/ml

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.701 min
Response: 0
Conc: N.D.

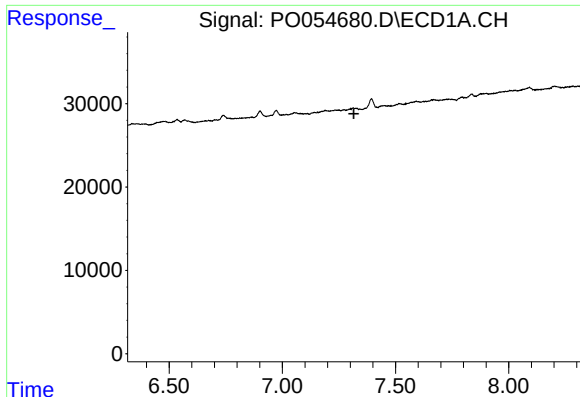

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MH-C05-SETTLED-3H-A

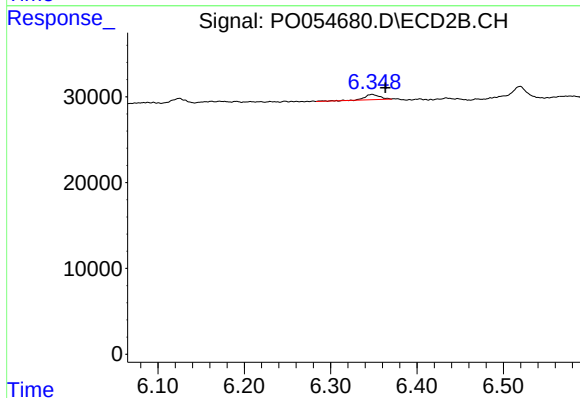


#32 AR-1260-2

R.T.: 6.348 min
Delta R.T.: -0.015 min
Response: 7568
Conc: 2.75 ng/ml

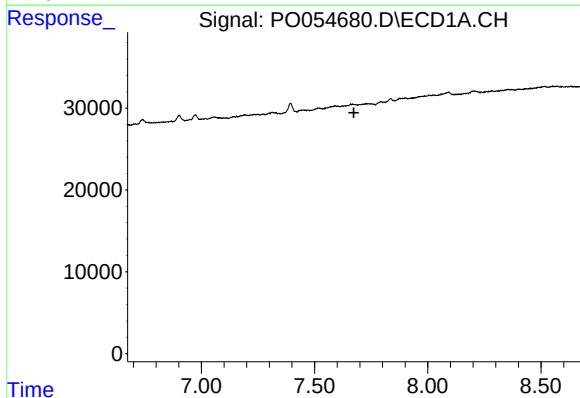

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.674 min
Response: 0
Conc: N.D.

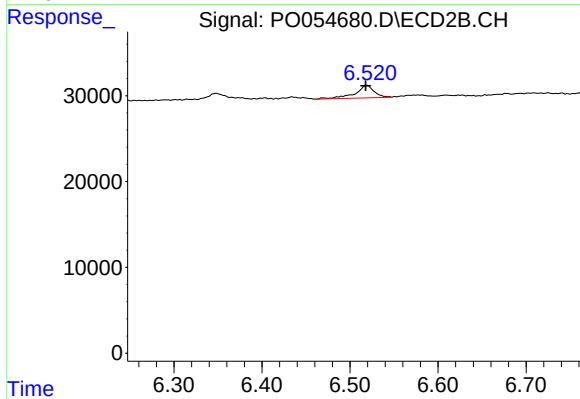

#33 AR-1260-3

R.T.: 6.520 min
Delta R.T.: 0.002 min
Response: 21900
Conc: 8.50 ng/ml