

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032719\
 Data File : P0054671.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 18:10
 Operator : SM/SJ
 Sample : K2099-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleID :
 SHORE-RD-CLVRT-STLD-2H-B

Manual Integrations
 APPROVED

Sohil
 3/28/2019 4:07:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 00:52:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.302	3.620	527937	481368	15.212	15.084
2) SA Decachlor...	9.920	8.596	692443	498354	14.046	15.648m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032719\
Data File : P0054671.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 18:10
Operator : SM/SJ
Sample : K2099-08
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-2H-B


Manual Integrations
APPROVED

Sohil
3/28/2019 4:07:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 00:52:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

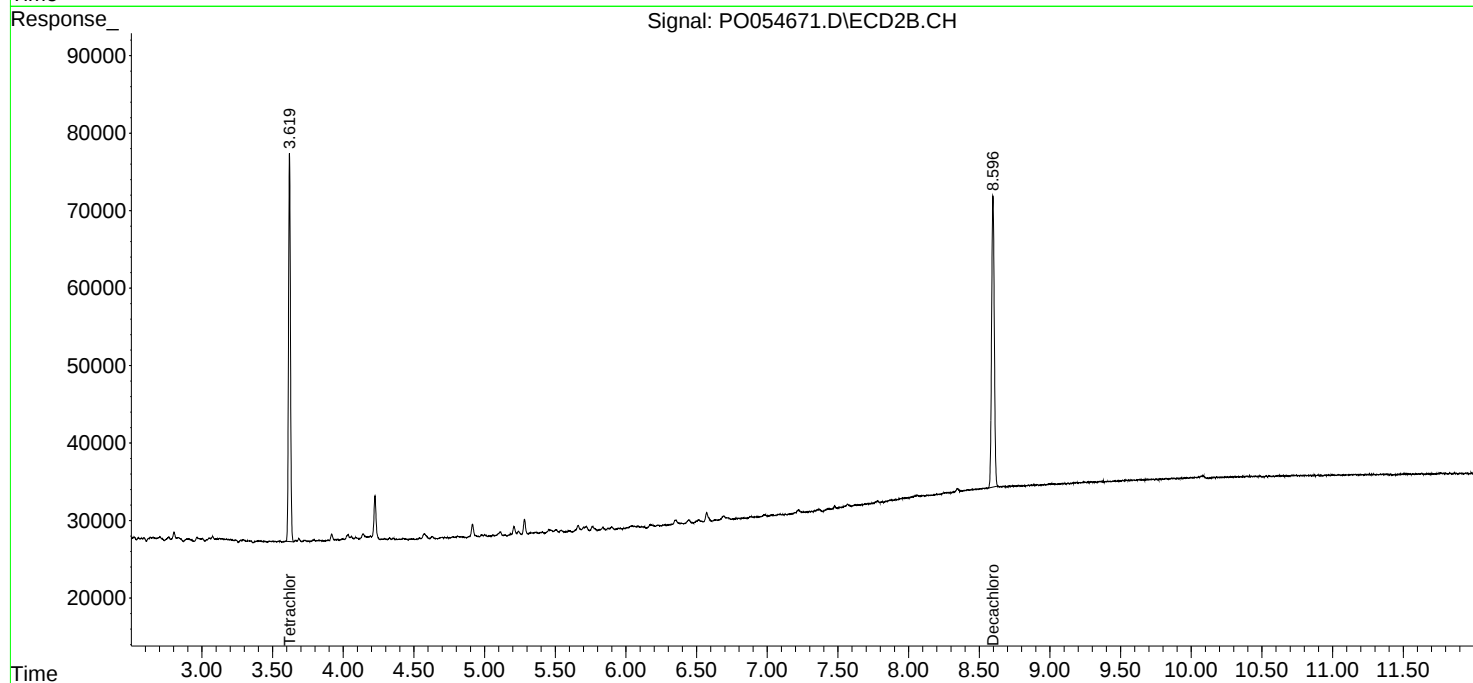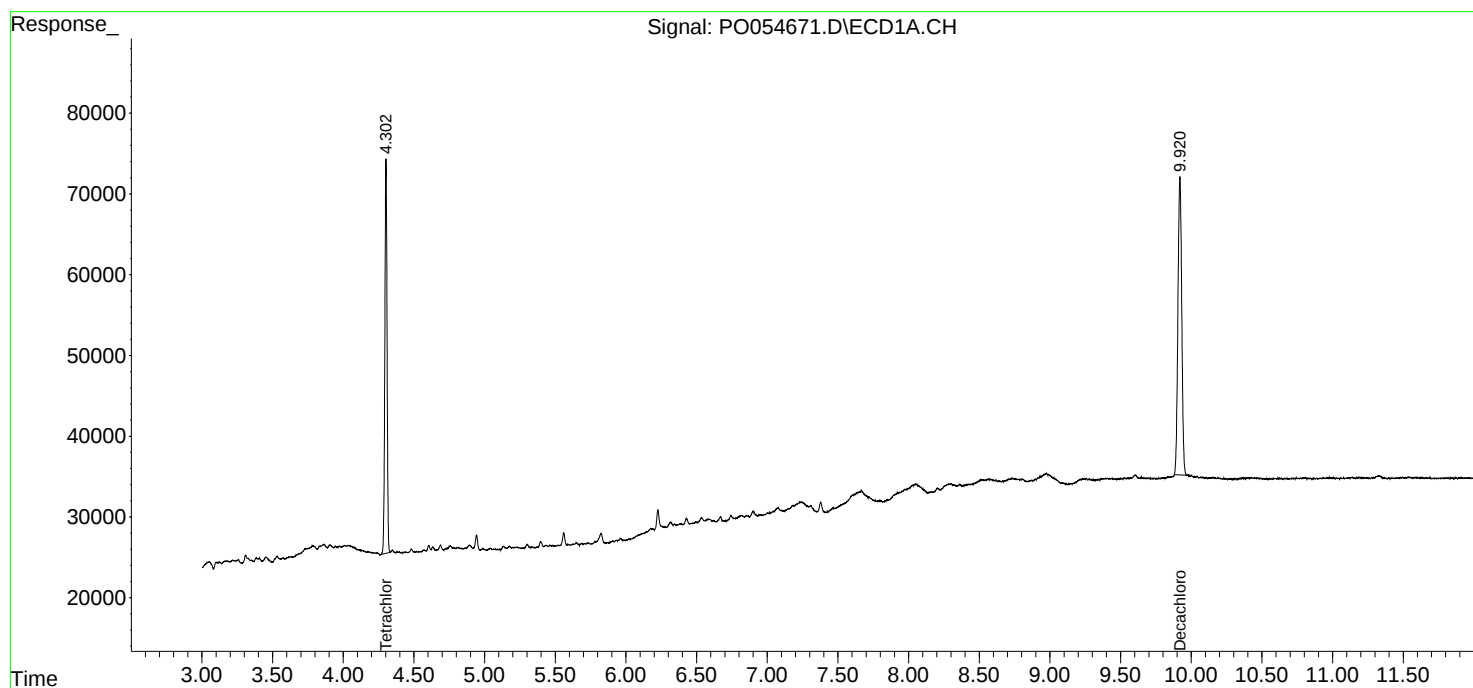

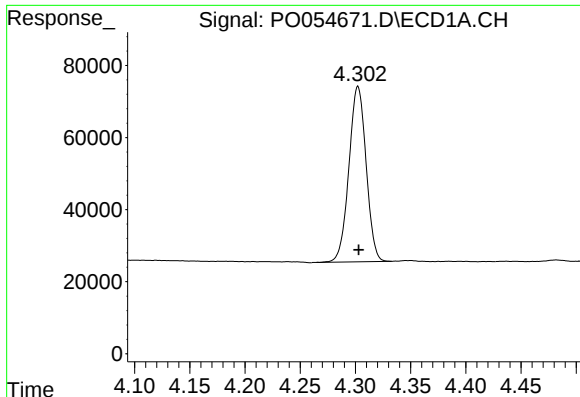


#1 Tetrachloro-m-xylene

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 527937
Conc: 15.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-CLVRT-STLD-2H-B


Manual Integrations
APPROVED

Sohil
3/28/2019 4:07:56 PM

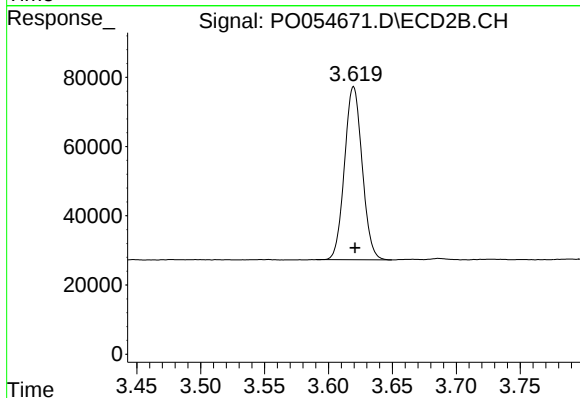


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.001 min
Response: 481368
Conc: 15.08 ng/ml

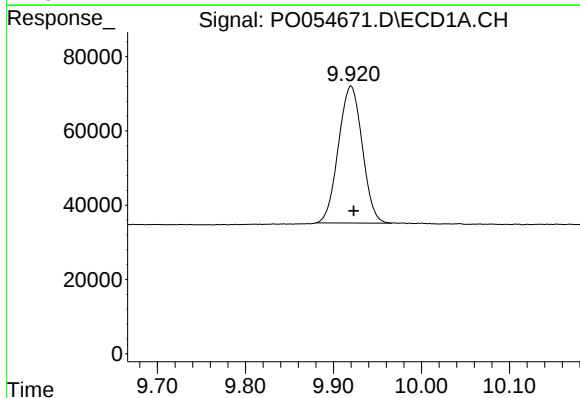

#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.003 min
Response: 692443
Conc: 14.05 ng/ml

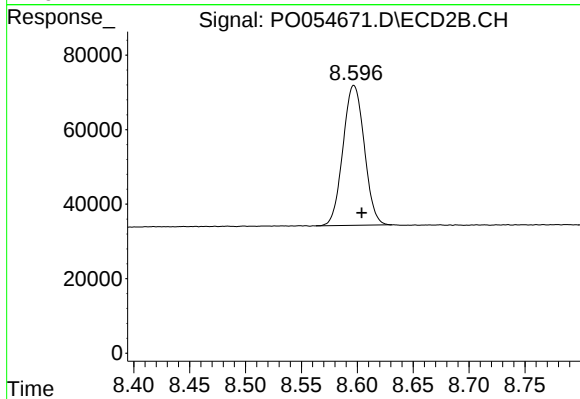

#2 Decachlorobiphenyl

R.T.: 8.596 min
Delta R.T.: -0.008 min
Response: 498354
Conc: 15.65 ng/ml m