

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032719\
 Data File : P0054674.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 19:01
 Operator : SM/SJ
 Sample : K2103-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH-C02-SETTLED-2H-A

Manual Integrations
 APPROVED

Sohil

3/28/2019 4:07:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 00:54:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.303	3.620	426935	390303	12.302	12.230
2) SA Decachlor...	9.920	8.596	597275	427932	12.116m	13.437m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032719\
Data File : P0054674.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 19:01
Operator : SM/SJ
Sample : K2103-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MH-C02-SETTLED-2H-A



Manual Integrations
APPROVED


Sohil

3/28/2019 4:07:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 00:54:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

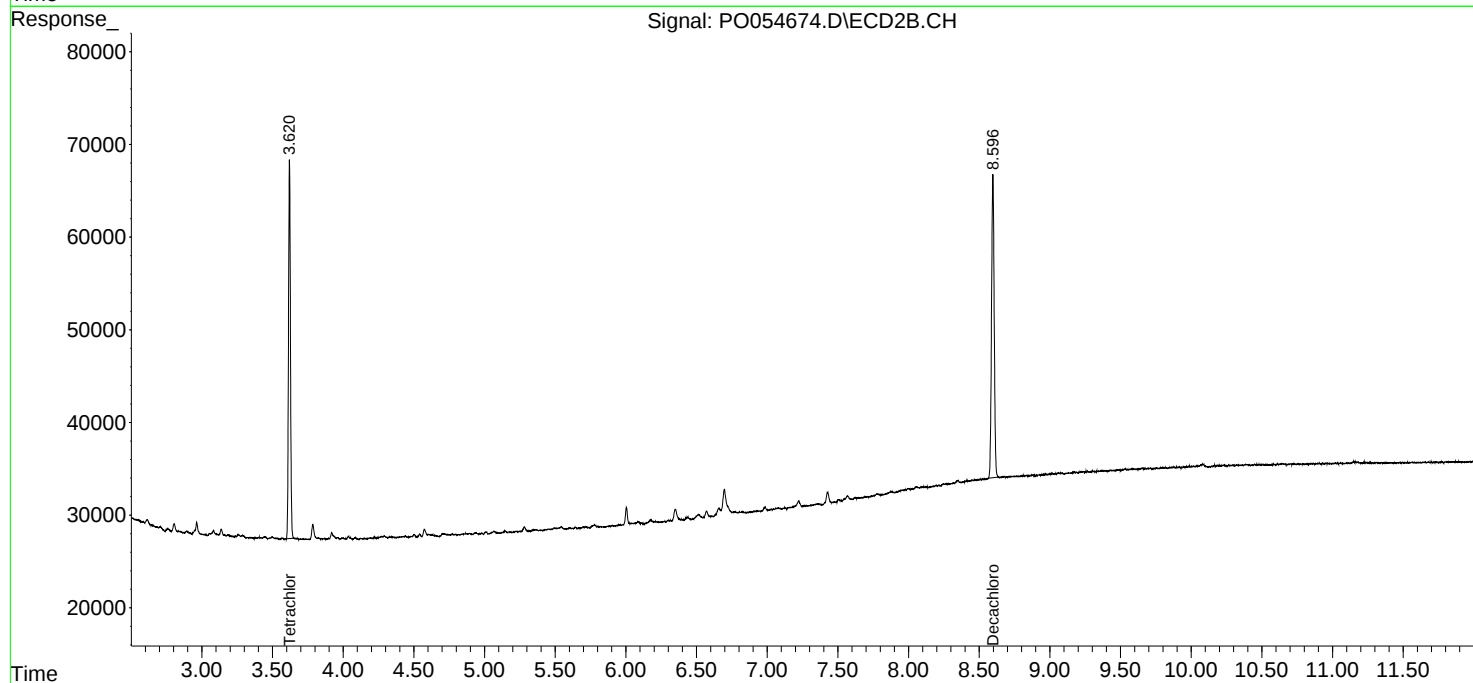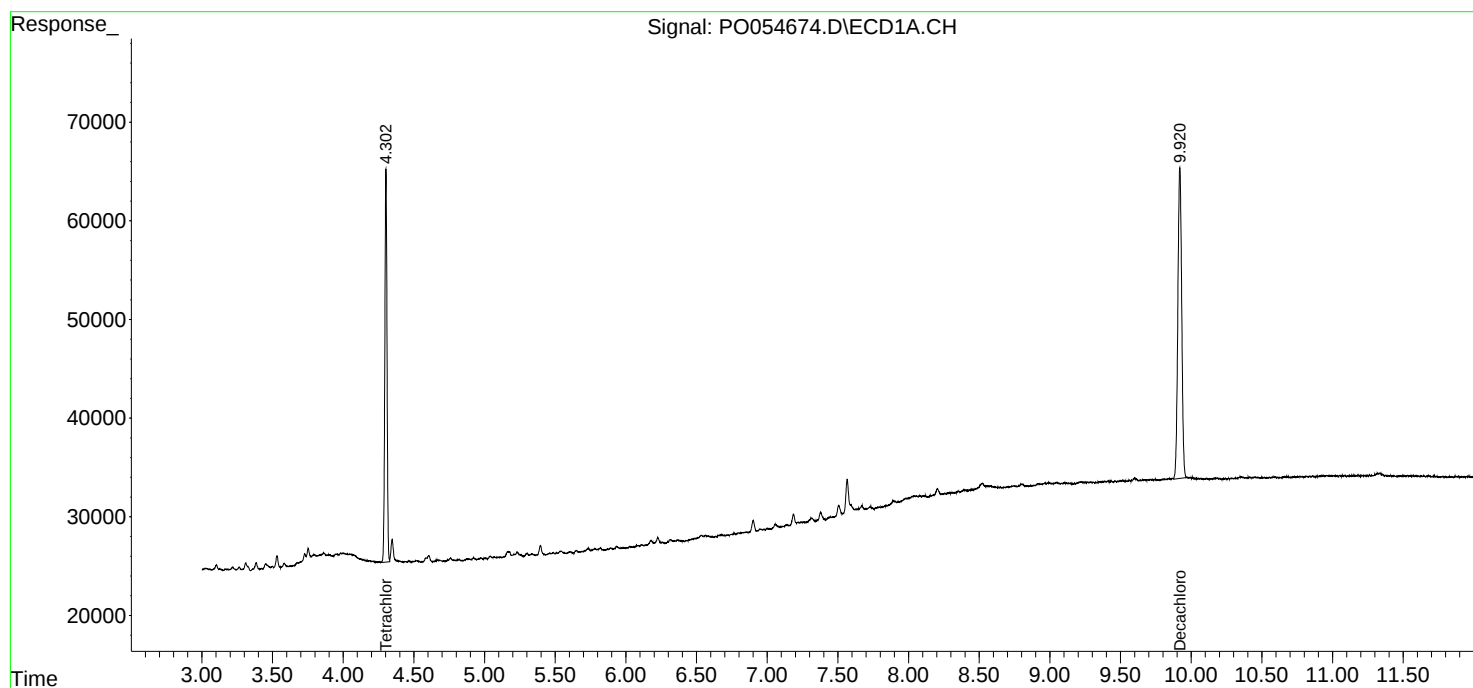

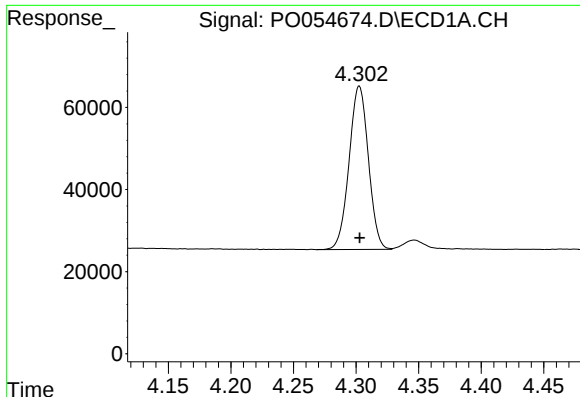

#1 Tetrachloro-m-xylene


R.T.: 4.303 min
Delta R.T.: 0.000 min
Response: 426935
Conc: 12.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-C02-SETTLED-2H-A

Manual Integrations
APPROVED


Sohil

3/28/2019 4:07:57 PM

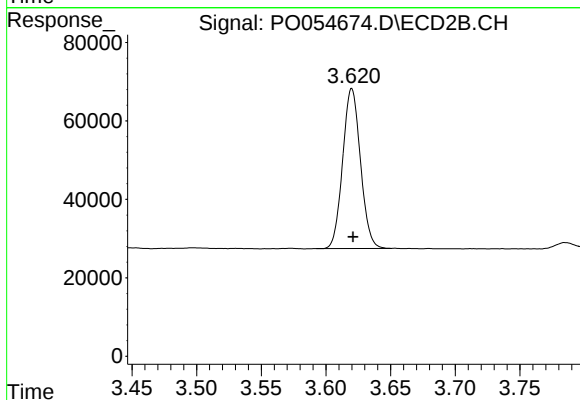


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: 0.000 min
Response: 390303
Conc: 12.23 ng/ml

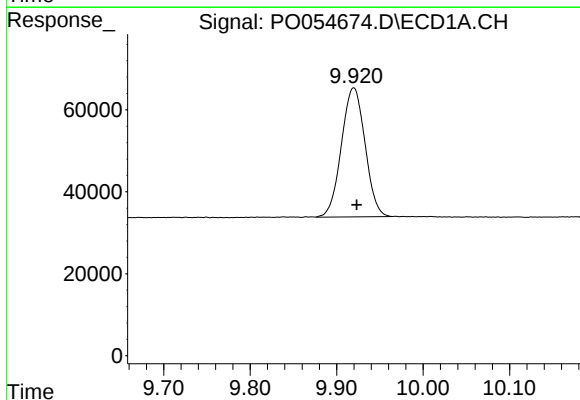

#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.004 min
Response: 597275
Conc: 12.12 ng/ml m

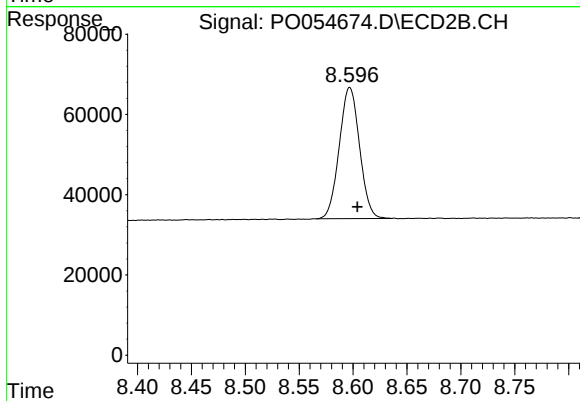

#2 Decachlorobiphenyl

R.T.: 8.596 min
Delta R.T.: -0.008 min
Response: 427932
Conc: 13.44 ng/ml m