

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032720\
 Data File : P0067485.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2020 17:29
 Operator : DD\AJ
 Sample : L2031-22
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WATER-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 19:00:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.939	3.948	259205	399720	12.196	11.434
2)	SA Decachlor...	10.924	9.240	186451	247180	6.489	6.337
Target Compounds							
3)	L1 AR-1016-1	0.000	5.224	0	44457	N.D.	29.062 #
4)	L1 AR-1016-2	0.000	5.224	0	44457	N.D.	22.036 #
5)	L1 AR-1016-3	0.000	5.417	0	67104	N.D.	60.127 #
6)	L1 AR-1016-4	0.000	5.417	0	67104	N.D.	72.149 #
12)	L3 AR-1232-2	0.000	5.224	0	44457	N.D.	60.595 #
13)	L3 AR-1232-3	0.000	5.417	0	67104	N.D.	171.723 #
16)	L4 AR-1242-1	0.000	5.224	0	44457	N.D.	38.087 #
17)	L4 AR-1242-2	0.000	5.224	0	44457	N.D.	29.032 #
18)	L4 AR-1242-3	0.000	5.417	0	67104	N.D.	79.535 #
20)	L4 AR-1242-5	0.000	6.046	0	19878	N.D.	18.588 #
21)	L5 AR-1248-1	0.000	5.224	0	44457	N.D.	56.084 #
22)	L5 AR-1248-2	0.000	5.417	0	67104	N.D.	65.039 #
26)	L6 AR-1254-1	0.000	6.046	0	19878	N.D.	10.209 #
28)	L6 AR-1254-3	0.000	6.661	0	223664	N.D.	79.747 #
38)	L8 AR-1262-3	0.000	8.161	0	67166	N.D.	33.641 #
39)	L8 AR-1262-4	0.000	8.161	0	67166	N.D.	19.141 #
41)	L9 AR-1268-1	0.000	8.161	0	67166	N.D.	12.657 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032720\
Data File : P0067485.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2020 17:29
Operator : DD\AJ
Sample : L2031-22
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 19:00:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

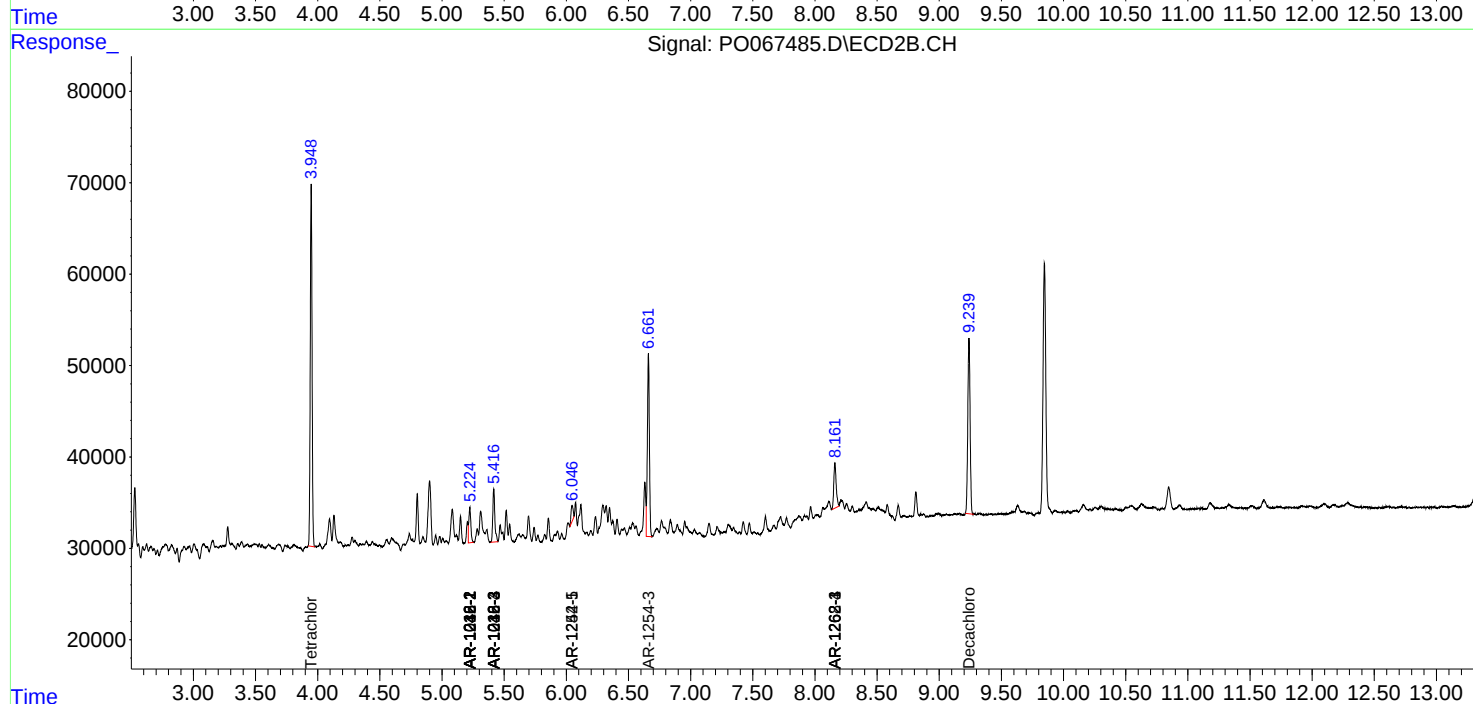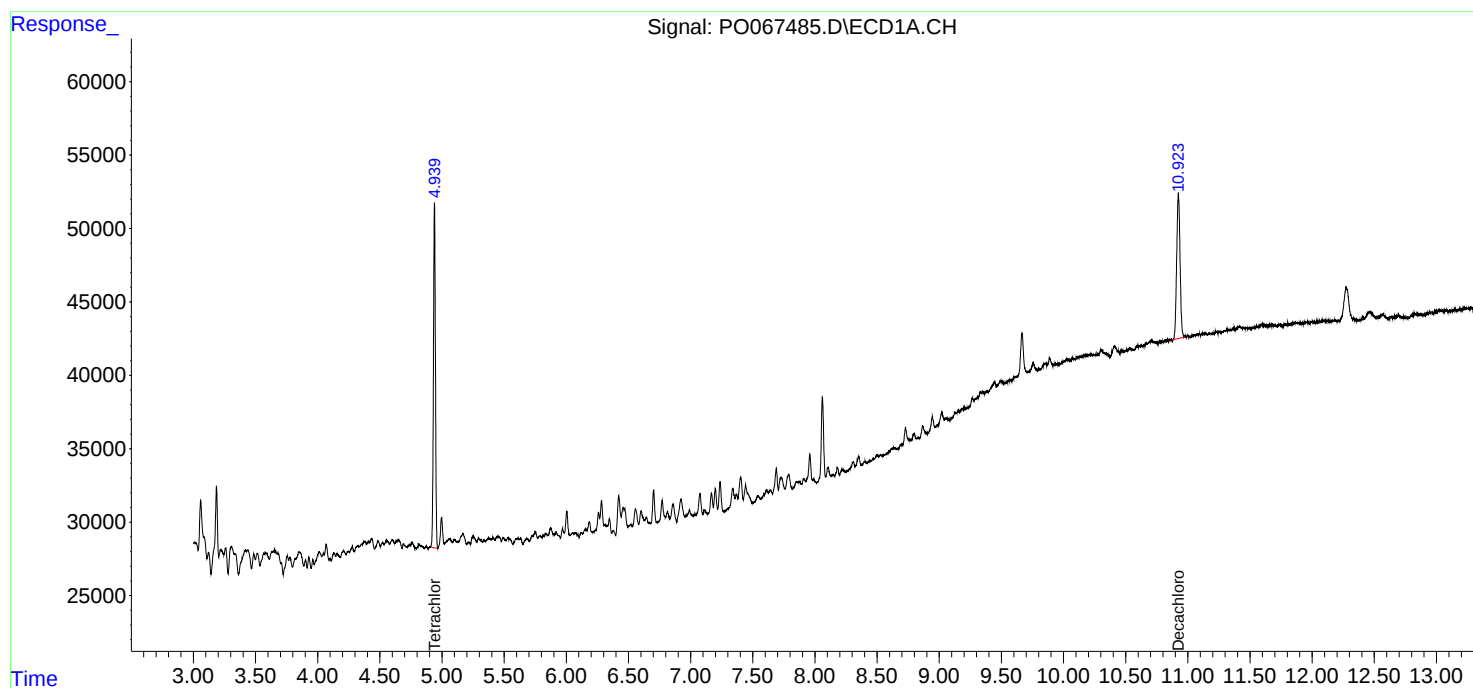


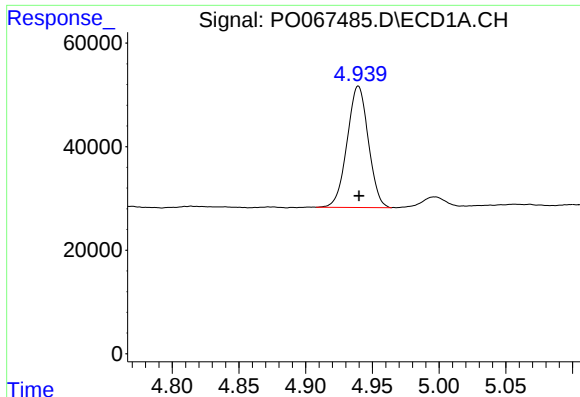

#1 Tetrachloro-m-xylene


R.T.: 4.939 min
Delta R.T.: 0.000 min
Response: 259205
Conc: 12.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

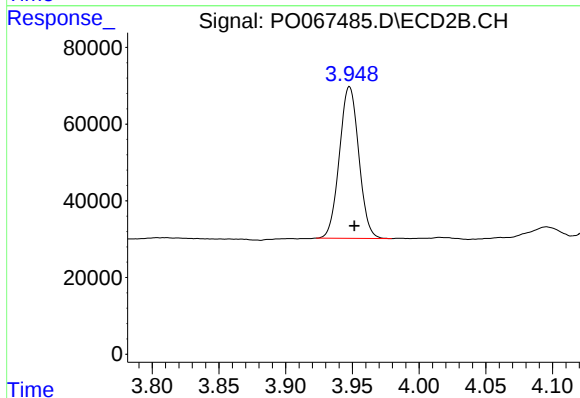


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.004 min
Response: 399720
Conc: 11.43 ng/ml

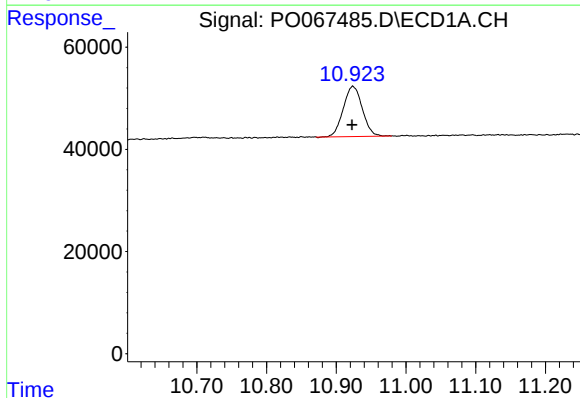


#2 Decachlorobiphenyl

R.T.: 10.924 min
Delta R.T.: 0.000 min
Response: 186451
Conc: 6.49 ng/ml

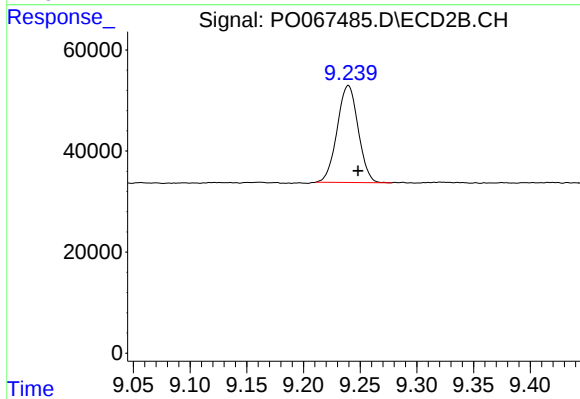

#2 Decachlorobiphenyl


R.T.: 9.240 min
Delta R.T.: -0.009 min
Response: 247180
Conc: 6.34 ng/ml

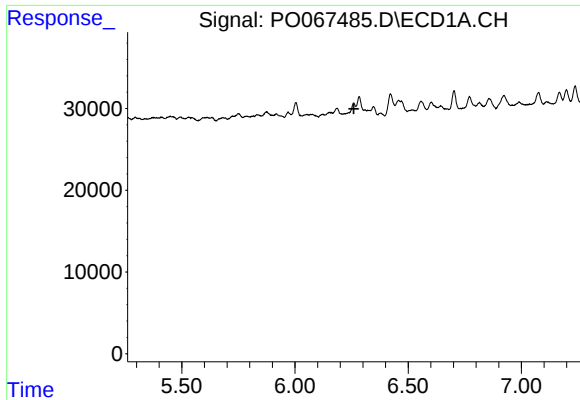

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 6.260 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

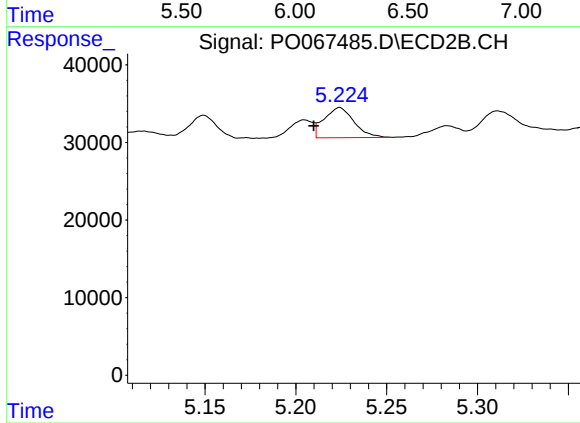


#3 AR-1016-1

R.T.: 5.224 min
Delta R.T.: 0.014 min
Response: 44457
Conc: 29.06 ng/ml

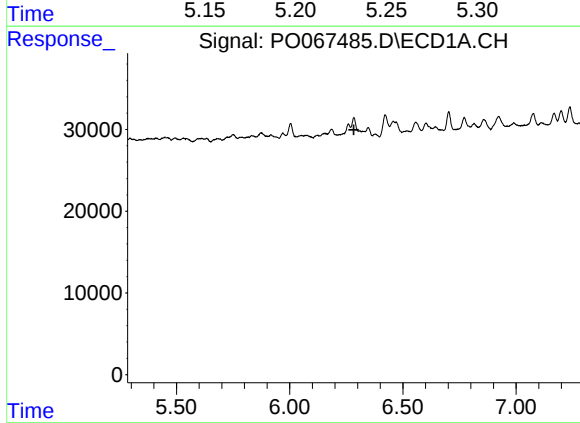


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 6.284 min
Response: 0
Conc: N.D.

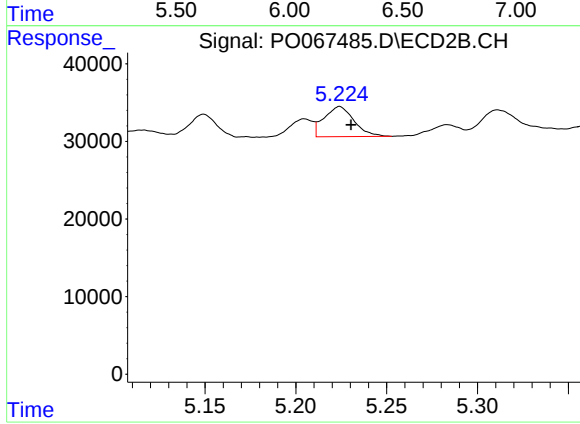

#4 AR-1016-2


R.T.: 5.224 min
Delta R.T.: -0.006 min
Response: 44457
Conc: 22.04 ng/ml

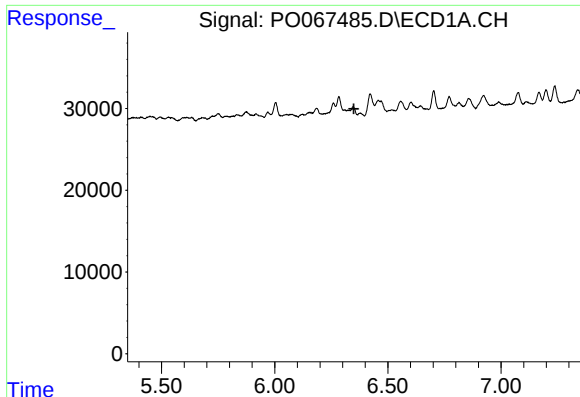

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

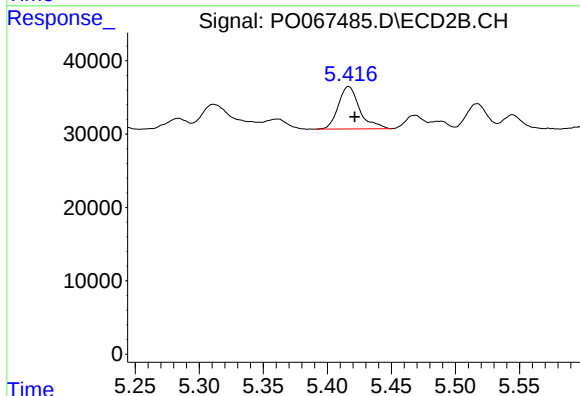


#5 AR-1016-3

R.T.: 5.417 min
Delta R.T.: -0.005 min
Response: 67104
Conc: 60.13 ng/ml

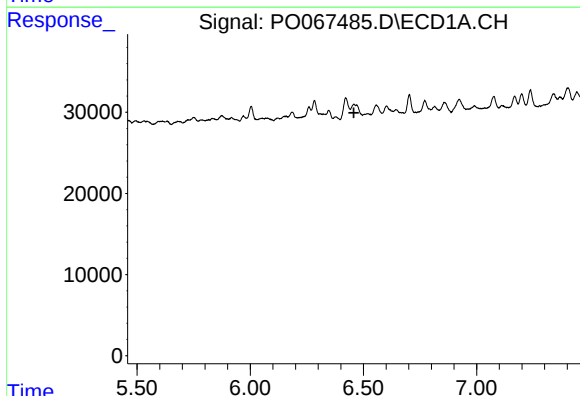


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

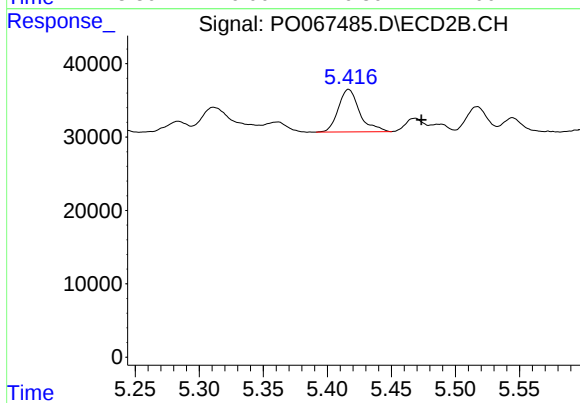

#6 AR-1016-4


R.T.: 5.417 min
Delta R.T.: -0.057 min
Response: 67104
Conc: 72.15 ng/ml

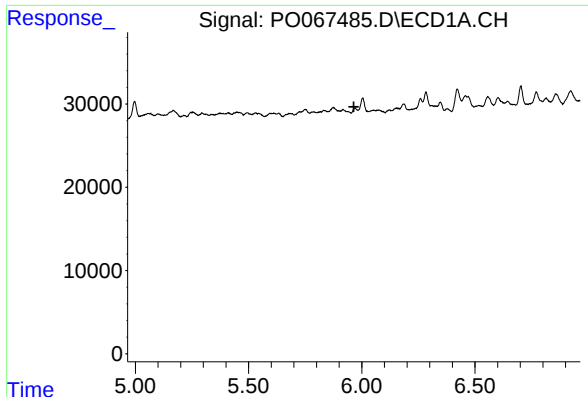

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

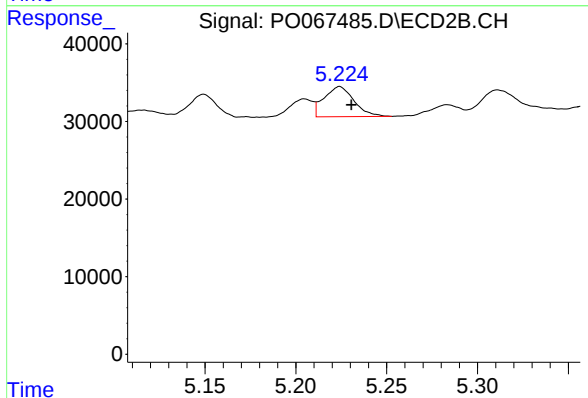


#12 AR-1232-2

R.T.: 5.224 min
Delta R.T.: -0.006 min
Response: 44457
Conc: 60.60 ng/ml

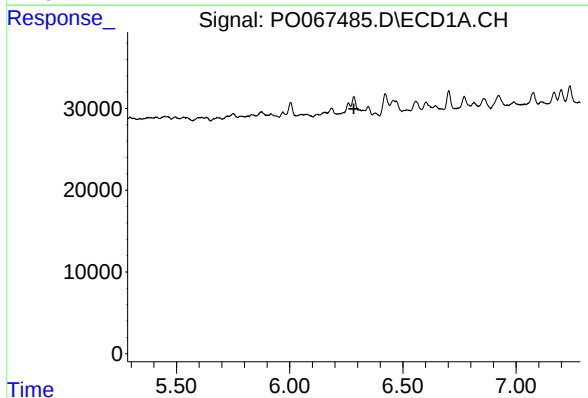


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T.: 6.283 min
Response: 0
Conc: N.D.

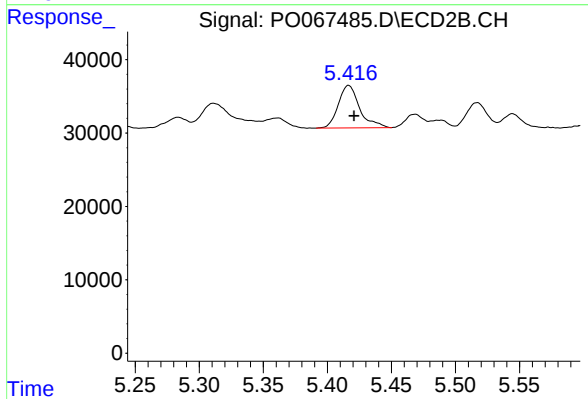

#13 AR-1232-3


R.T.: 5.417 min
Delta R.T.: -0.004 min
Response: 67104
Conc: 171.72 ng/ml

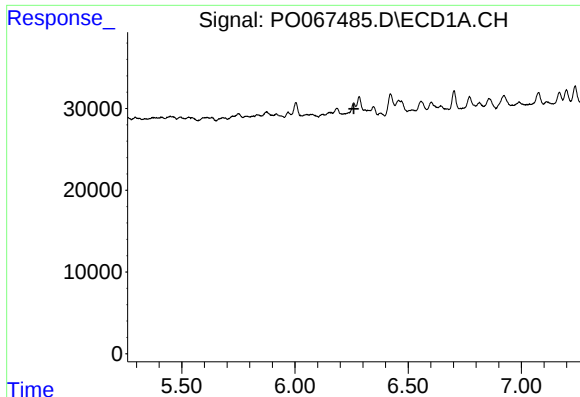

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 6.260 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

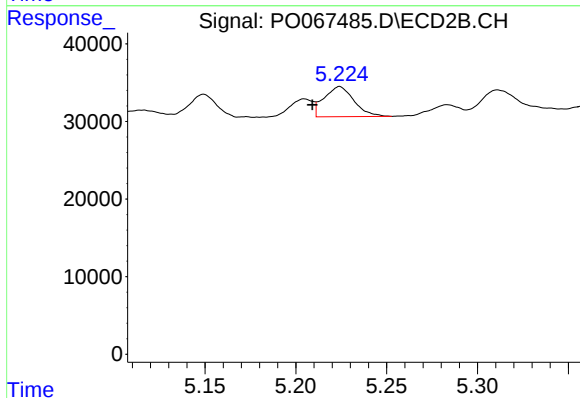


#16 AR-1242-1

R.T.: 5.224 min
Delta R.T.: 0.015 min
Response: 44457
Conc: 38.09 ng/ml

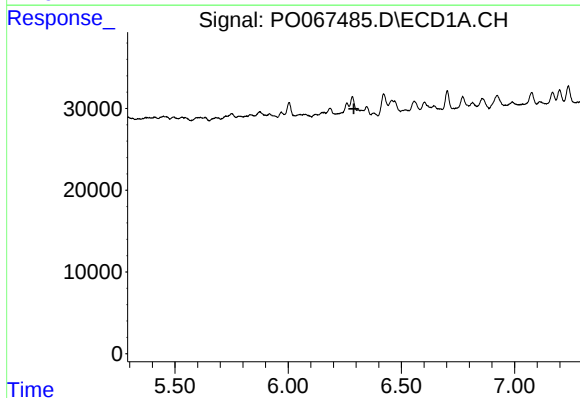


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 6.290 min
Response: 0
Conc: N.D.

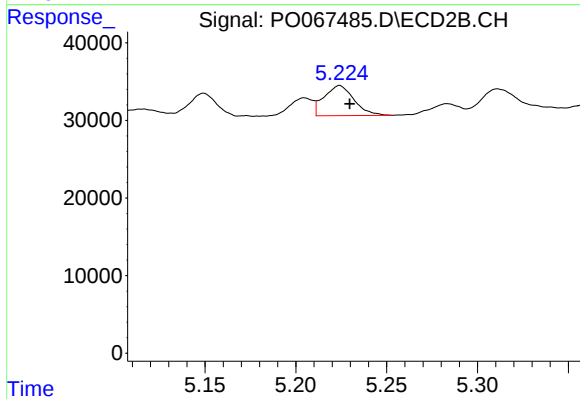

#17 AR-1242-2


R.T.: 5.224 min
Delta R.T.: -0.006 min
Response: 44457
Conc: 29.03 ng/ml

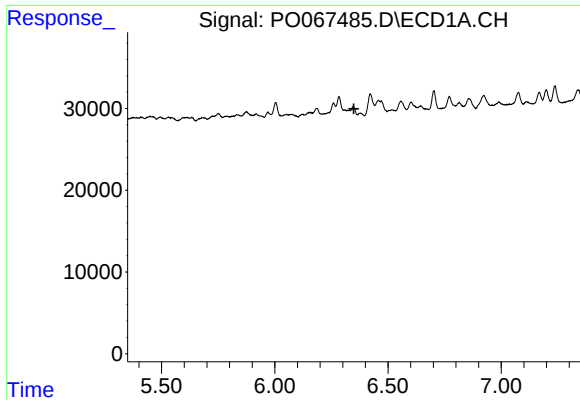

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 6.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

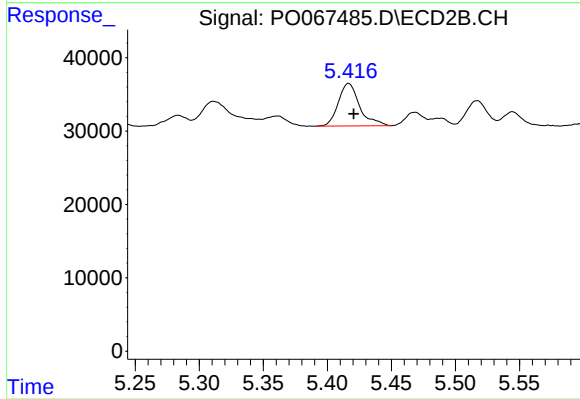


#18 AR-1242-3

R.T.: 5.417 min
Delta R.T.: -0.004 min
Response: 67104
Conc: 79.53 ng/ml

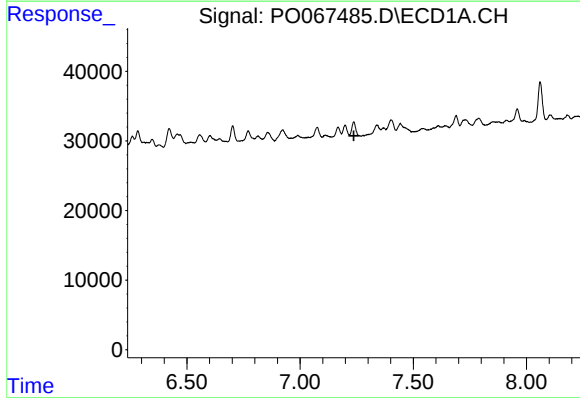


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.237 min
Response: 0
Conc: N.D.

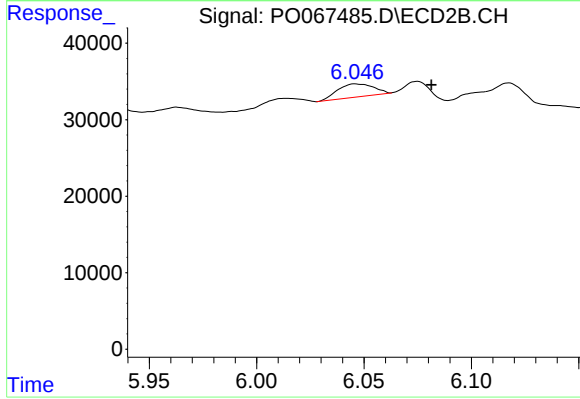

#20 AR-1242-5


R.T.: 6.046 min
Delta R.T.: -0.035 min
Response: 19878
Conc: 18.59 ng/ml

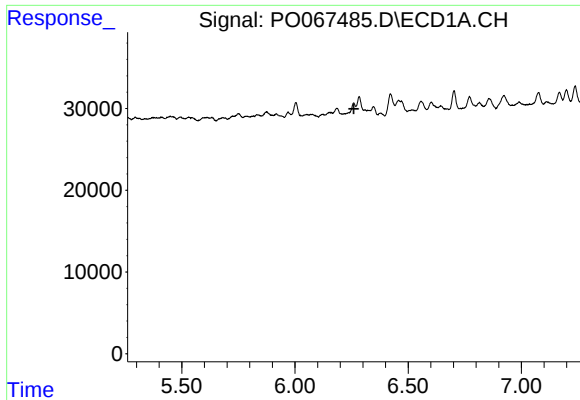

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 6.260 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

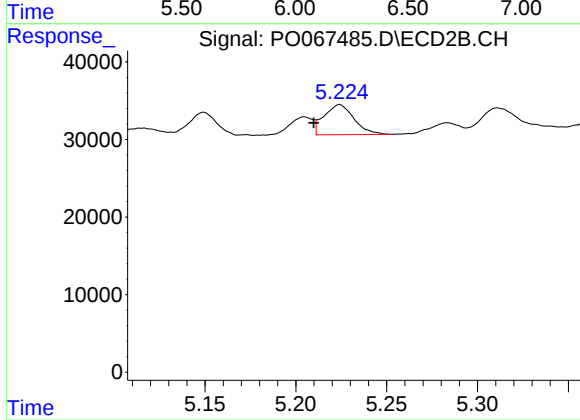


#21 AR-1248-1

R.T.: 5.224 min
Delta R.T.: 0.014 min
Response: 44457
Conc: 56.08 ng/ml

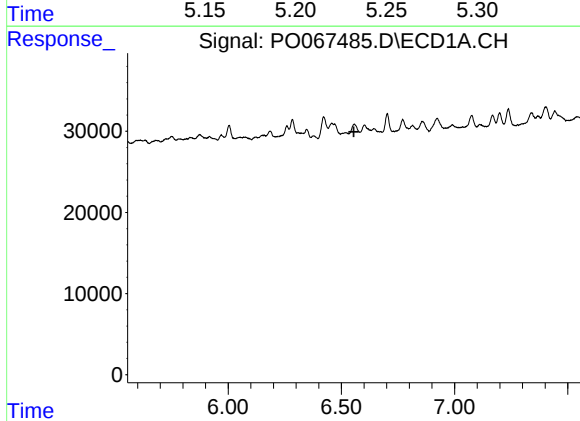


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 6.555 min
Response: 0
Conc: N.D.

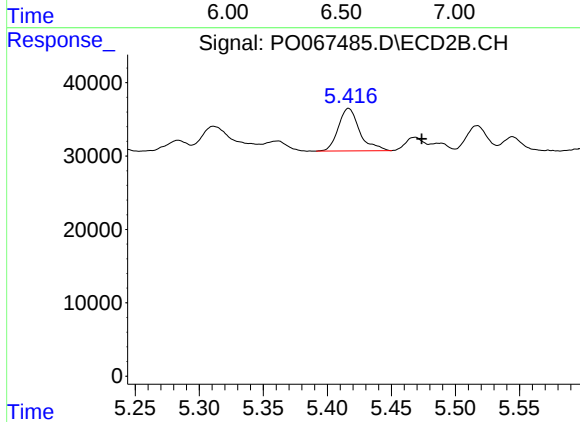

#22 AR-1248-2


R.T.: 5.417 min
Delta R.T.: -0.057 min
Response: 67104
Conc: 65.04 ng/ml

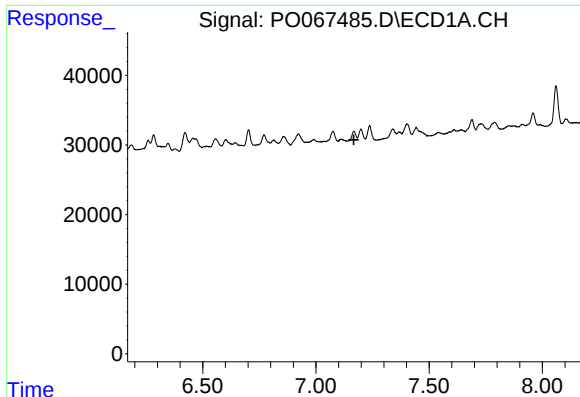

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

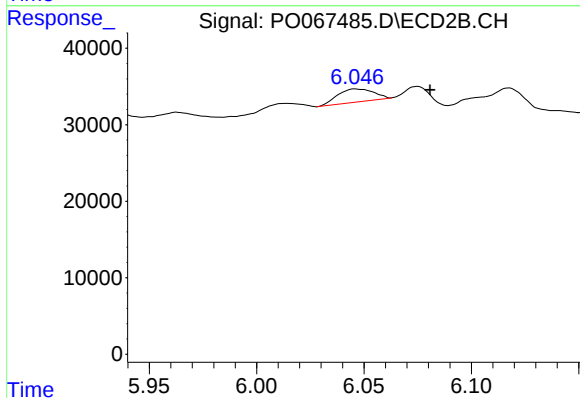


#26 AR-1254-1

R.T.: 6.046 min
Delta R.T.: -0.035 min
Response: 19878
Conc: 10.21 ng/ml

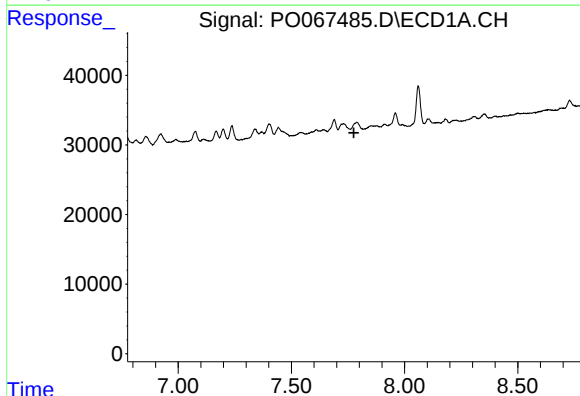


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 7.776 min
Response: 0
Conc: N.D.

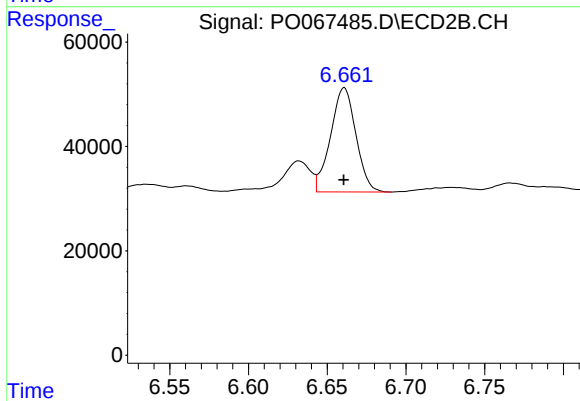

#28 AR-1254-3


R.T.: 6.661 min
Delta R.T.: 0.000 min
Response: 223664
Conc: 79.75 ng/ml

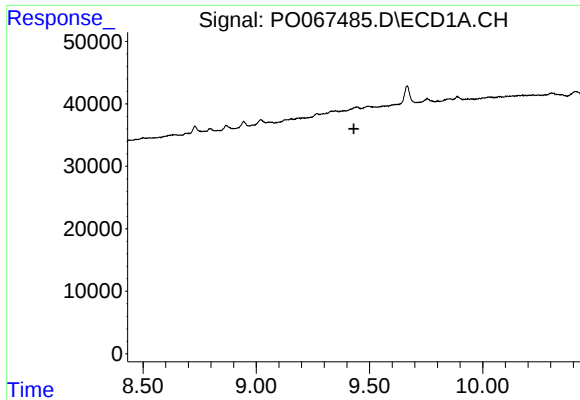

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

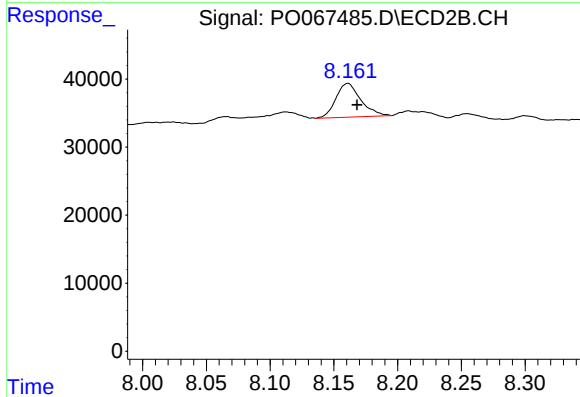


#38 AR-1262-3

R.T.: 8.161 min
Delta R.T.: -0.007 min
Response: 67166
Conc: 33.64 ng/ml

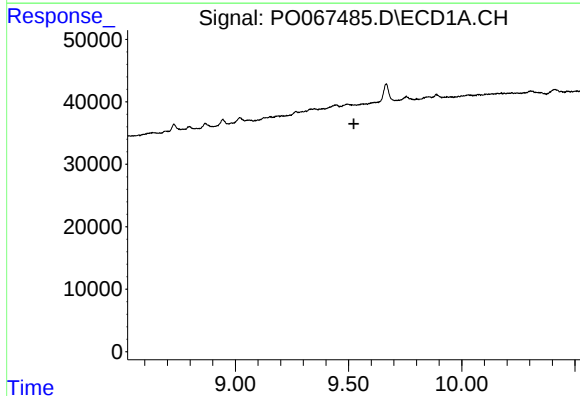


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.524 min
Response: 0
Conc: N.D.

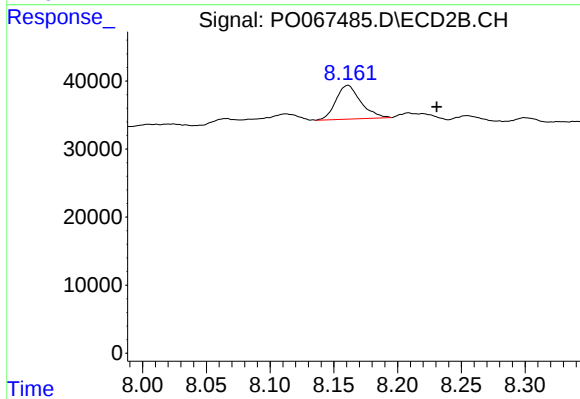

#39 AR-1262-4


R.T.: 8.161 min
Delta R.T.: -0.070 min
Response: 67166
Conc: 19.14 ng/ml

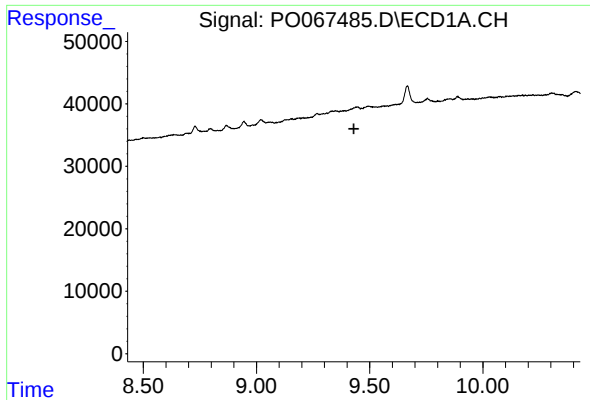

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

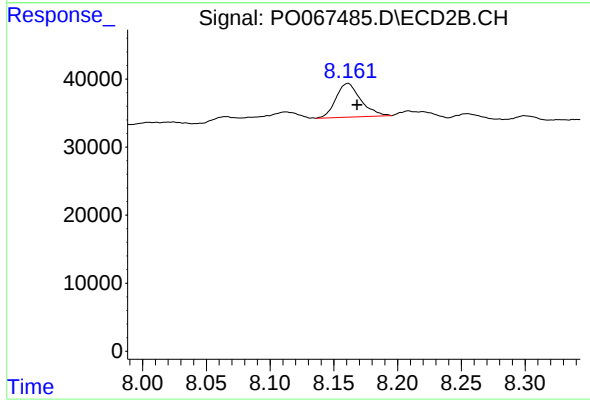

#41 AR-1268-1

R.T.: 8.161 min
Delta R.T.: -0.007 min
Response: 67166
Conc: 12.66 ng/ml