

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032720\
 Data File : P0067469.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2020 9:00
 Operator : DD\AJ
 Sample : L2027-01 2X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-24-A

Manual Integrations
 APPROVED

Sohil
 3/30/2020 11:37:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 12:27:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.951	3.951	239085	379281	11.249	10.849
2) SA Decachlor...	10.933	9.245	323775	416916	11.268	10.689m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032720\
Data File : P0067469.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2020 9:00
Operator : DD\AJ
Sample : L2027-01 2X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-24-A


Manual Integrations
APPROVED

Sohil
3/30/2020 11:37:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 12:27:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

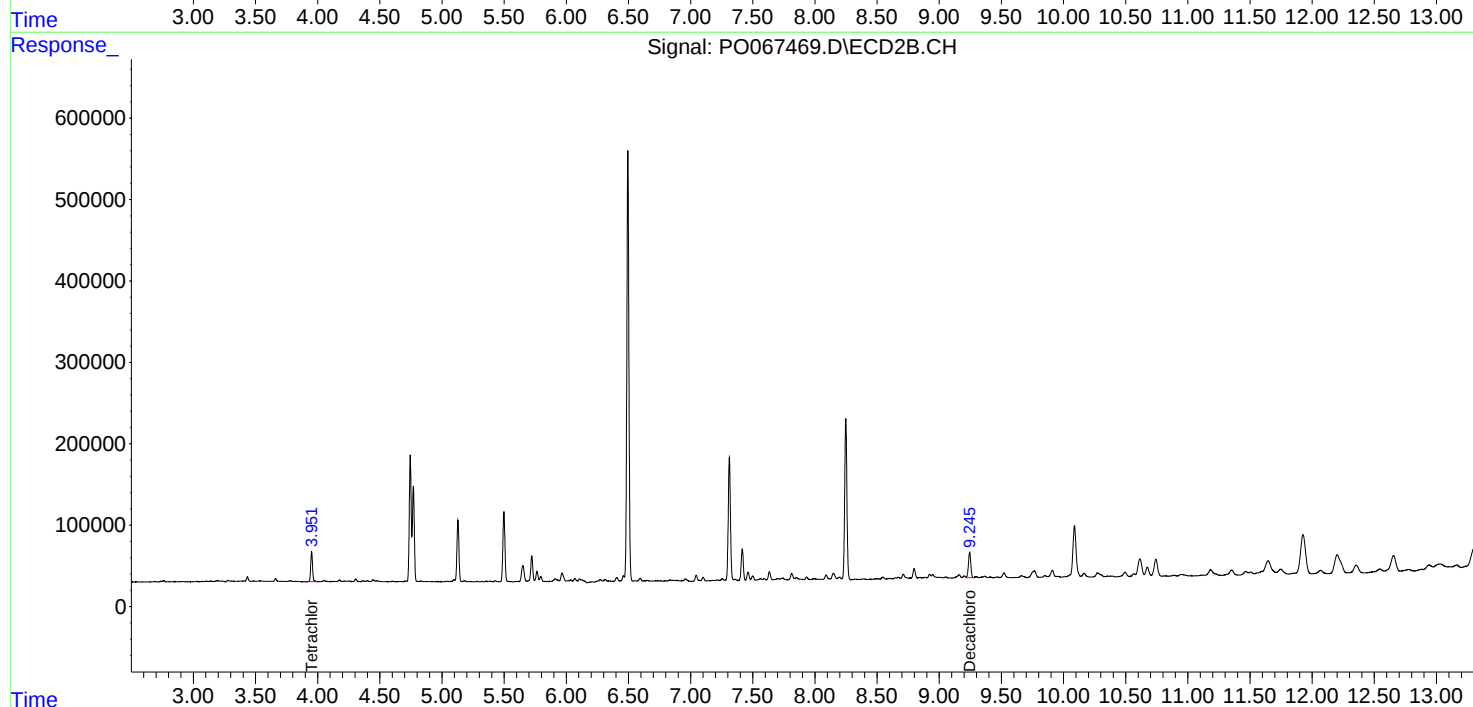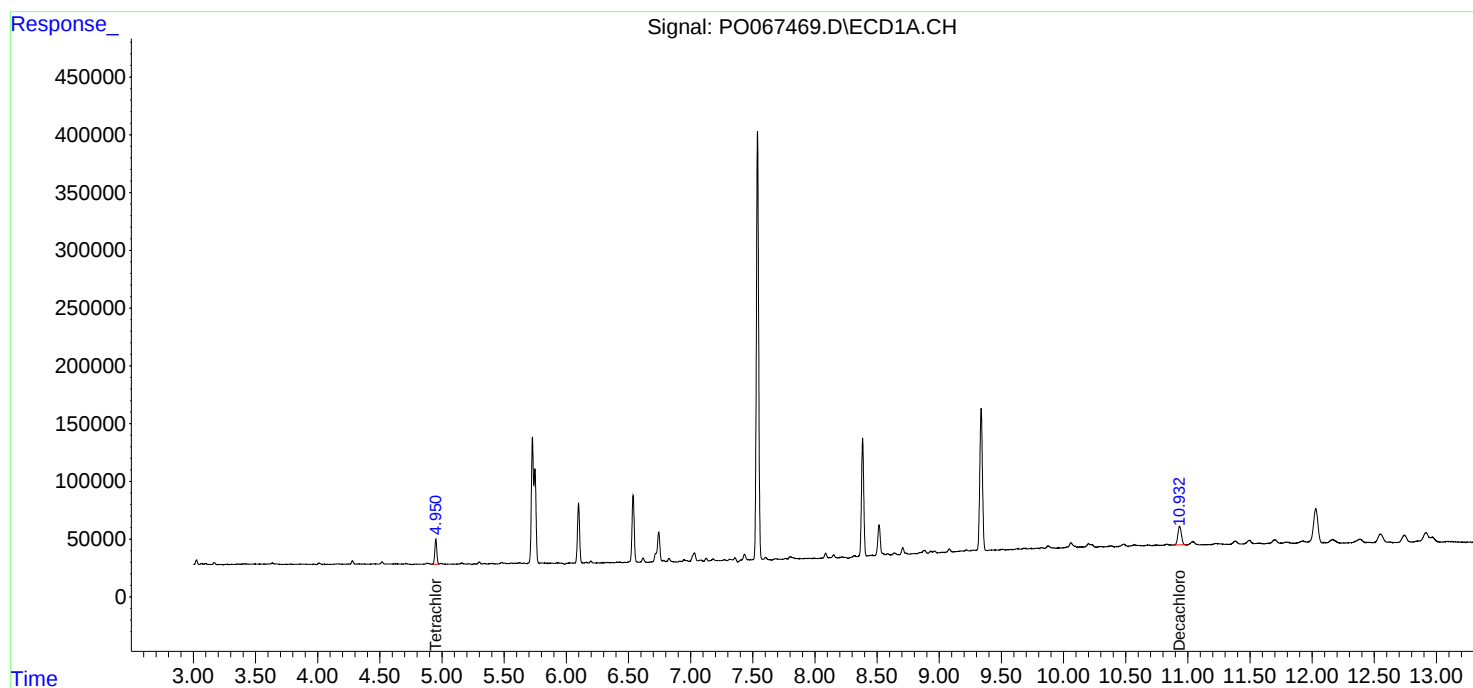

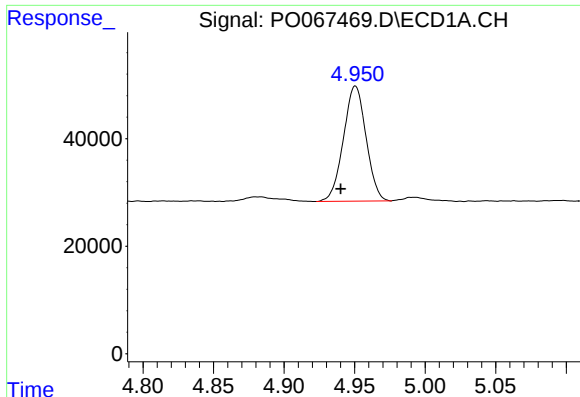


#1 Tetrachloro-m-xylene

R.T.: 4.951 min
Delta R.T.: 0.011 min
Response: 239085
Conc: 11.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-24-A


Manual Integrations
APPROVED

Sohil
3/30/2020 11:37:32 AM

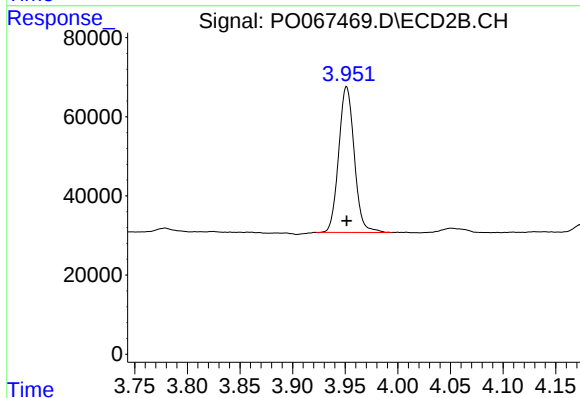


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 379281
Conc: 10.85 ng/ml

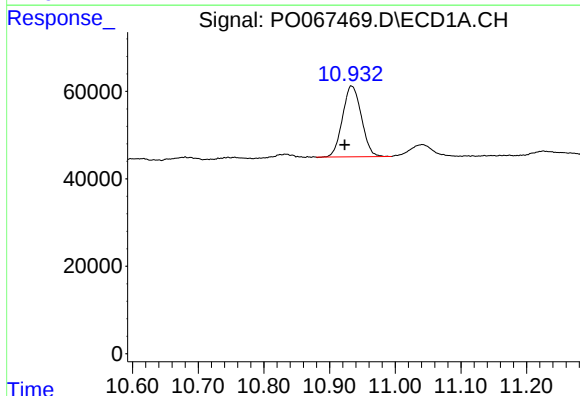

#2 Decachlorobiphenyl

R.T.: 10.933 min
Delta R.T.: 0.011 min
Response: 323775
Conc: 11.27 ng/ml

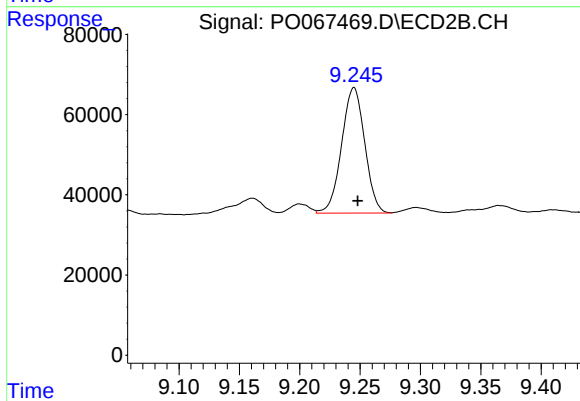

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.004 min
Response: 416916
Conc: 10.69 ng/ml m