

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032720\
 Data File : P0067481.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2020 16:21
 Operator : DD\AJ
 Sample : L2056-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 01-A-01-B-01-C

Manual Integrations
 APPROVED

Sohil
 3/30/2020 11:37:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 18:59:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	3.947	557107	809595	26.212	23.159
2) SA Decachlor...	10.922	9.239	690514	876465	24.032m	22.470m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032720\
Data File : P0067481.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2020 16:21
Operator : DD\AJ
Sample : L2056-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Sohil
3/30/2020 11:37:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 18:59:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

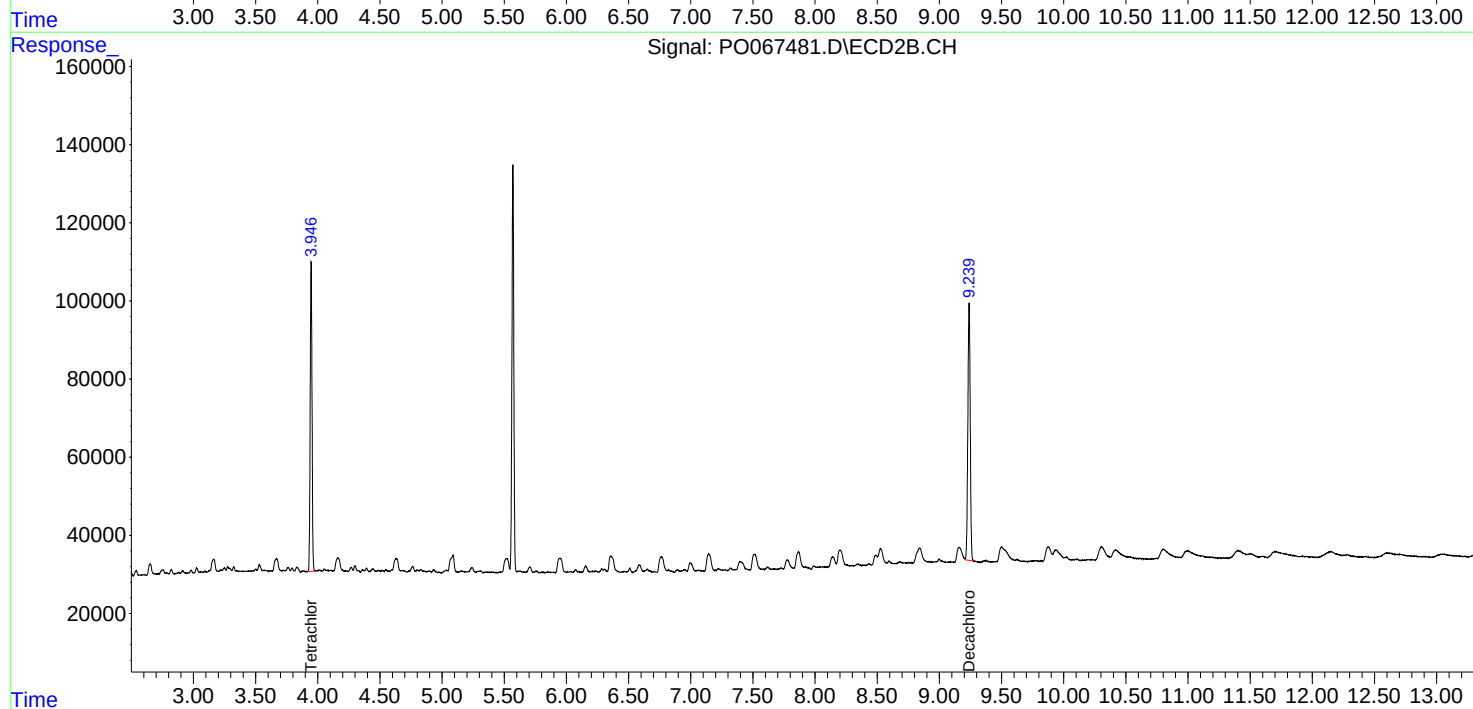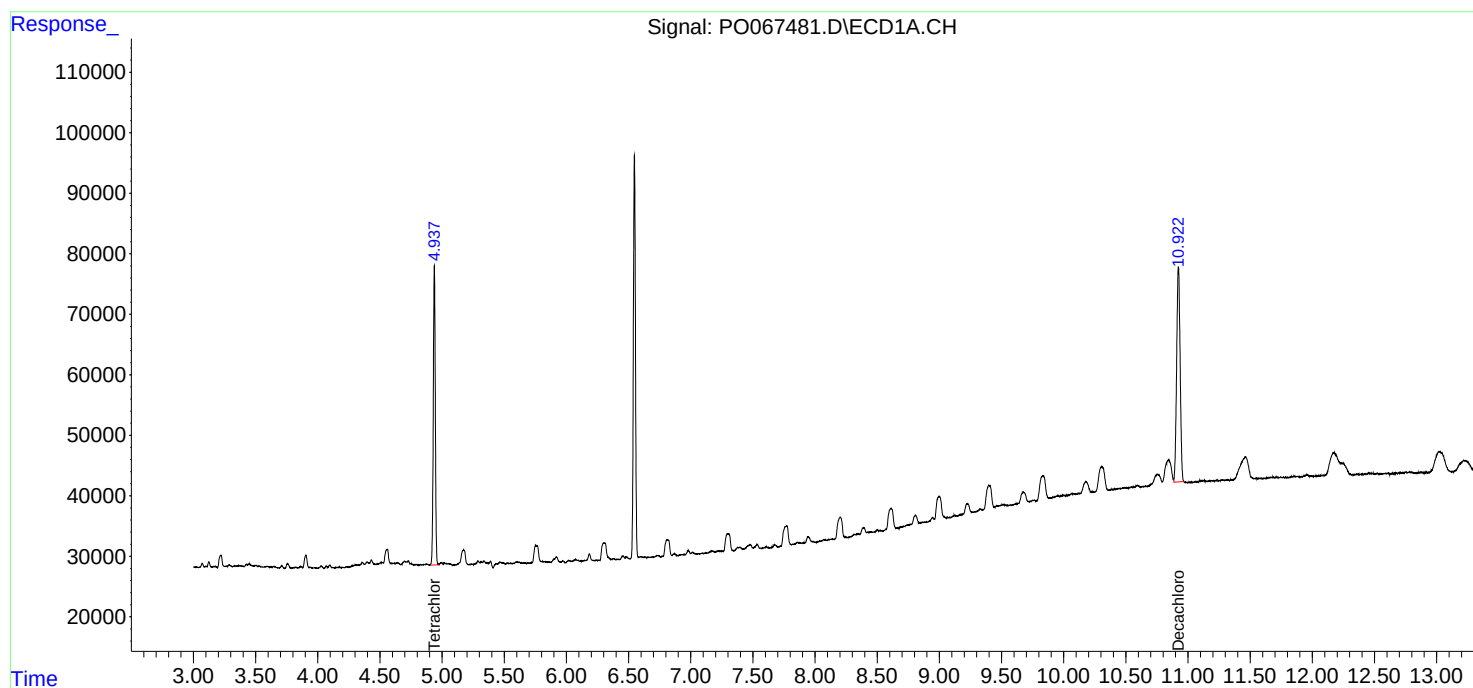

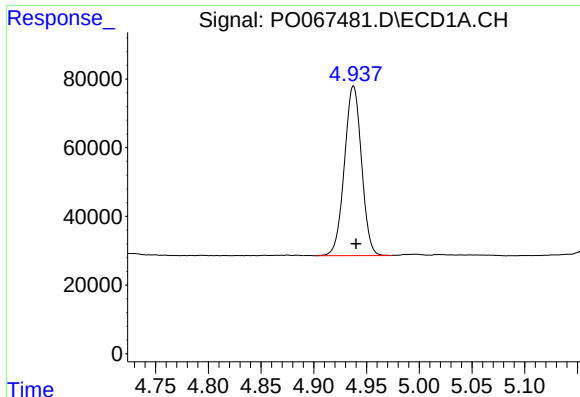


#1 Tetrachloro-m-xylene

R.T.: 4.938 min
Delta R.T.: -0.002 min
Response: 557107
Conc: 26.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Sohil
3/30/2020 11:37:43 AM

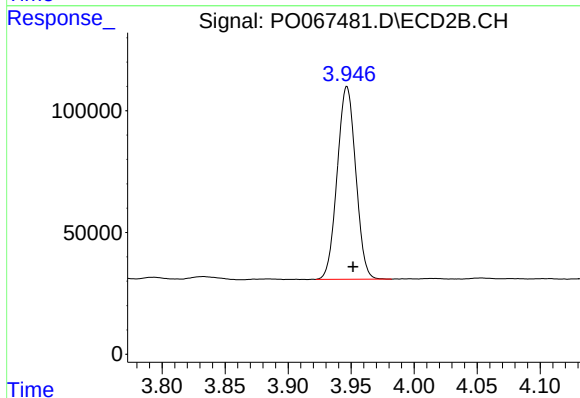


#1 Tetrachloro-m-xylene

R.T.: 3.947 min
Delta R.T.: -0.005 min
Response: 809595
Conc: 23.16 ng/ml

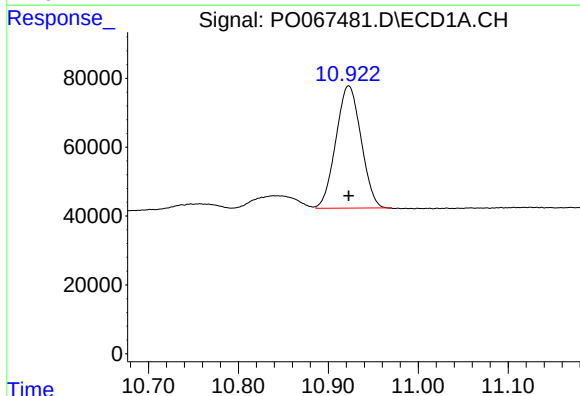

#2 Decachlorobiphenyl

R.T.: 10.922 min
Delta R.T.: 0.000 min
Response: 690514
Conc: 24.03 ng/ml m

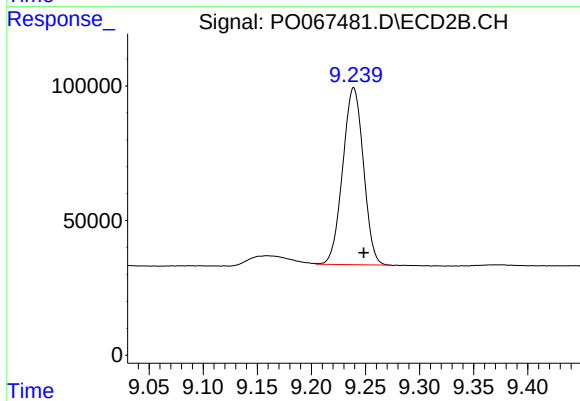

#2 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: -0.010 min
Response: 876465
Conc: 22.47 ng/ml m