

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032720\
 Data File : P0067496.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2020 20:37
 Operator : DD\AJ
 Sample : L2049-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-5-(10-12)

Manual Integrations
 APPROVED

Sohil
 3/30/2020 11:37:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 05:34:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	3.946	613163	894819	28.850	25.597m
2) SA Decachlor...	10.923	9.238	711862	897284	24.775	23.004

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032720\
Data File : P0067496.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2020 20:37
Operator : DD\AJ
Sample : L2049-07
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-5-(10-12)


Manual Integrations
APPROVED

Sohil
3/30/2020 11:37:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 05:34:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

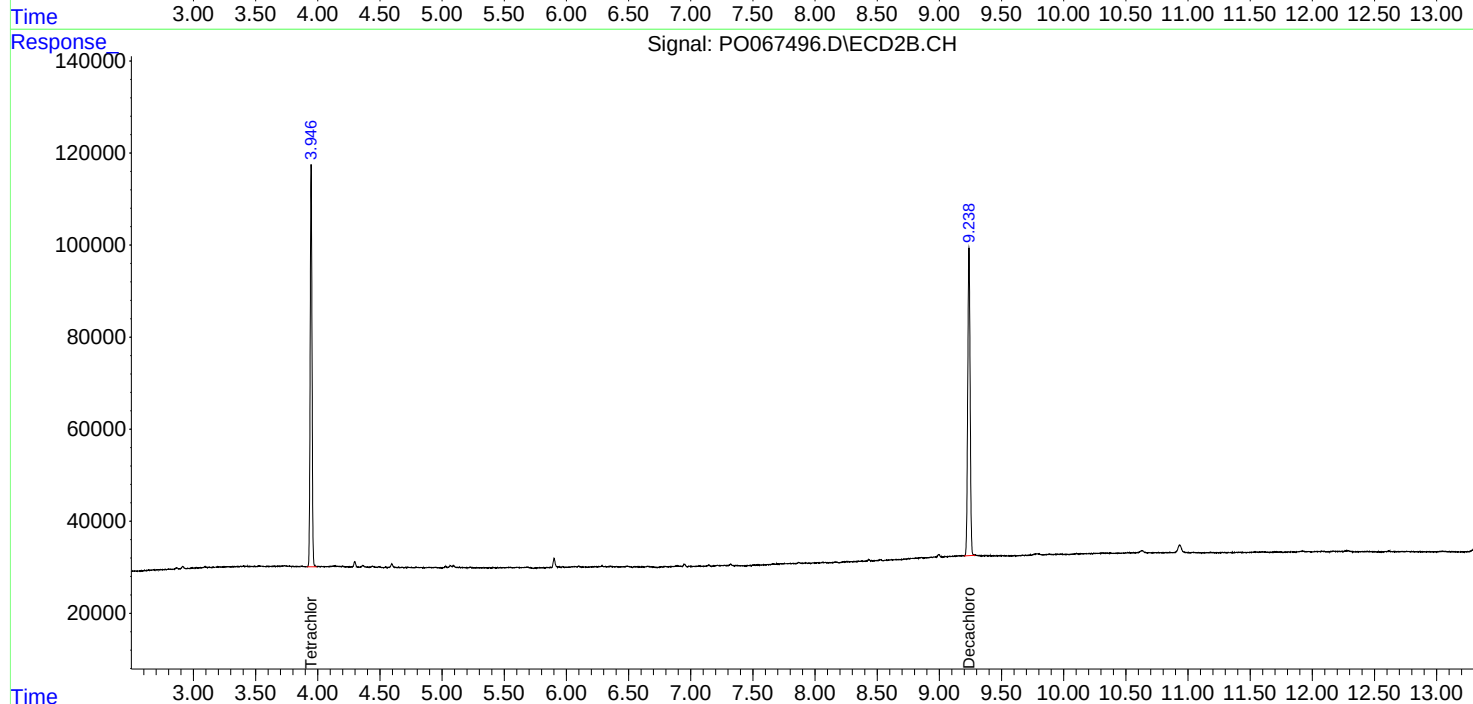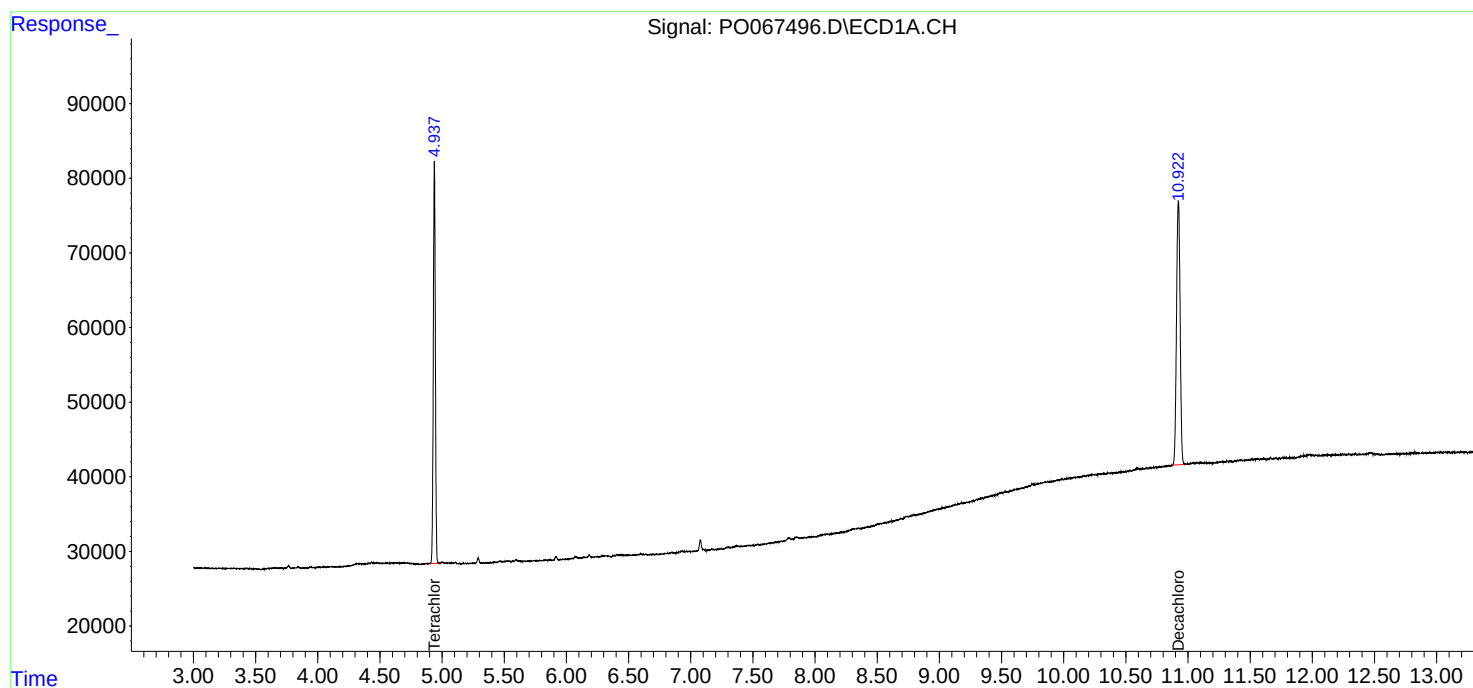

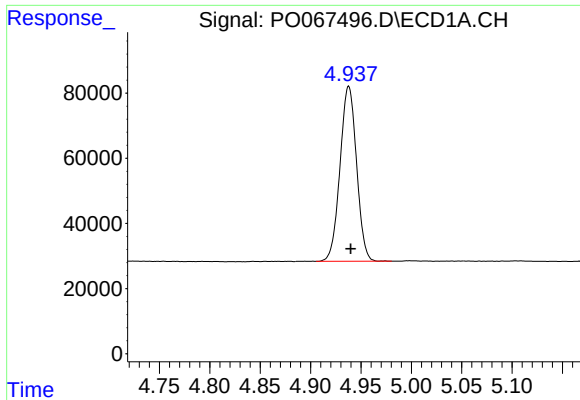


#1 Tetrachloro-m-xylene

R.T.: 4.938 min
Delta R.T.: -0.002 min
Response: 613163
Conc: 28.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-5-(10-12)


Manual Integrations
APPROVED

Sohil
3/30/2020 11:37:52 AM

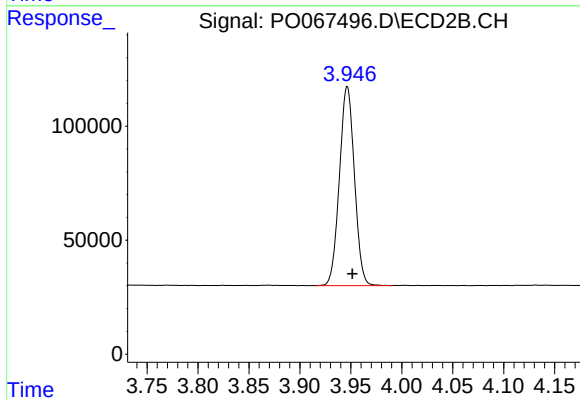


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: -0.005 min
Response: 894819
Conc: 25.60 ng/ml m

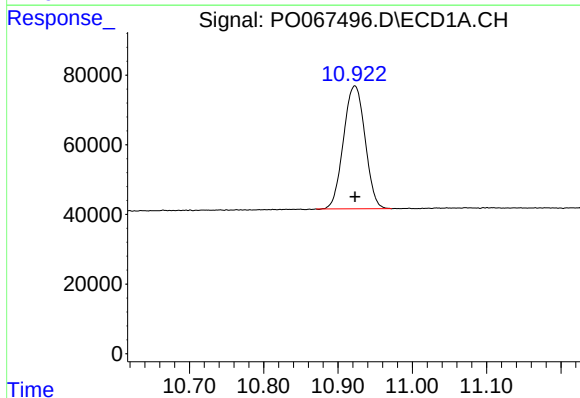

#2 Decachlorobiphenyl

R.T.: 10.923 min
Delta R.T.: 0.000 min
Response: 711862
Conc: 24.78 ng/ml

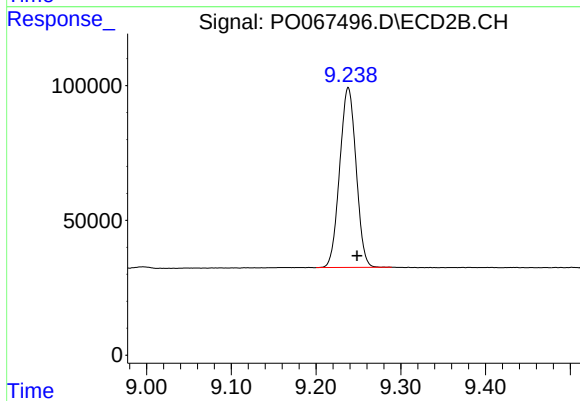

#2 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: -0.010 min
Response: 897284
Conc: 23.00 ng/ml