

Data Path : P:\HPCHEM1\ECD 0\Data\P0032818\
 Data File : P0043354.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2018 13:27
 Operator : SM/UA
 Sample : J2064-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-CV-2532

Manual Integrations
 APPROVED

UGO
 4/2/2018 10:47:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 16:30:27 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 23 05:22:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.076	3.333	2505418	2832580	11.824m	9.677
2) SA Decachlor...	9.426	8.097	2853208	3629171	11.748	10.148

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032818\
Data File : P0043354.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2018 13:27
Operator : SM/UA
Sample : J2064-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-CV-2532


Manual Integrations
APPROVED

UGO
4/2/2018 10:47:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 16:30:27 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

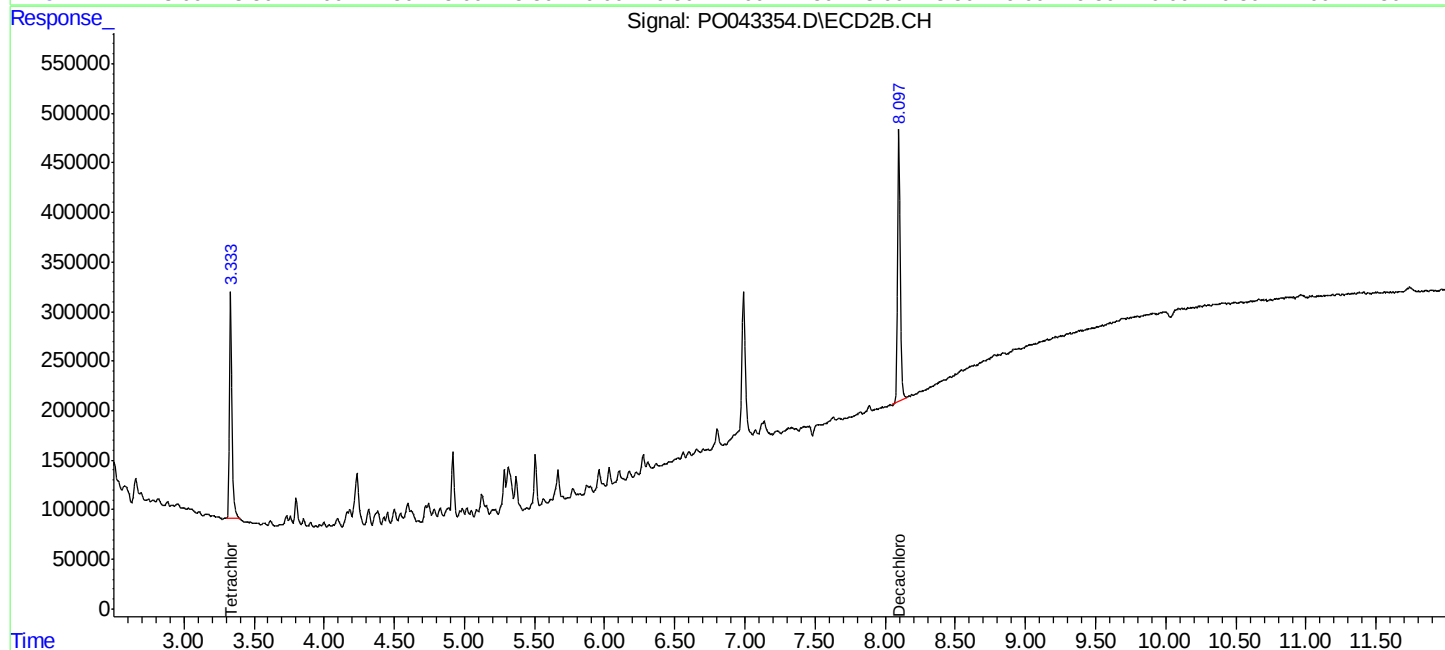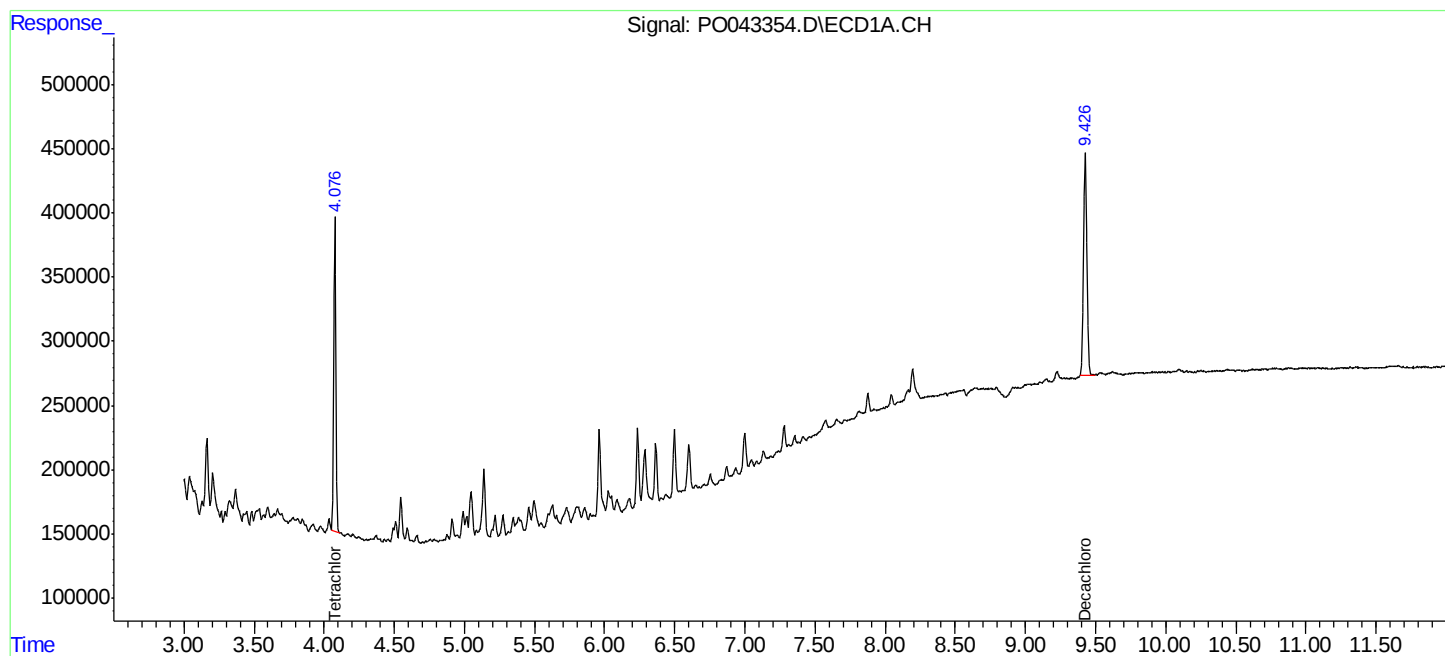

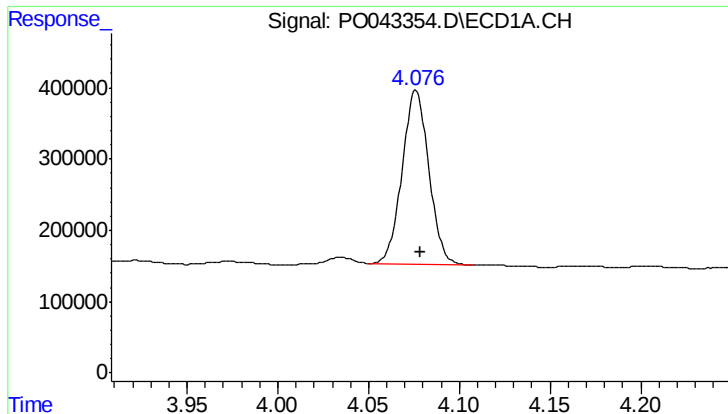


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.003 min
Response: 2505418
Conc: 11.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-CV-2532


Manual Integrations
APPROVED

UGO
4/2/2018 10:47:14 AM

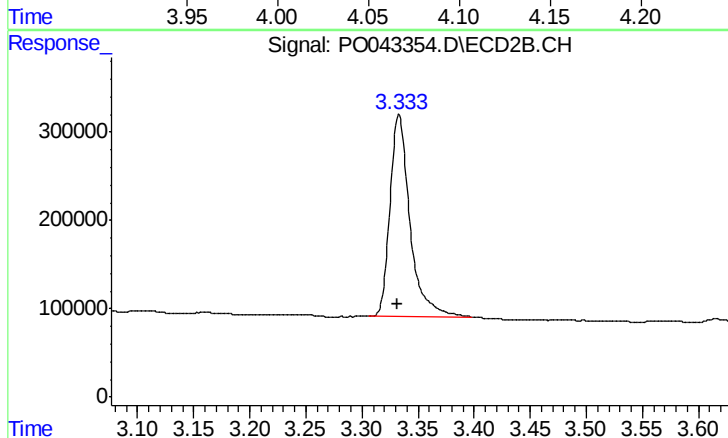


#1 Tetrachloro-m-xylene

R.T.: 3.333 min
Delta R.T.: 0.000 min
Response: 2832580
Conc: 9.68 ng/ml

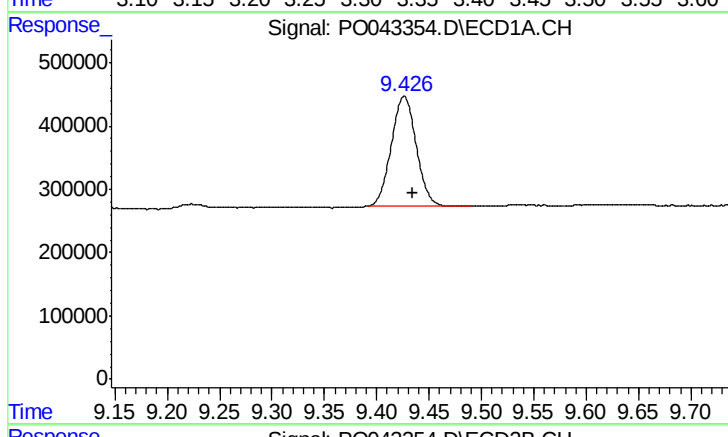

#2 Decachlorobiphenyl

R.T.: 9.426 min
Delta R.T.: -0.009 min
Response: 2853208
Conc: 11.75 ng/ml

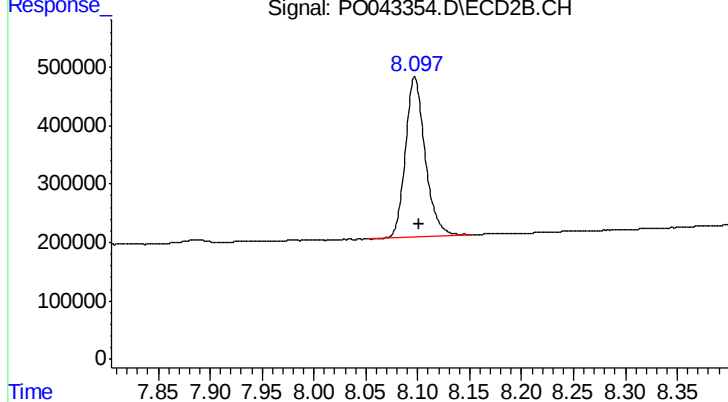

#2 Decachlorobiphenyl

R.T.: 8.097 min
Delta R.T.: -0.005 min
Response: 3629171
Conc: 10.15 ng/ml