

Data Path : P:\HPCHEM1\ECD 0\Data\P0032818\
Data File : P0043359.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2018 15:35
Operator : SM/UA
Sample : J2066-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RO-CV-2036

Manual Integrations
APPROVED

UGO
4/2/2018 10:47:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 10:33:51 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.075	3.331	3695936	4354895	17.442	14.878
2) SA Decachlor...	9.425	8.096	5440521	6707802	22.401	18.757

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032818\
Data File : P0043359.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2018 15:35
Operator : SM/UA
Sample : J2066-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-CV-2036


Manual Integrations
APPROVED

UGO
4/2/2018 10:47:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 10:33:51 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

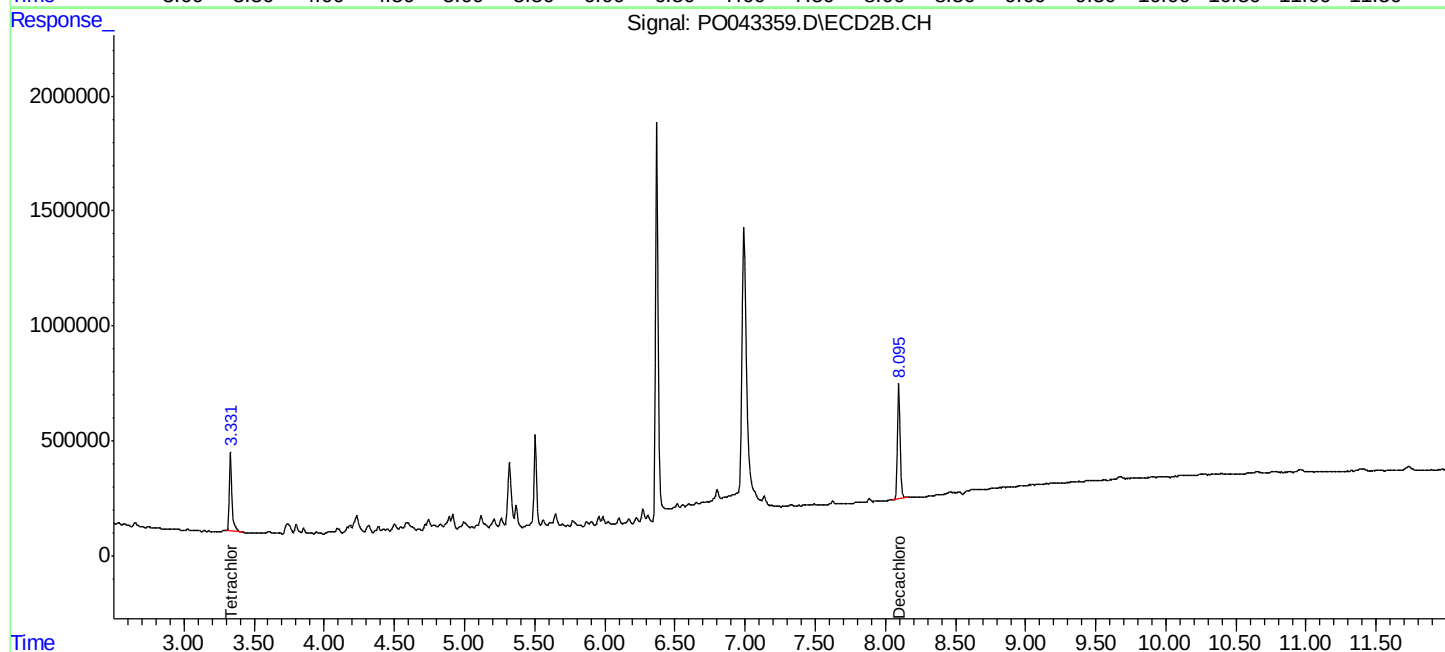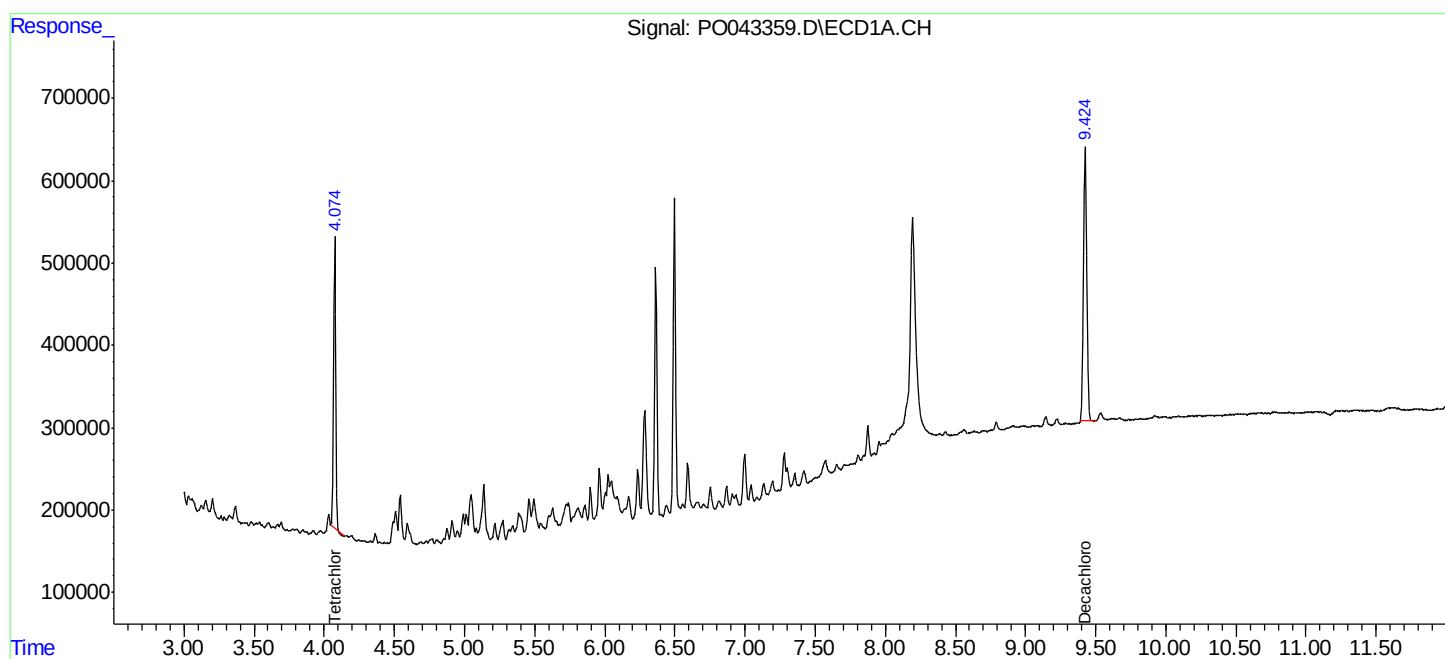

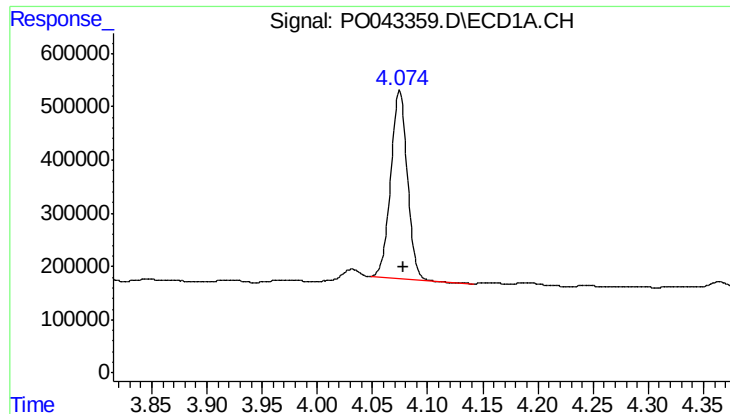


#1 Tetrachloro-m-xylene

R.T.: 4.075 min
Delta R.T.: -0.004 min
Response: 3695936
Conc: 17.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-CV-2036


Manual Integrations
APPROVED

UGO
4/2/2018 10:47:24 AM

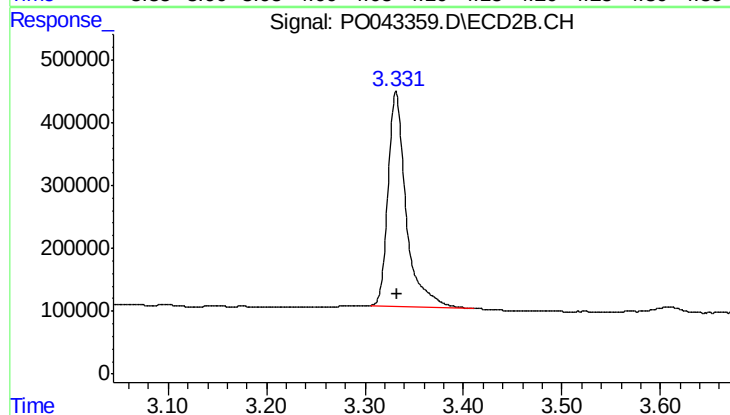


#1 Tetrachloro-m-xylene

R.T.: 3.331 min
Delta R.T.: 0.000 min
Response: 4354895
Conc: 14.88 ng/ml

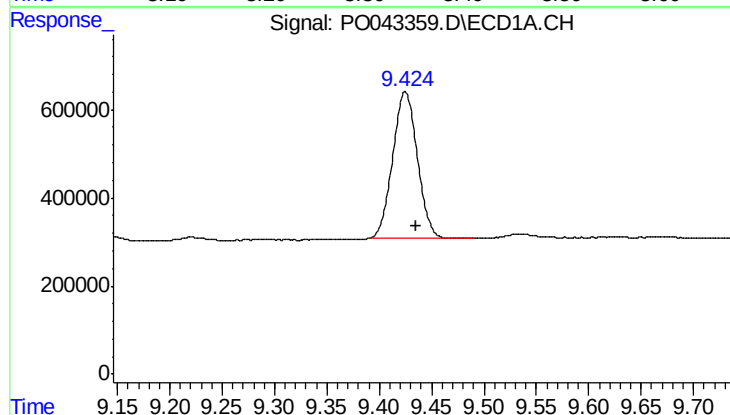

#2 Decachlorobiphenyl

R.T.: 9.425 min
Delta R.T.: -0.010 min
Response: 5440521
Conc: 22.40 ng/ml

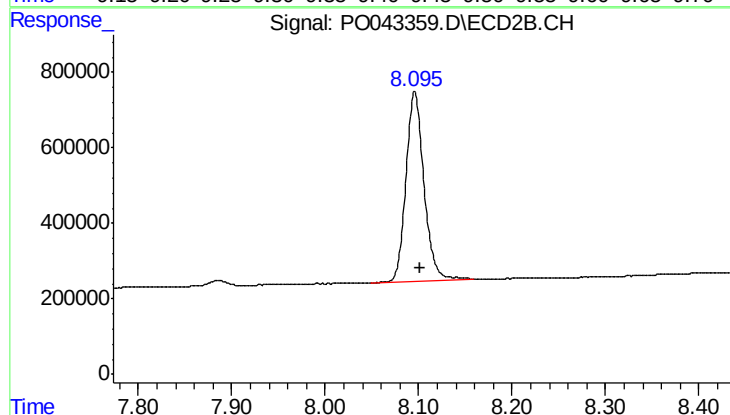

#2 Decachlorobiphenyl

R.T.: 8.096 min
Delta R.T.: -0.006 min
Response: 6707802
Conc: 18.76 ng/ml