

Data Path : P:\HPCHEM1\ECD 0\Data\P0032818\
Data File : P0043366.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2018 18:04
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

UGO
4/2/2018 10:47:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 04:02:52 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.072	3.328	6280486	8174360	29.639m	27.928
2) SA Decachlor...	9.422	8.095	6947791	8986400	28.607m	25.128

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032818\
Data File : P0043366.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2018 18:04
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

UGO
4/2/2018 10:47:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 04:02:52 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

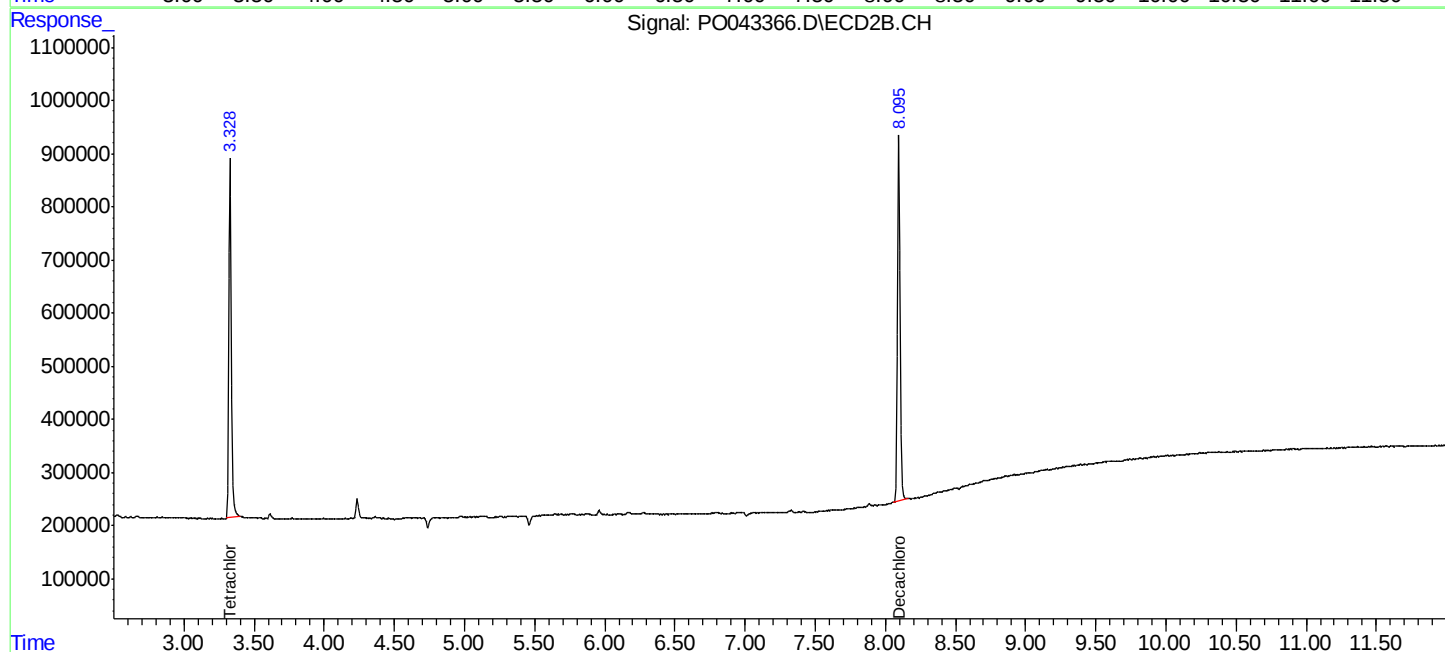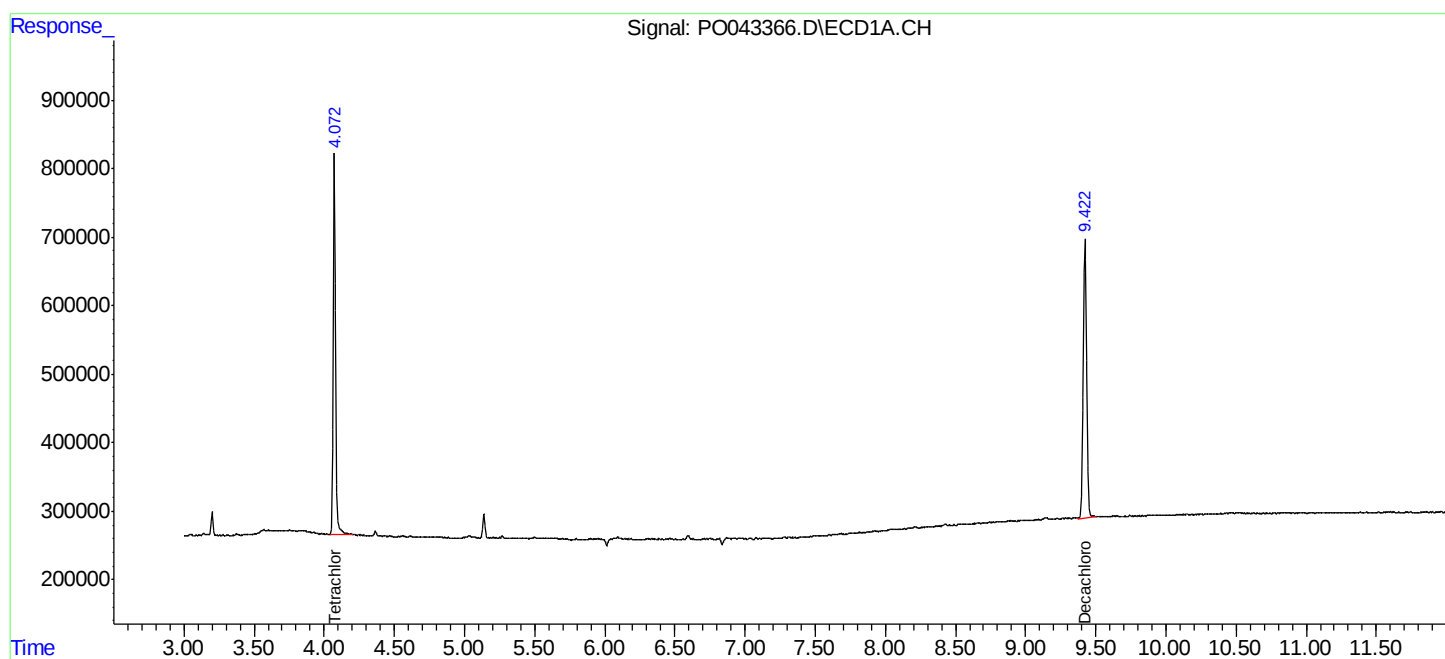

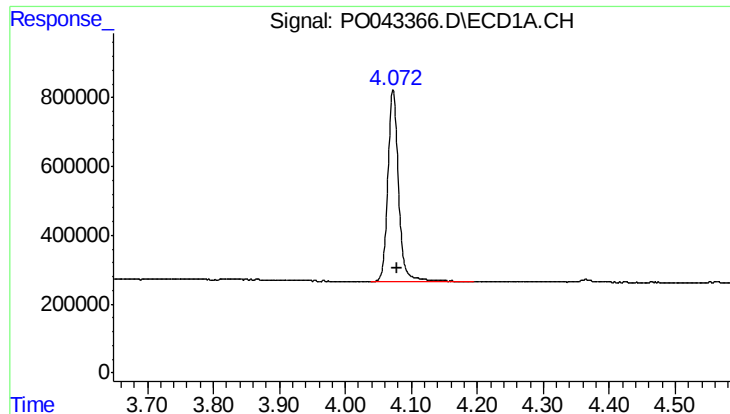


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: -0.006 min
Response: 6280486
Conc: 29.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

UGO
4/2/2018 10:47:46 AM

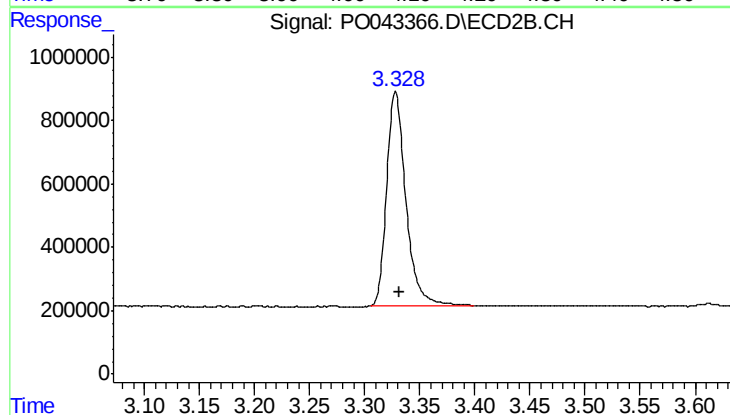


#1 Tetrachloro-m-xylene

R.T.: 3.328 min
Delta R.T.: -0.004 min
Response: 8174360
Conc: 27.93 ng/ml

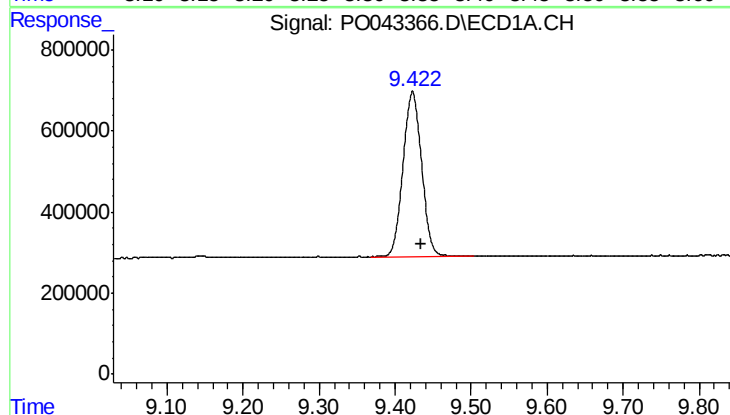

#2 Decachlorobiphenyl

R.T.: 9.422 min
Delta R.T.: -0.013 min
Response: 6947791
Conc: 28.61 ng/ml m

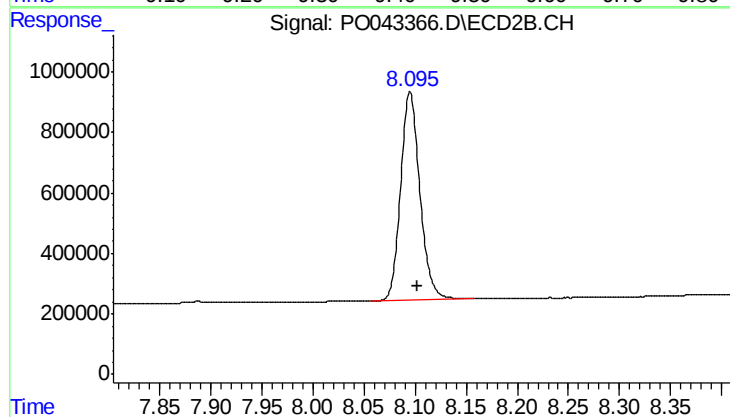

#2 Decachlorobiphenyl

R.T.: 8.095 min
Delta R.T.: -0.007 min
Response: 8986400
Conc: 25.13 ng/ml