

Data Path : P:\HPCHEM1\ECD 0\Data\P0032918\
Data File : P0043373.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2018 9:18
Operator : SM/UA
Sample : J2067-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RO-CV-RB47185RT

Manual Integrations
APPROVED

UGO
3/30/2018 11:28:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 10:50:35 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.081	3.343	2840387	3061942	13.405m	10.461m
2) SA Decachlor...	9.427	8.097	1913200	2476190	7.878	6.924m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032918\
Data File : P0043373.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2018 9:18
Operator : SM/UA
Sample : J2067-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-CV-RB47185RT


Manual Integrations
APPROVED

UGO
3/30/2018 11:28:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 10:50:35 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

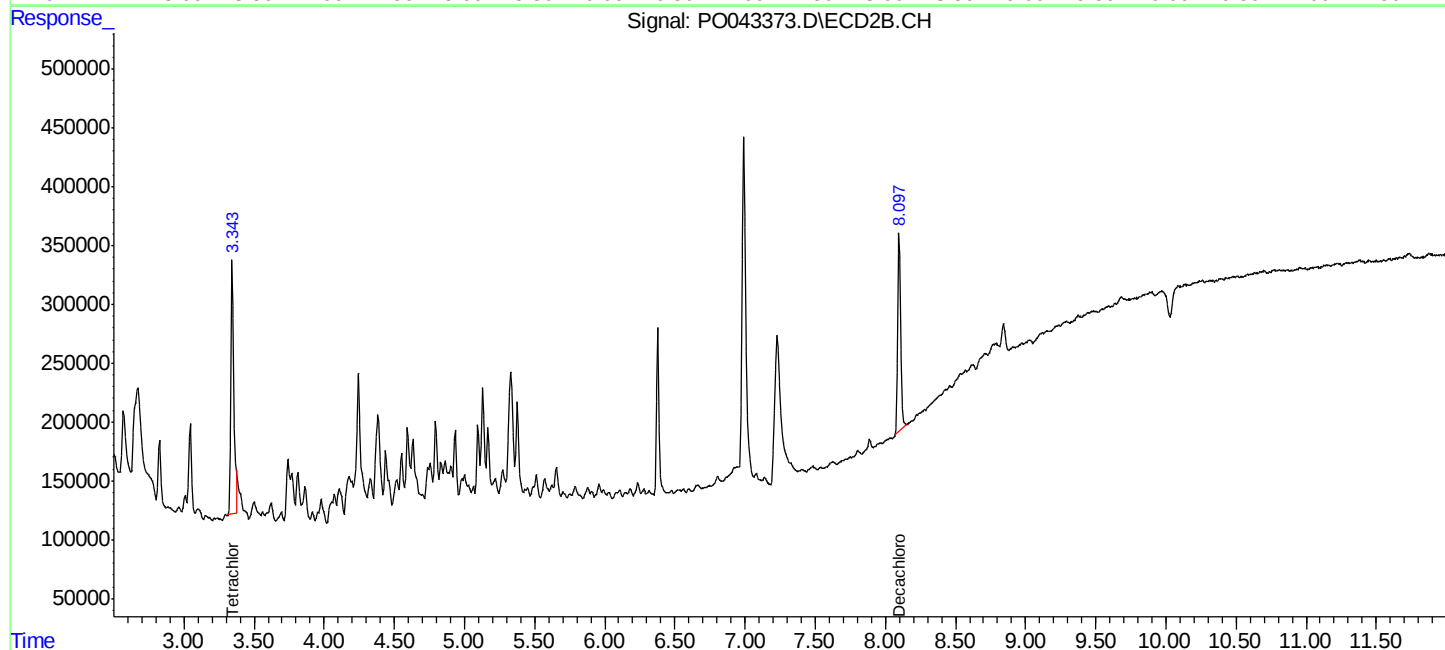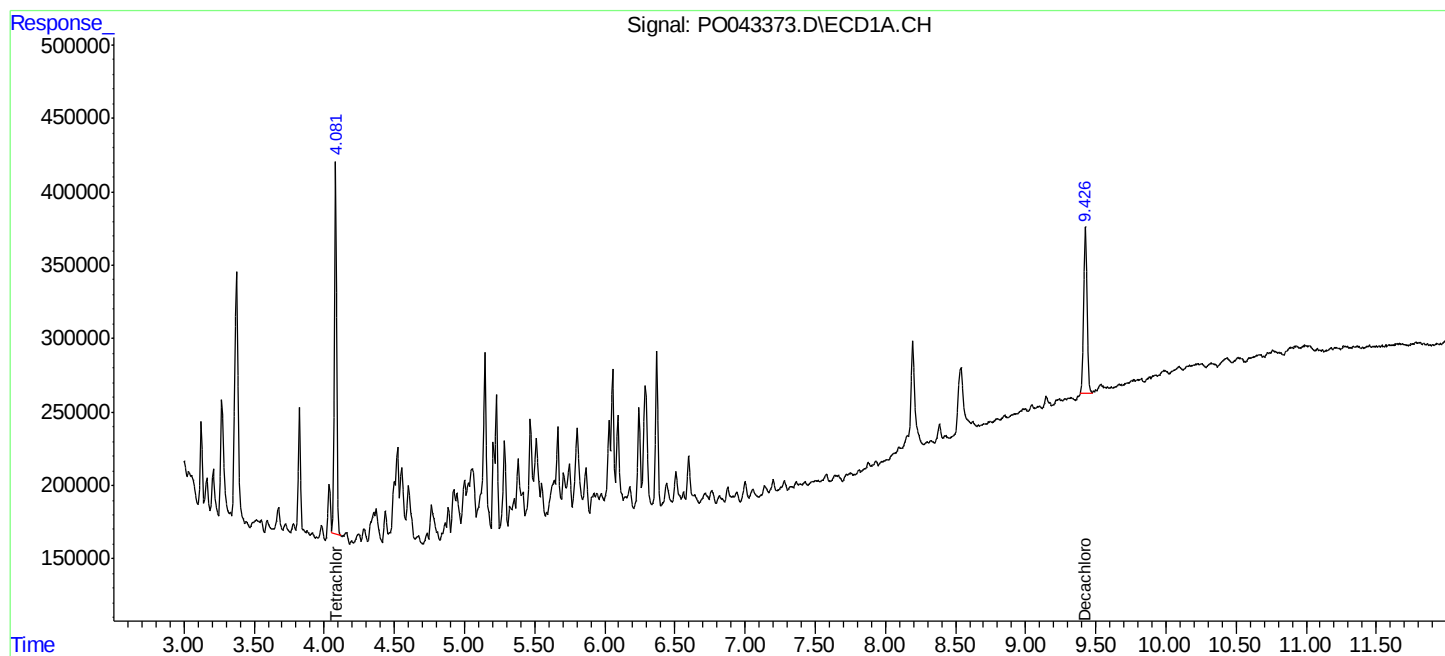

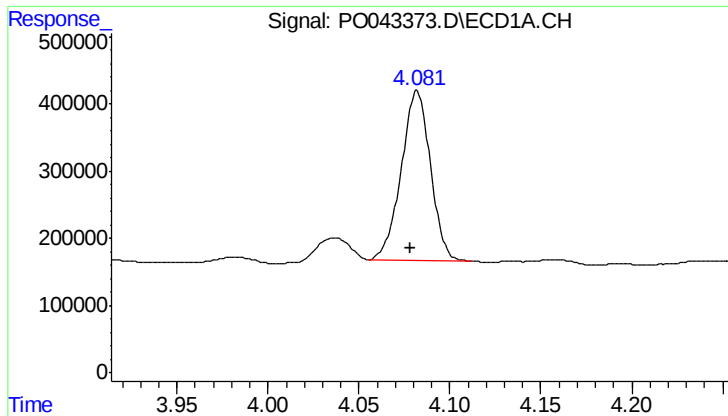


#1 Tetrachloro-m-xylene

R.T.: 4.081 min
Delta R.T.: 0.003 min
Response: 2840387
Conc: 13.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-CV-RB47185RT


Manual Integrations
APPROVED

UGO
3/30/2018 11:28:25 AM

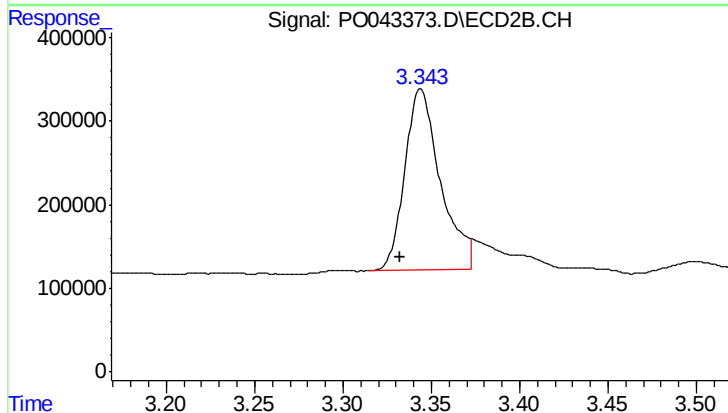


#1 Tetrachloro-m-xylene

R.T.: 3.343 min
Delta R.T.: 0.011 min
Response: 3061942
Conc: 10.46 ng/ml m

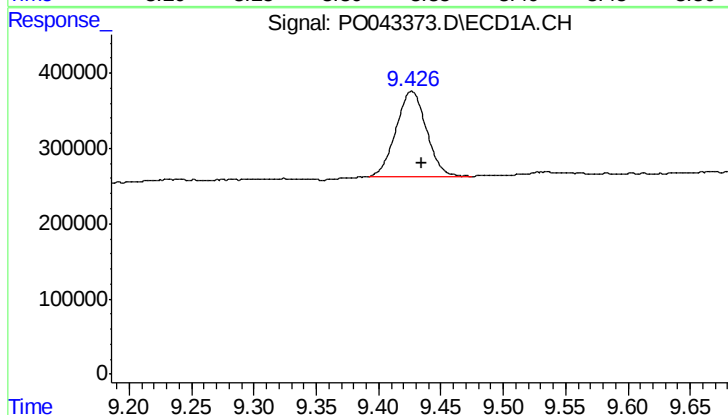

#2 Decachlorobiphenyl

R.T.: 9.427 min
Delta R.T.: -0.008 min
Response: 1913200
Conc: 7.88 ng/ml

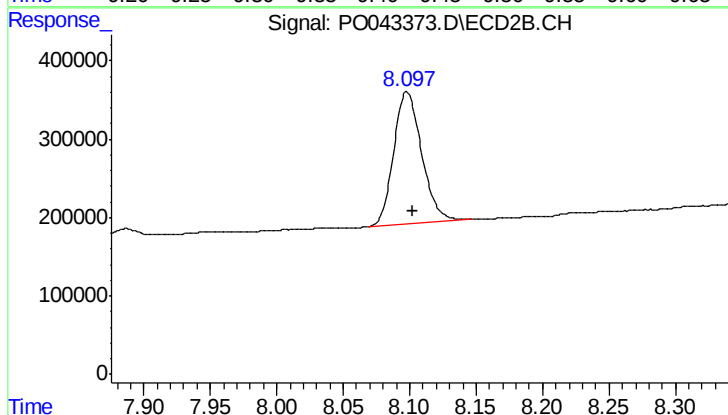

#2 Decachlorobiphenyl

R.T.: 8.097 min
Delta R.T.: -0.005 min
Response: 2476190
Conc: 6.92 ng/ml m