

Data Path : P:\HPCHEM1\ECD 0\Data\P0032918\
 Data File : P0043374.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2018 9:34
 Operator : SM/UA
 Sample : J2067-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-CV-RB47185RTRE

Manual Integrations
 APPROVED

UGO
 3/30/2018 11:28:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 10:52:59 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 23 05:22:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.082	3.343	2833569	3116241	13.372m	10.647m
2) SA Decachlor...	9.427	8.100	1830937	2818965	7.539	7.883

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032918\
Data File : P0043374.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2018 9:34
Operator : SM/UA
Sample : J2067-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-CV-RB47185RTRE


Manual Integrations
APPROVED

UGO
3/30/2018 11:28:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 10:52:59 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

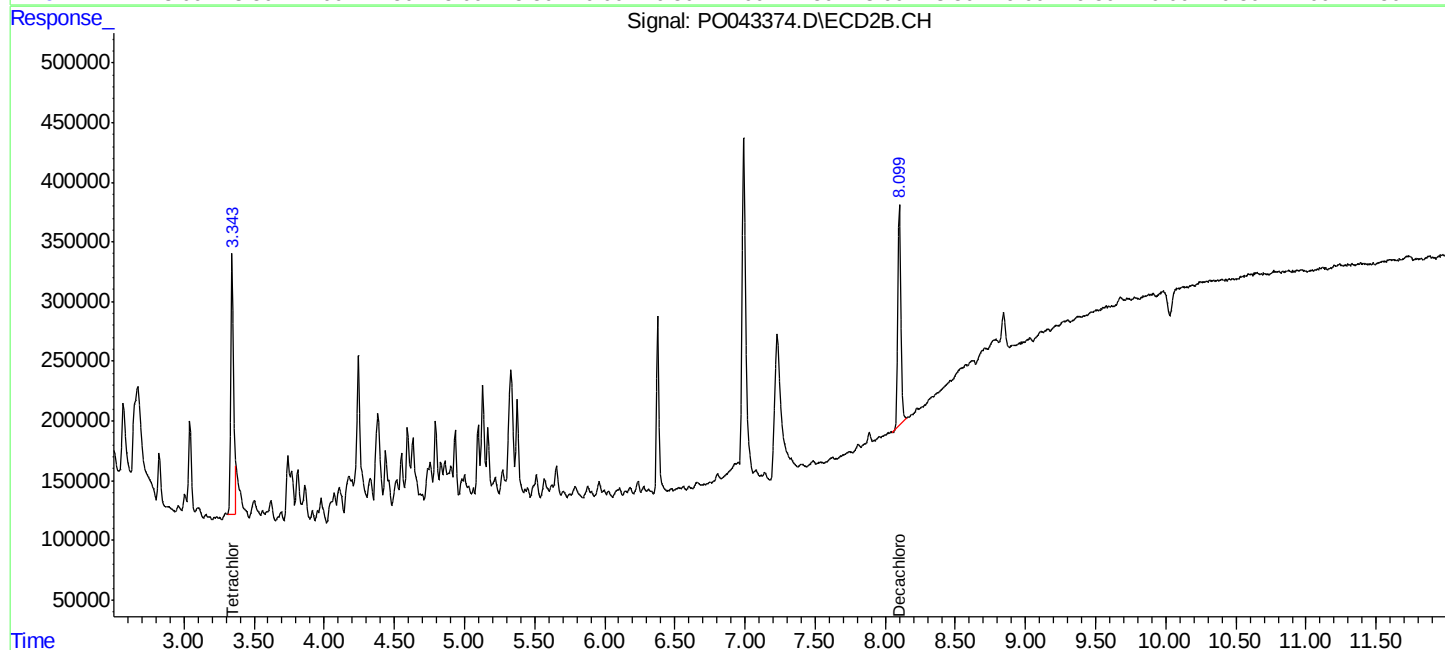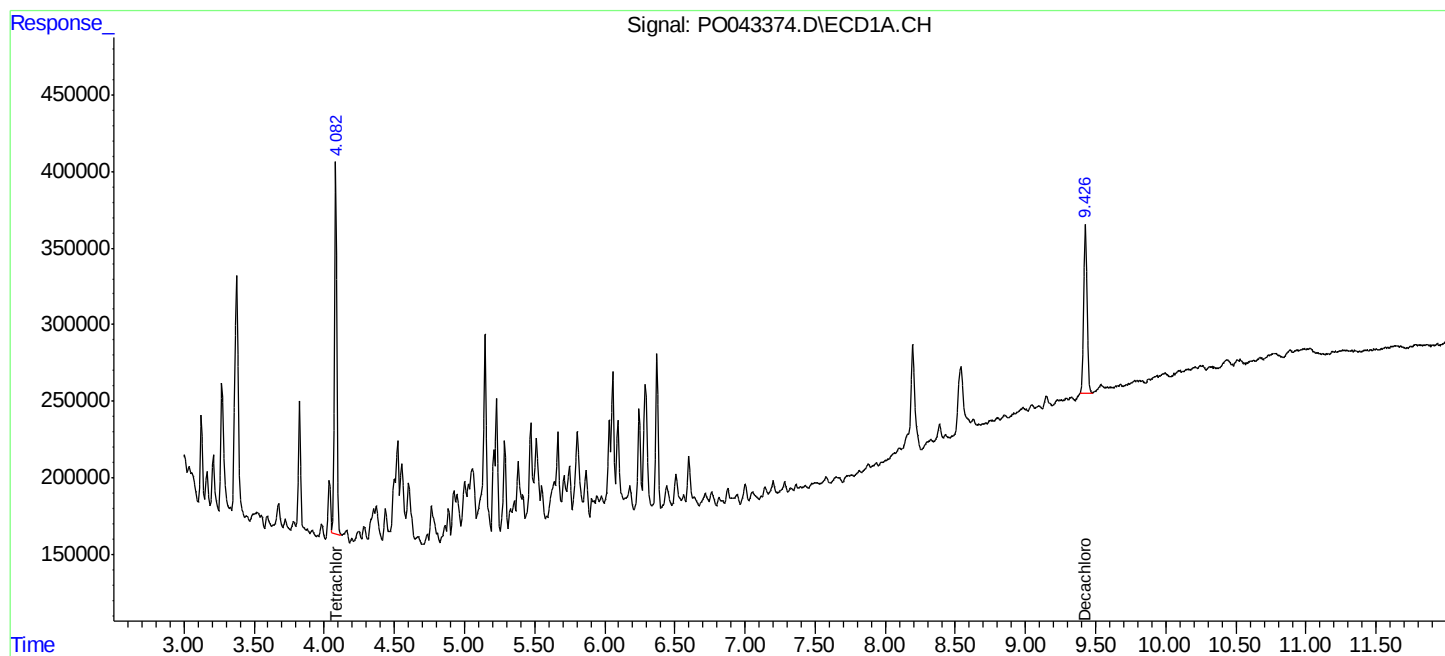

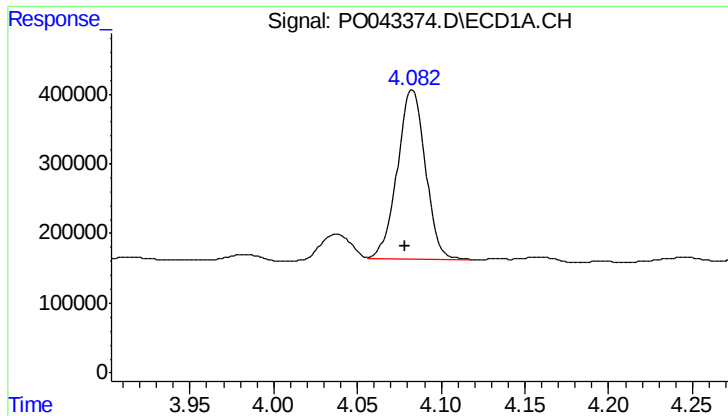


#1 Tetrachloro-m-xylene

R.T.: 4.082 min
Delta R.T.: 0.004 min
Response: 2833569
Conc: 13.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-CV-RB47185RTRE


Manual Integrations
APPROVED

UGO
3/30/2018 11:28:28 AM

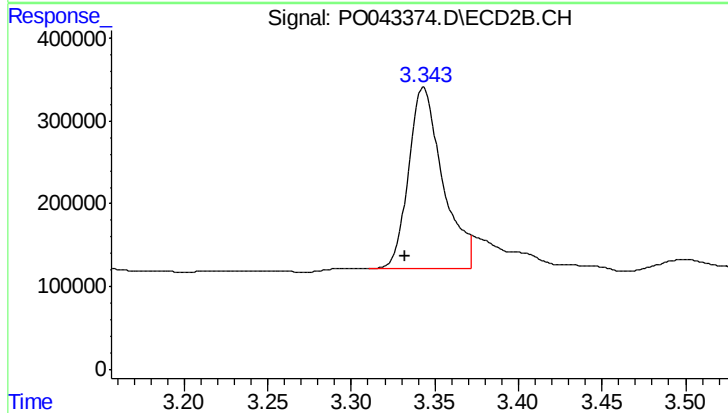


#1 Tetrachloro-m-xylene

R.T.: 3.343 min
Delta R.T.: 0.011 min
Response: 3116241
Conc: 10.65 ng/ml m

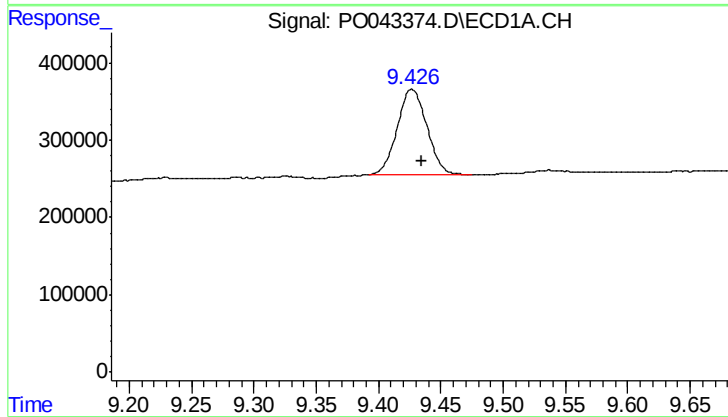

#2 Decachlorobiphenyl

R.T.: 9.427 min
Delta R.T.: -0.008 min
Response: 1830937
Conc: 7.54 ng/ml

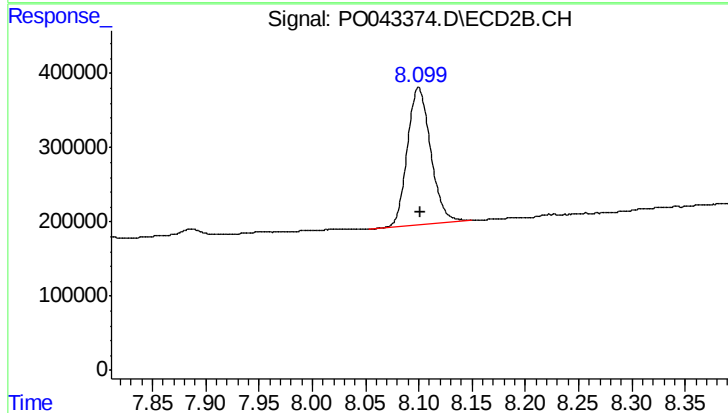

#2 Decachlorobiphenyl

R.T.: 8.100 min
Delta R.T.: -0.002 min
Response: 2818965
Conc: 7.88 ng/ml