

Data Path : P:\HPCHEM1\ECD 0\Data\P0032918\
 Data File : P0043378.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2018 10:34
 Operator : SM/UA
 Sample : J2062-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 19643

Manual Integrations
 APPROVED

UGO
 3/30/2018 11:27:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 11:45:50 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 23 05:22:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.073	3.329	4423603	6015193	20.876	20.551m
2) SA Decachlor...	9.423	8.094	3871824	4764073	15.942m	13.322

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032918\
Data File : P0043378.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2018 10:34
Operator : SM/UA
Sample : J2062-10
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
19643


Manual Integrations
APPROVED

UGO
3/30/2018 11:27:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 11:45:50 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

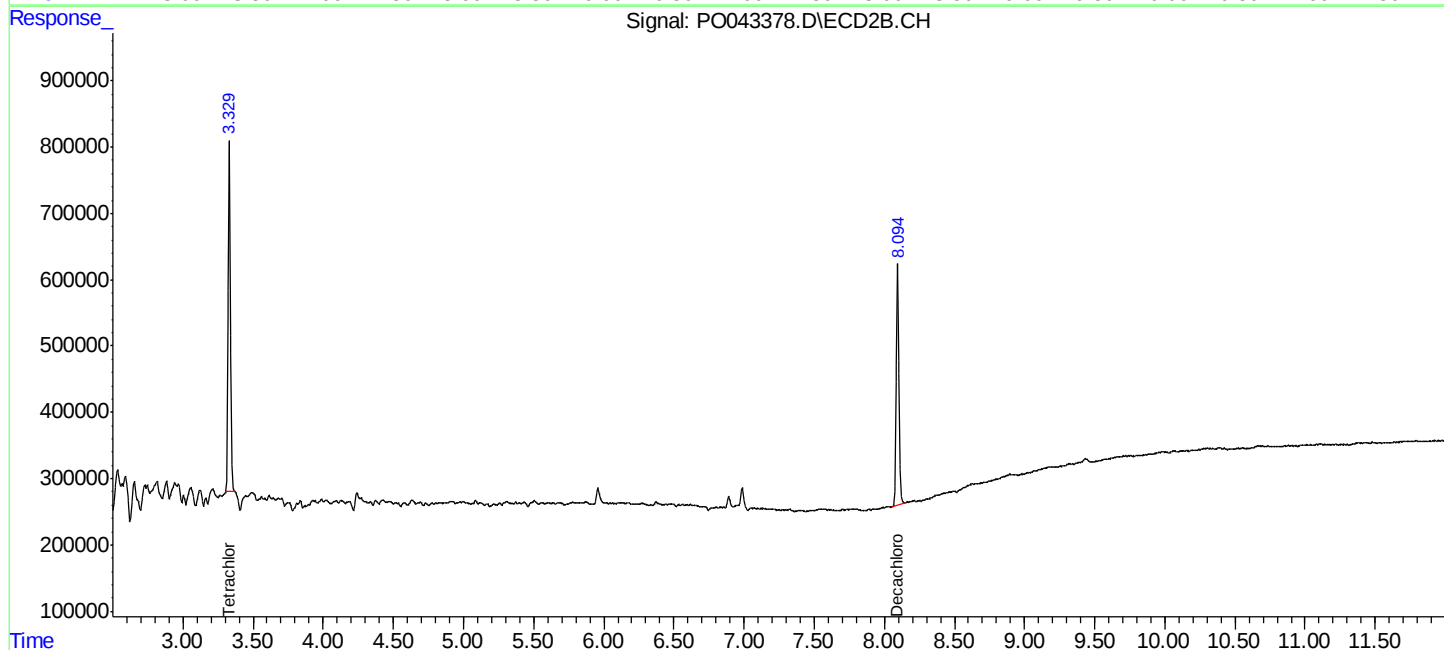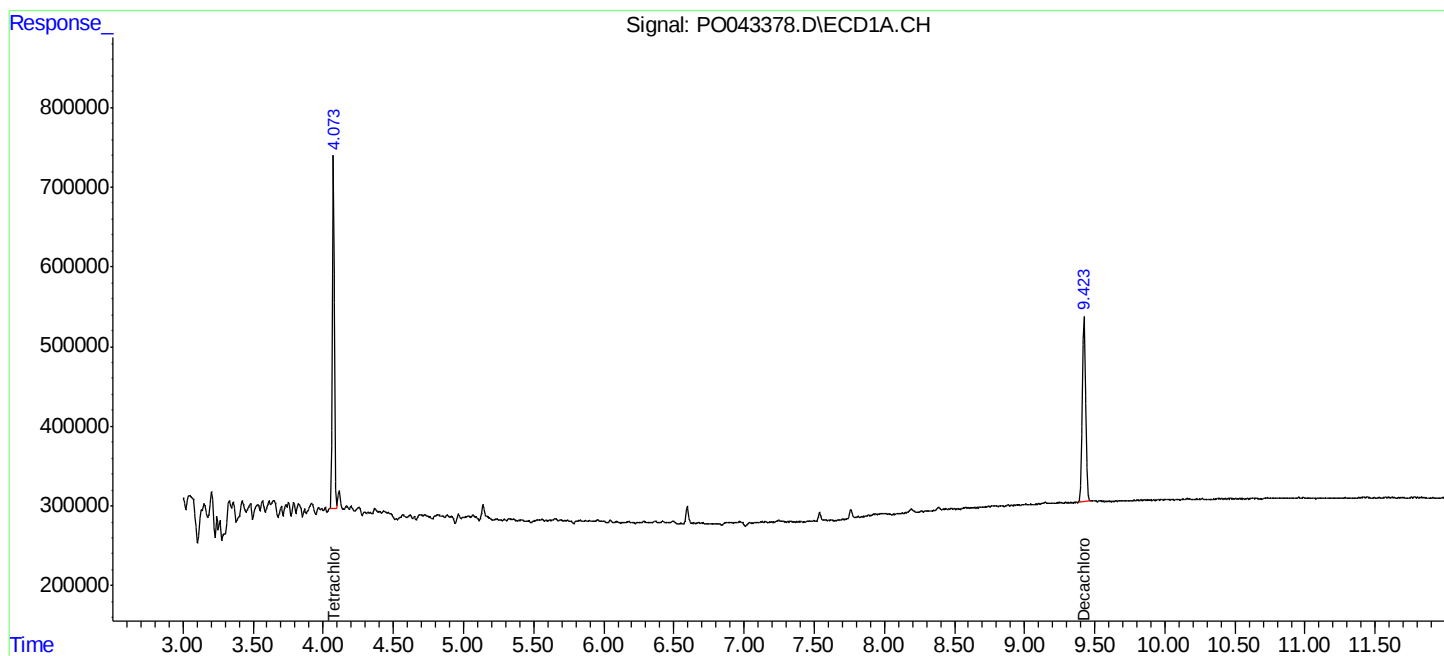

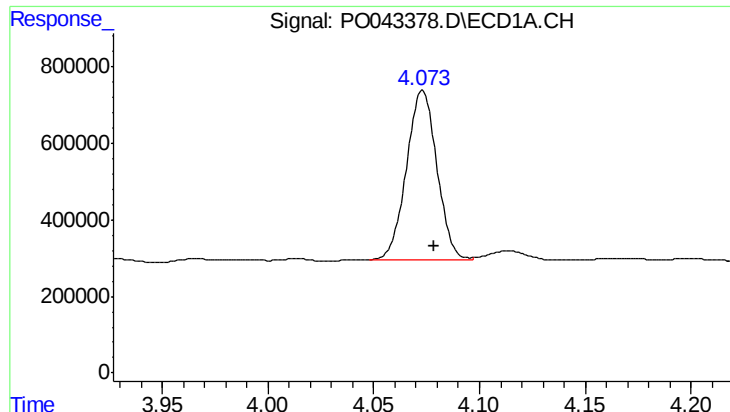


#1 Tetrachloro-m-xylene

R.T.: 4.073 min
Delta R.T.: -0.005 min
Response: 4423603
Conc: 20.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
19643


Manual Integrations
APPROVED

UGO
3/30/2018 11:27:54 AM

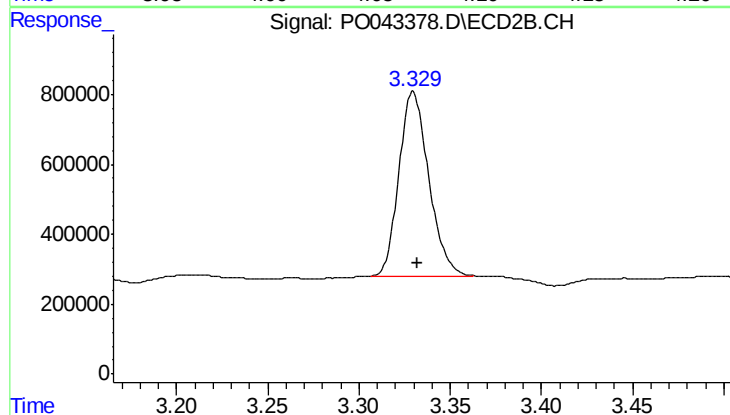


#1 Tetrachloro-m-xylene

R.T.: 3.329 min
Delta R.T.: -0.003 min
Response: 6015193
Conc: 20.55 ng/ml m

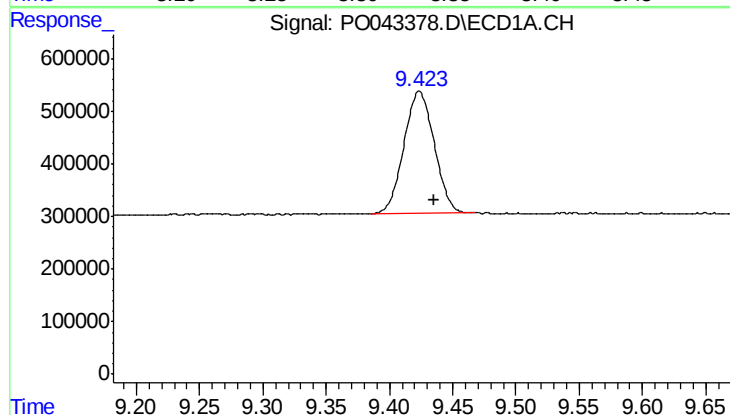

#2 Decachlorobiphenyl

R.T.: 9.423 min
Delta R.T.: -0.012 min
Response: 3871824
Conc: 15.94 ng/ml m

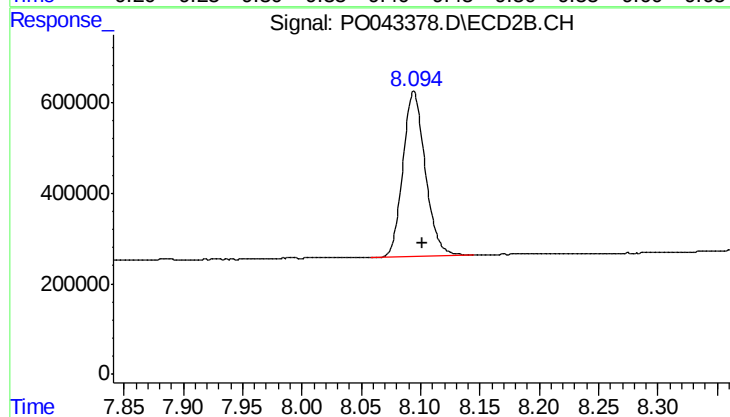

#2 Decachlorobiphenyl

R.T.: 8.094 min
Delta R.T.: -0.008 min
Response: 4764073
Conc: 13.32 ng/ml