

Data Path : P:\HPCHEM1\ECD 0\Data\P0032918\
 Data File : P0043393.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2018 14:40
 Operator : SM/UA
 Sample : J2080-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TEC-RCA-COMP

Manual Integrations
 APPROVED

UGO
 3/30/2018 11:27:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 15:17:09 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 23 05:22:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.081	3.330	4876646	6690070	23.014m	22.857
2) SA Decachlor...	9.436	8.099	3114655	3063492	12.824	8.566 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032918\
Data File : P0043393.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2018 14:40
Operator : SM/UA
Sample : J2080-07
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TEC-RCA-COMP


Manual Integrations
APPROVED

UGO
3/30/2018 11:27:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 15:17:09 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

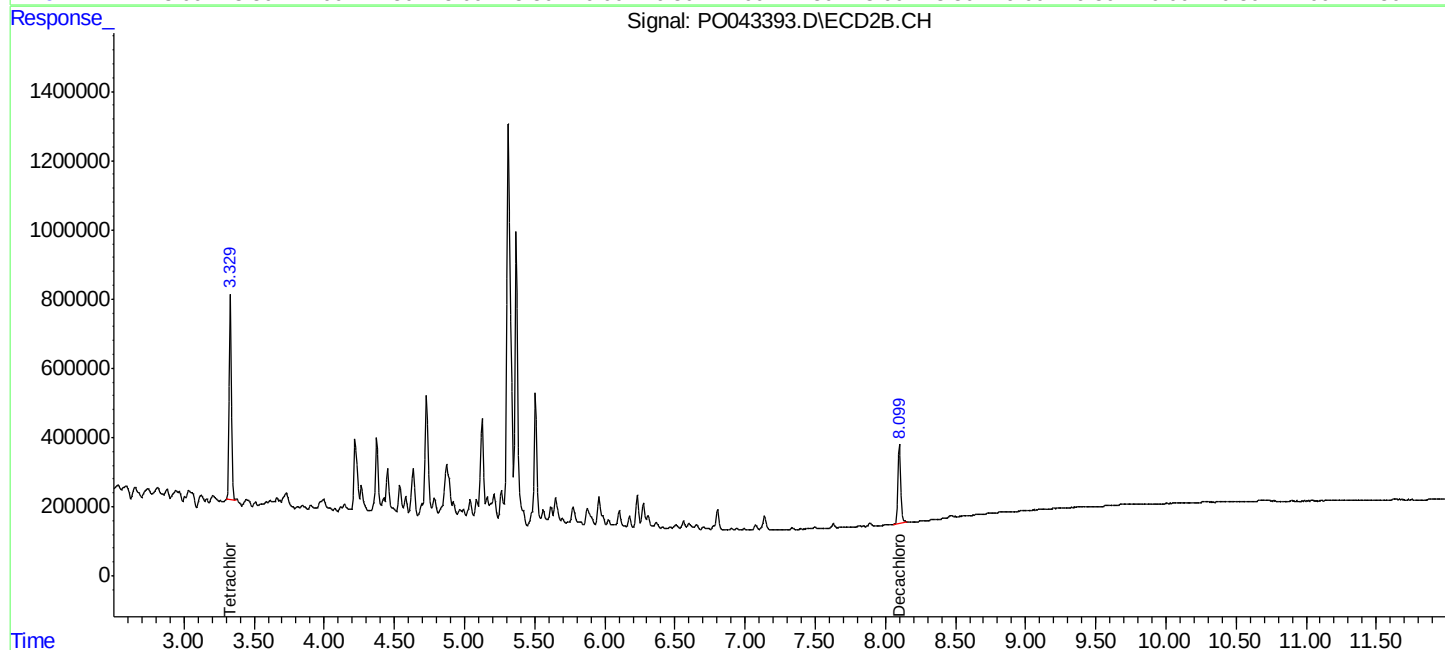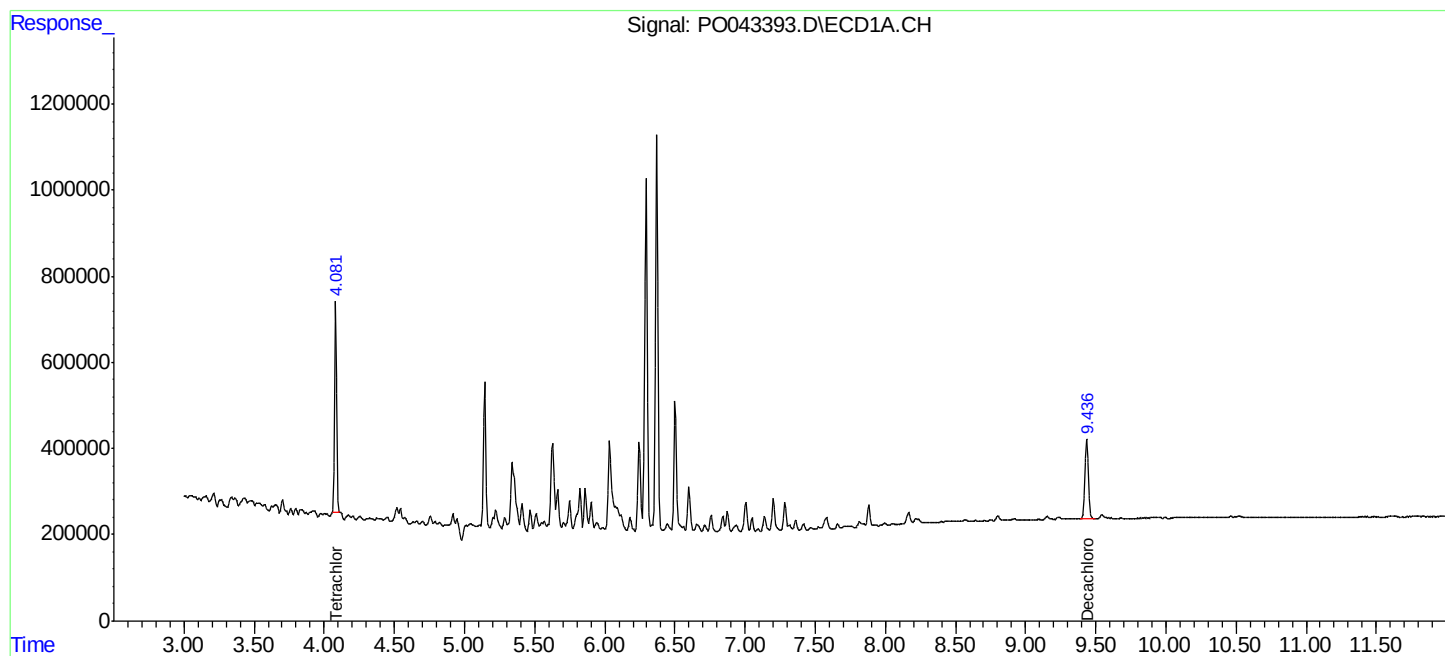

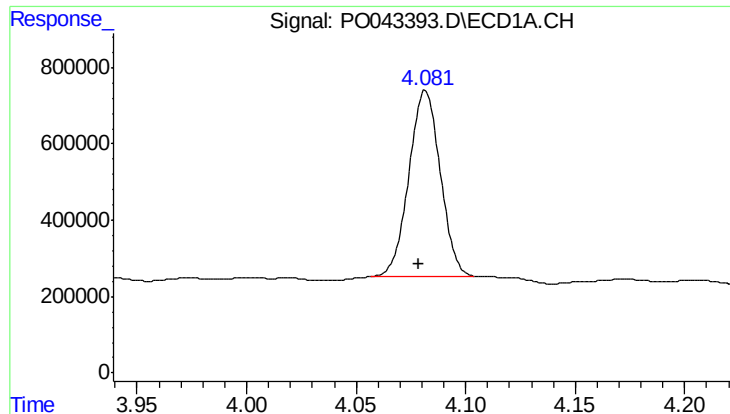


#1 Tetrachloro-m-xylene

R.T.: 4.081 min
Delta R.T.: 0.003 min
Response: 4876646
Conc: 23.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEC-RCA-COMP


Manual Integrations
APPROVED

UGO
3/30/2018 11:27:28 AM

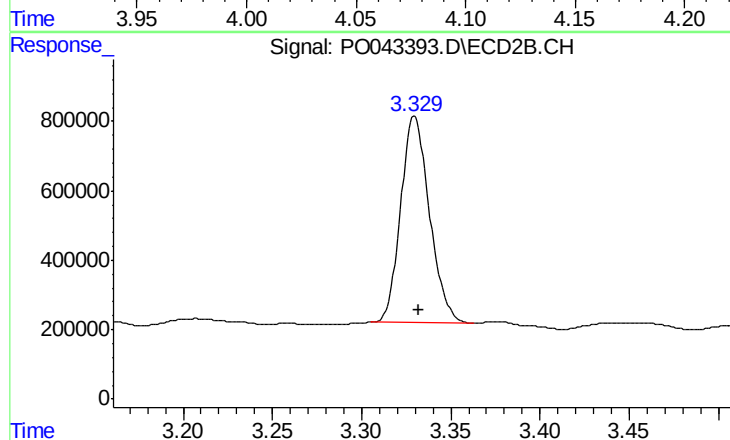


#1 Tetrachloro-m-xylene

R.T.: 3.330 min
Delta R.T.: -0.002 min
Response: 6690070
Conc: 22.86 ng/ml

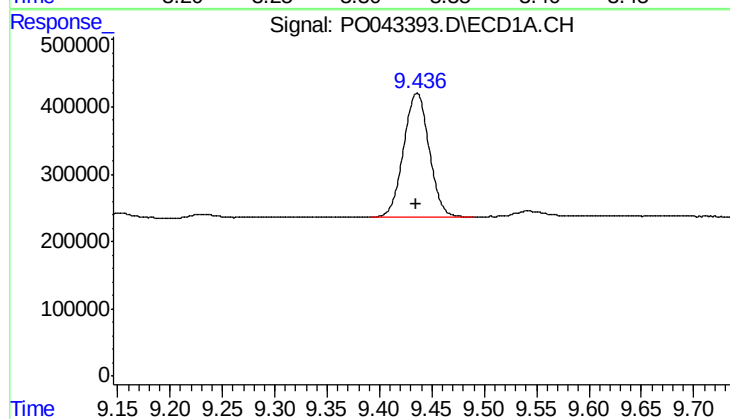

#2 Decachlorobiphenyl

R.T.: 9.436 min
Delta R.T.: 0.000 min
Response: 3114655
Conc: 12.82 ng/ml

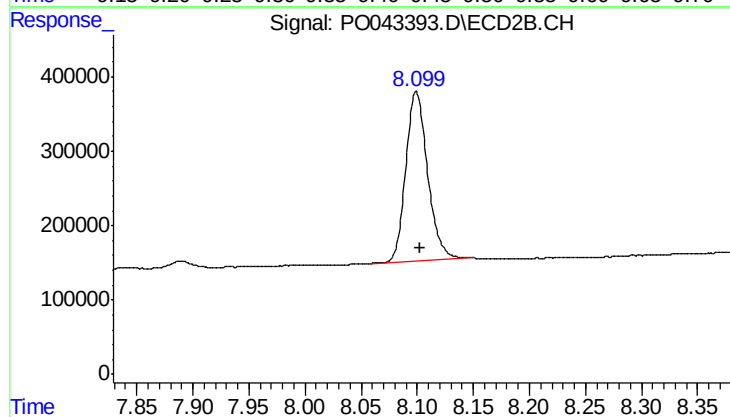

#2 Decachlorobiphenyl

R.T.: 8.099 min
Delta R.T.: -0.003 min
Response: 3063492
Conc: 8.57 ng/ml