

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032919\
Data File : P0054732.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 10:00
Operator : SM/SJ
Sample : K2107-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 10:20:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.304	3.620	494471	486905	14.248	15.258
2) SA Decachlor...	9.924	8.596	660427	474100	13.397	14.886

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032919\
Data File : P0054732.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 10:00
Operator : SM/SJ
Sample : K2107-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 10:20:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

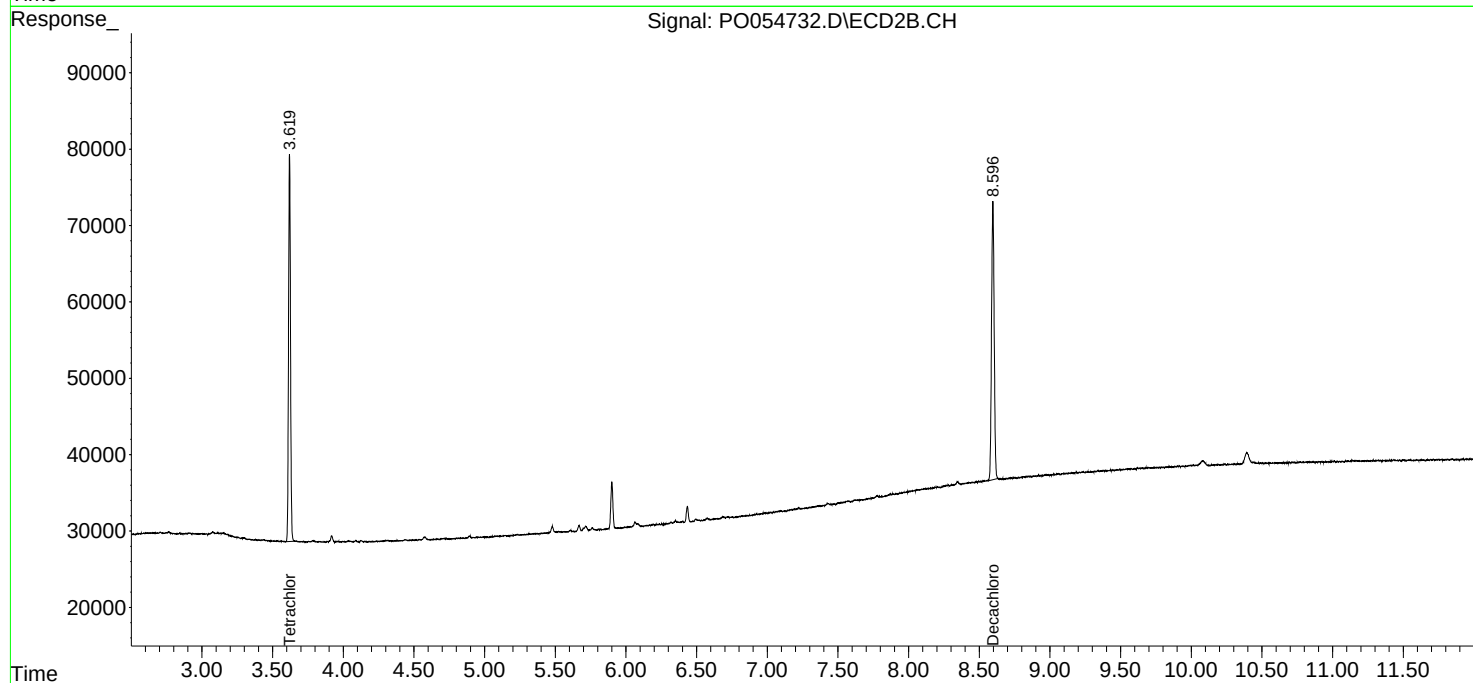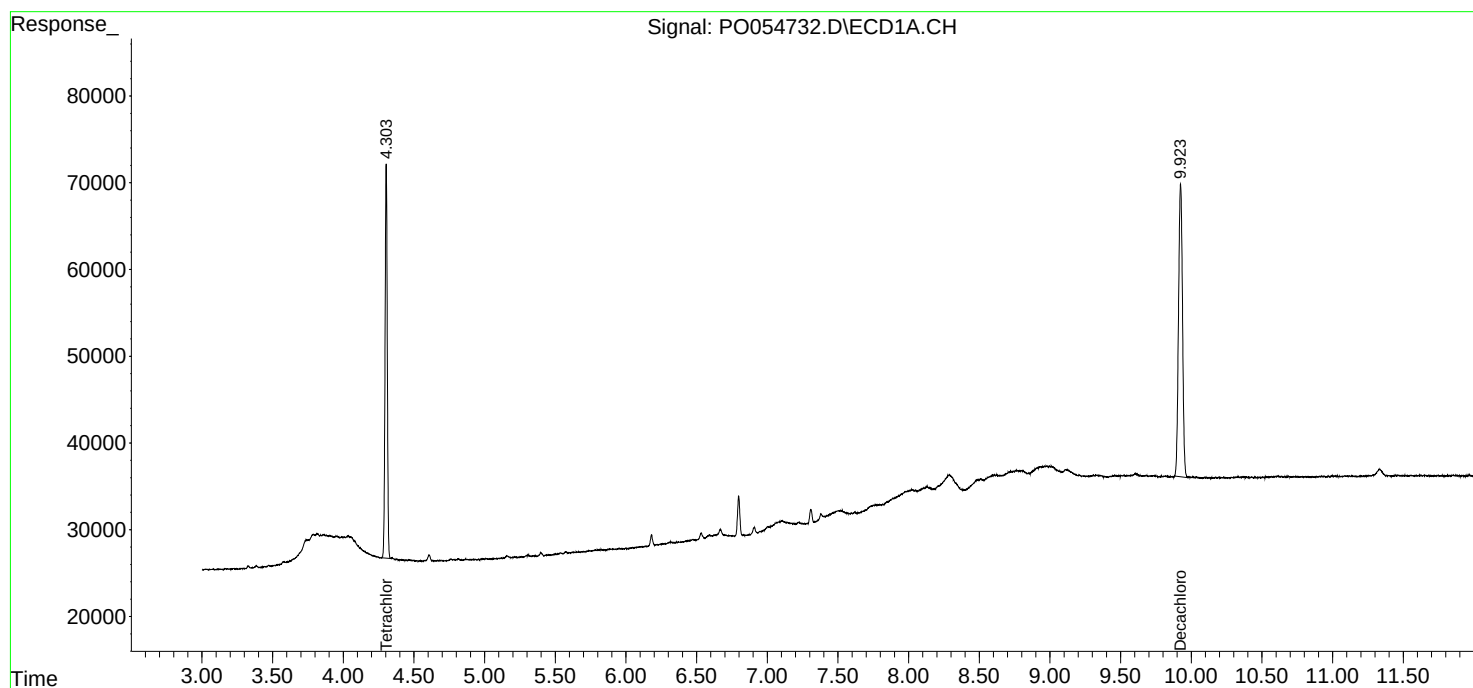


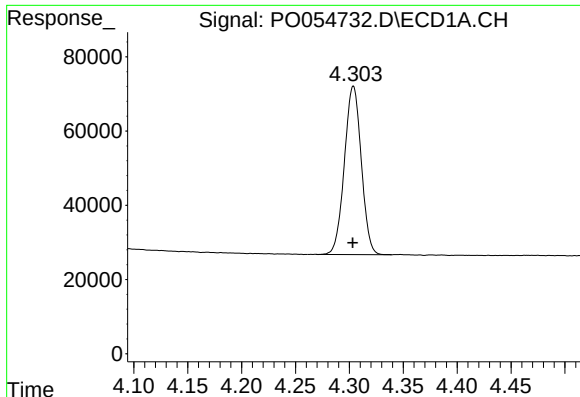

#1 Tetrachloro-m-xylene


R.T.: 4.304 min
Delta R.T.: 0.000 min
Response: 494471
Conc: 14.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4

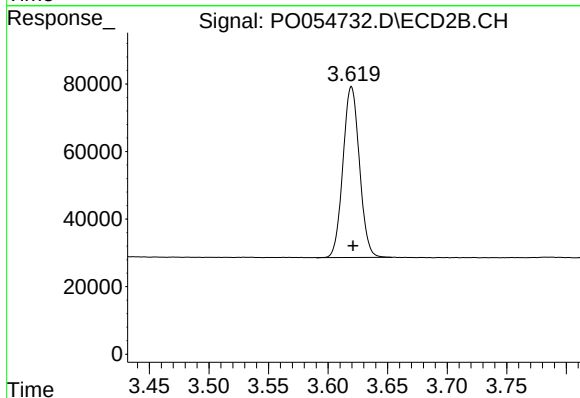


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.001 min
Response: 486905
Conc: 15.26 ng/ml

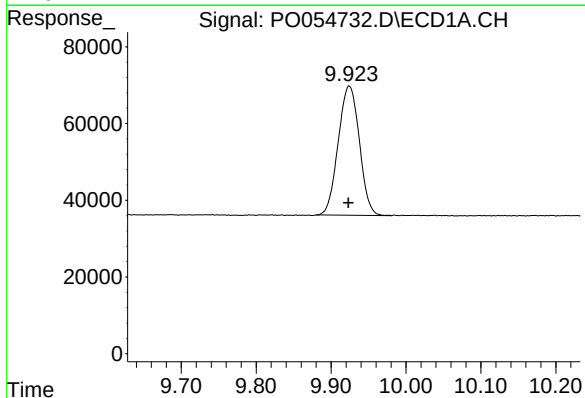

#2 Decachlorobiphenyl

R.T.: 9.924 min
Delta R.T.: 0.000 min
Response: 660427
Conc: 13.40 ng/ml

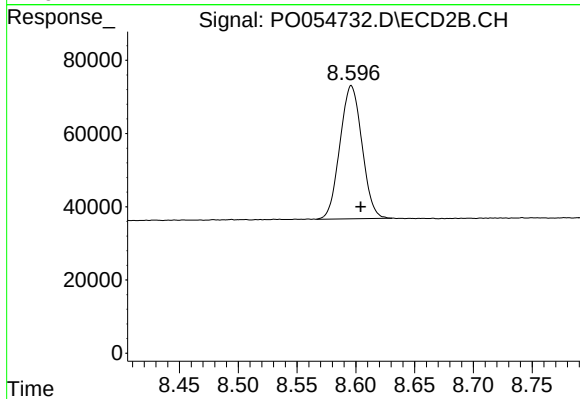

#2 Decachlorobiphenyl

R.T.: 8.596 min
Delta R.T.: -0.008 min
Response: 474100
Conc: 14.89 ng/ml