

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032919\
 Data File : P0054758.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 18:33
 Operator : SM/SJ
 Sample : K2093-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30063-3

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:15:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 03:29:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.303	3.620	781359	728232	22.514m	22.820
2) SA Decachlor...	9.921	8.596	665507	475580	13.500	14.933

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032919\
Data File : P0054758.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 18:33
Operator : SM/SJ
Sample : K2093-15
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
30063-3


Manual Integrations
APPROVED

Sohil
4/1/2019 5:15:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 03:29:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

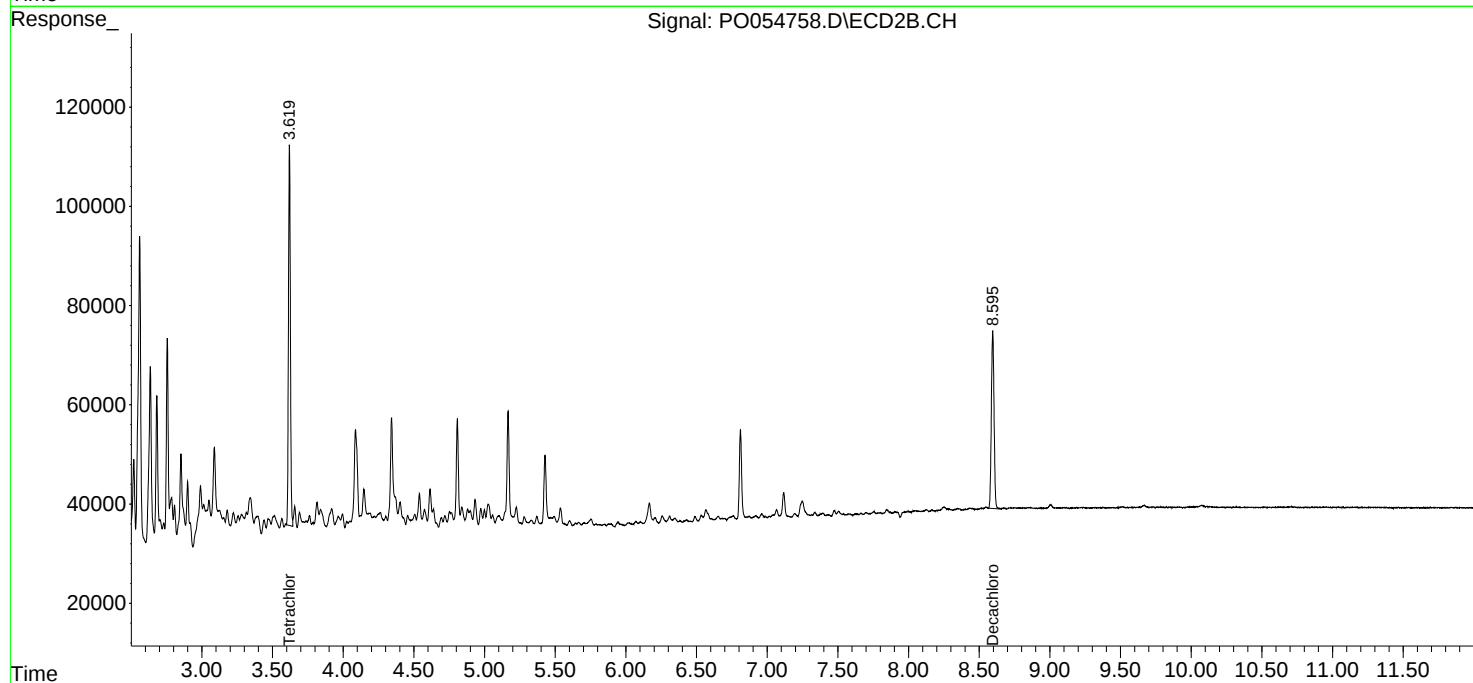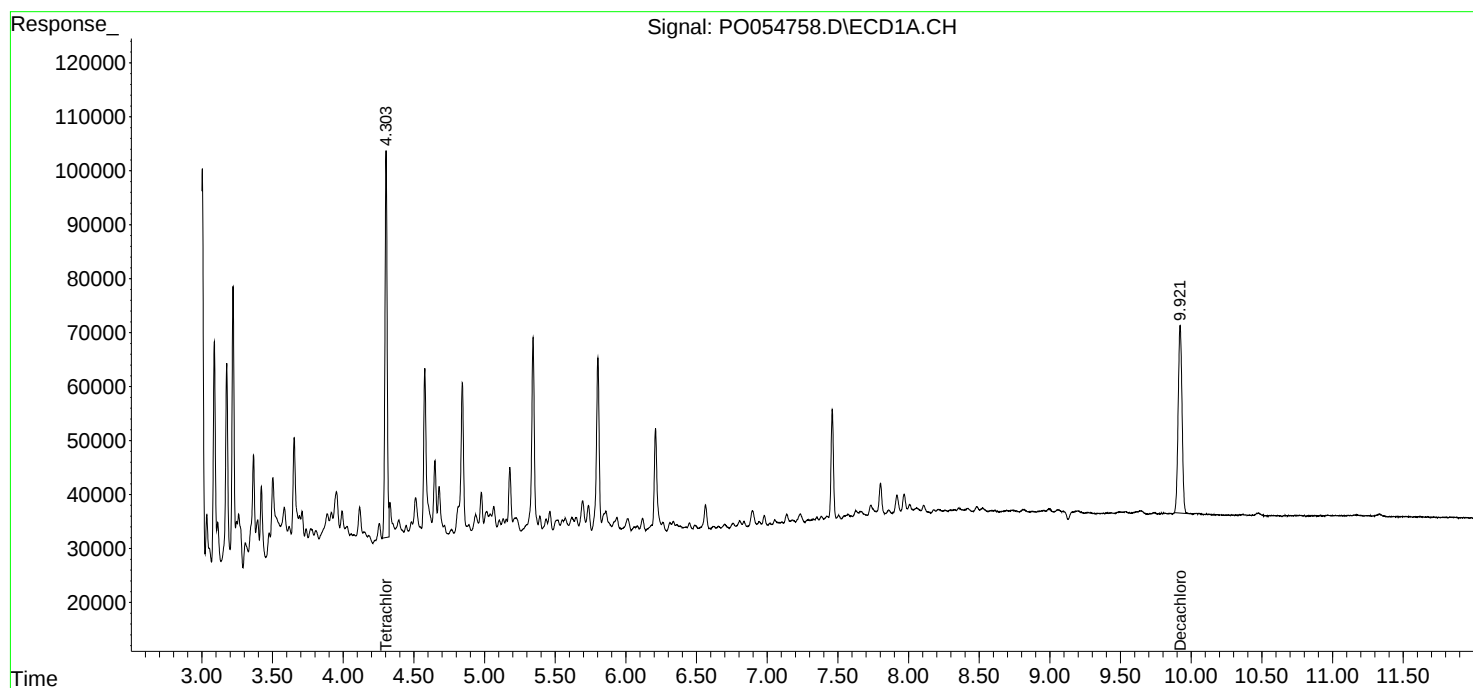

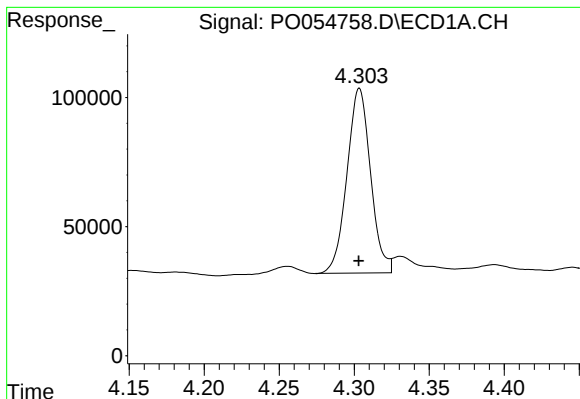


#1 Tetrachloro-m-xylene

R.T.: 4.303 min
Delta R.T.: 0.000 min
Response: 781359
Conc: 22.51 ng/ml m

Instrument :
ECD_O
ClientSampleId :
30063-3


Manual Integrations
APPROVED

Sohil
4/1/2019 5:15:35 PM

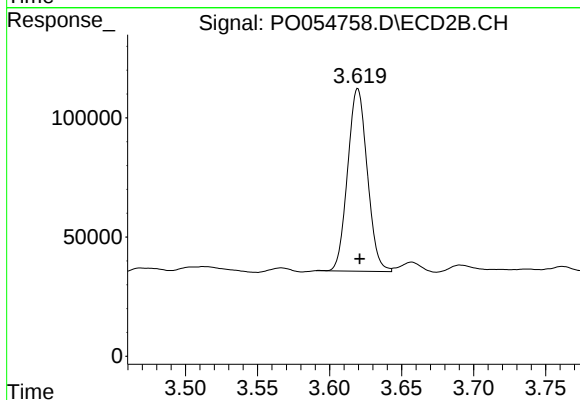


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.001 min
Response: 728232
Conc: 22.82 ng/ml

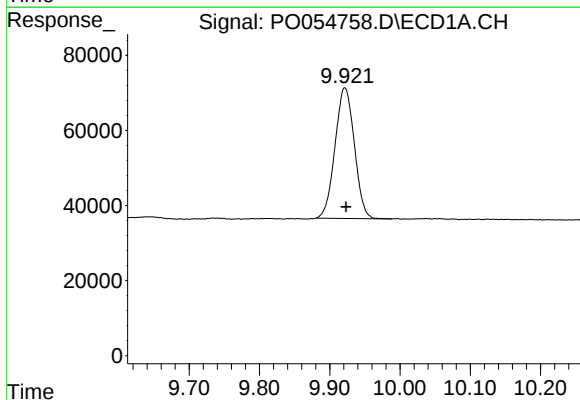

#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.002 min
Response: 665507
Conc: 13.50 ng/ml

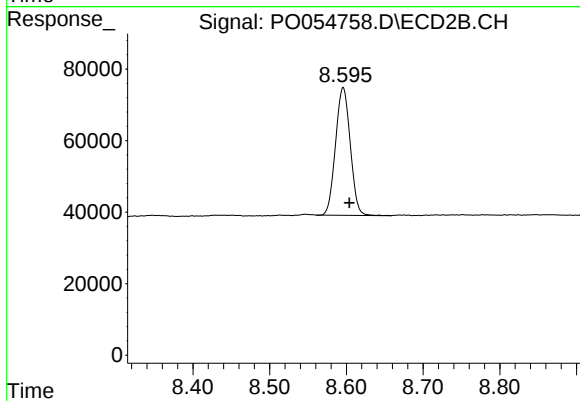

#2 Decachlorobiphenyl

R.T.: 8.596 min
Delta R.T.: -0.008 min
Response: 475580
Conc: 14.93 ng/ml