

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033020\
 Data File : P0067505.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2020 15:22
 Operator : DD\AJ
 Sample : L2049-03 20X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-5-(1-3)

Manual Integrations
 APPROVED

Sohil
 3/31/2020 4:50:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 16:00:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	3.945	28999	48729	1.364m	1.394
2) SA Decachlor...	10.919	9.236	41282	54869	1.437m	1.407

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033020\
Data File : P0067505.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2020 15:22
Operator : DD\AJ
Sample : L2049-03 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-5-(1-3)


Manual Integrations
APPROVED

Sohil
3/31/2020 4:50:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 16:00:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

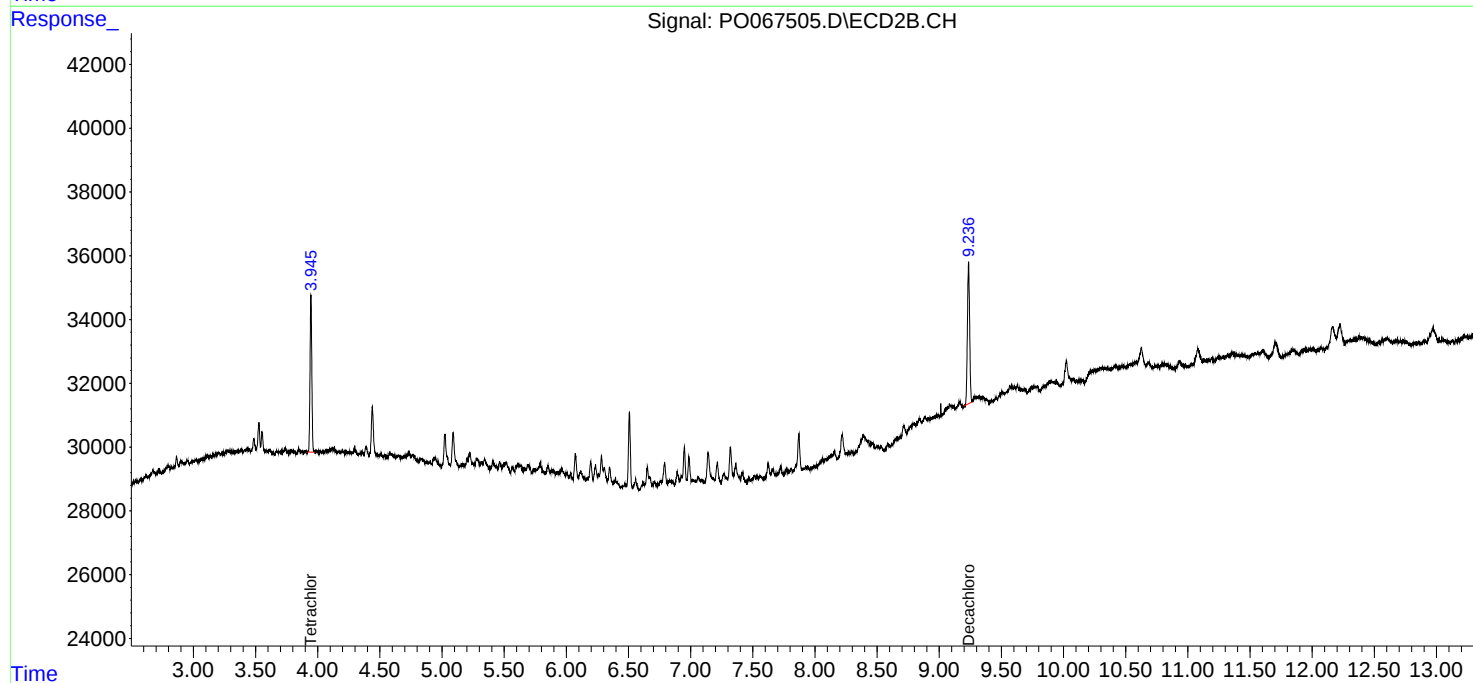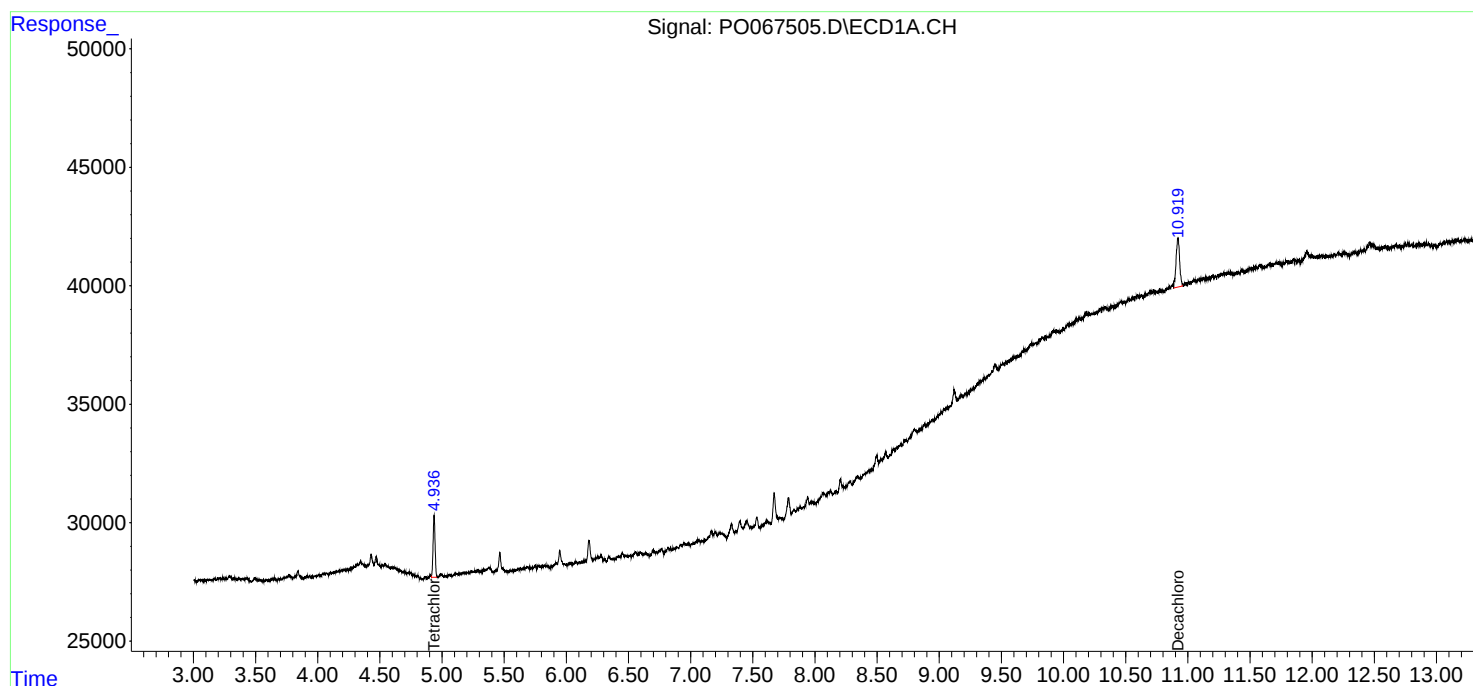

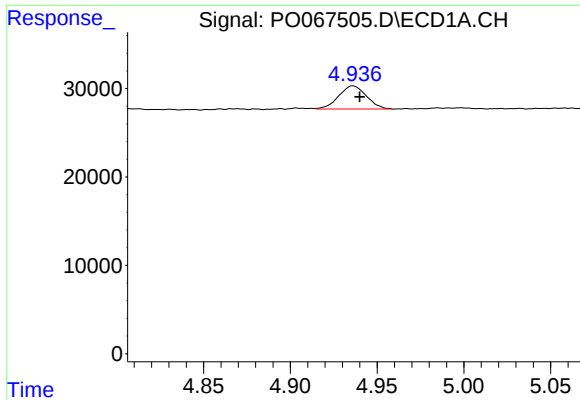


#1 Tetrachloro-m-xylene

R.T.: 4.936 min
Delta R.T.: -0.004 min
Response: 28999
Conc: 1.36 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-5-(1-3)


Manual Integrations
APPROVED

Sohil
3/31/2020 4:50:59 PM

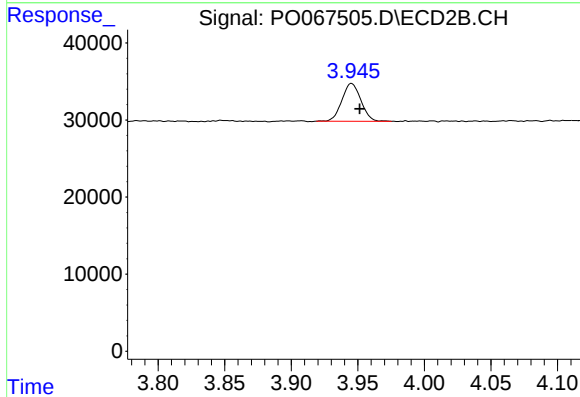


#1 Tetrachloro-m-xylene

R.T.: 3.945 min
Delta R.T.: -0.006 min
Response: 48729
Conc: 1.39 ng/ml

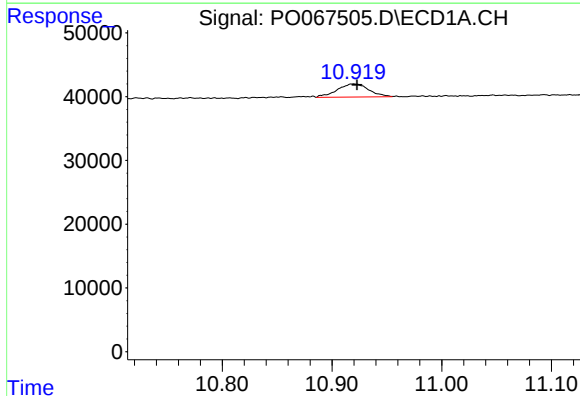

#2 Decachlorobiphenyl

R.T.: 10.919 min
Delta R.T.: -0.003 min
Response: 41282
Conc: 1.44 ng/ml m

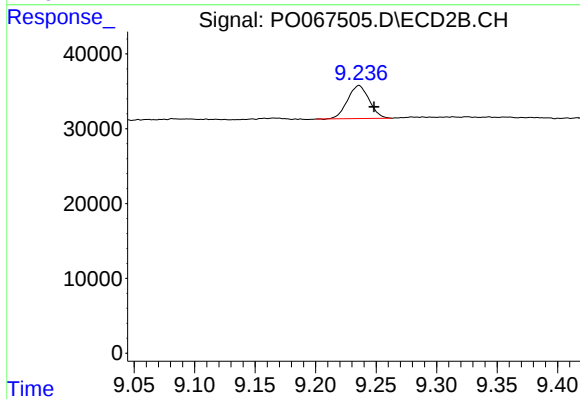

#2 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.012 min
Response: 54869
Conc: 1.41 ng/ml