

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033020\
 Data File : P0067506.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2020 15:55
 Operator : DD\AJ
 Sample : L1762-23
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-04-032720

Manual Integrations
 APPROVED

Sohil
 3/31/2020 4:51:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 16:19:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	3.946	483248	770938	22.737m	22.053
2) SA Decachlor...	10.919	9.236	572032	685629	19.908	17.578

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033020\
Data File : P0067506.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2020 15:55
Operator : DD\AJ
Sample : L1762-23
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-04-032720


Manual Integrations
APPROVED

Sohil
3/31/2020 4:51:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 16:19:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

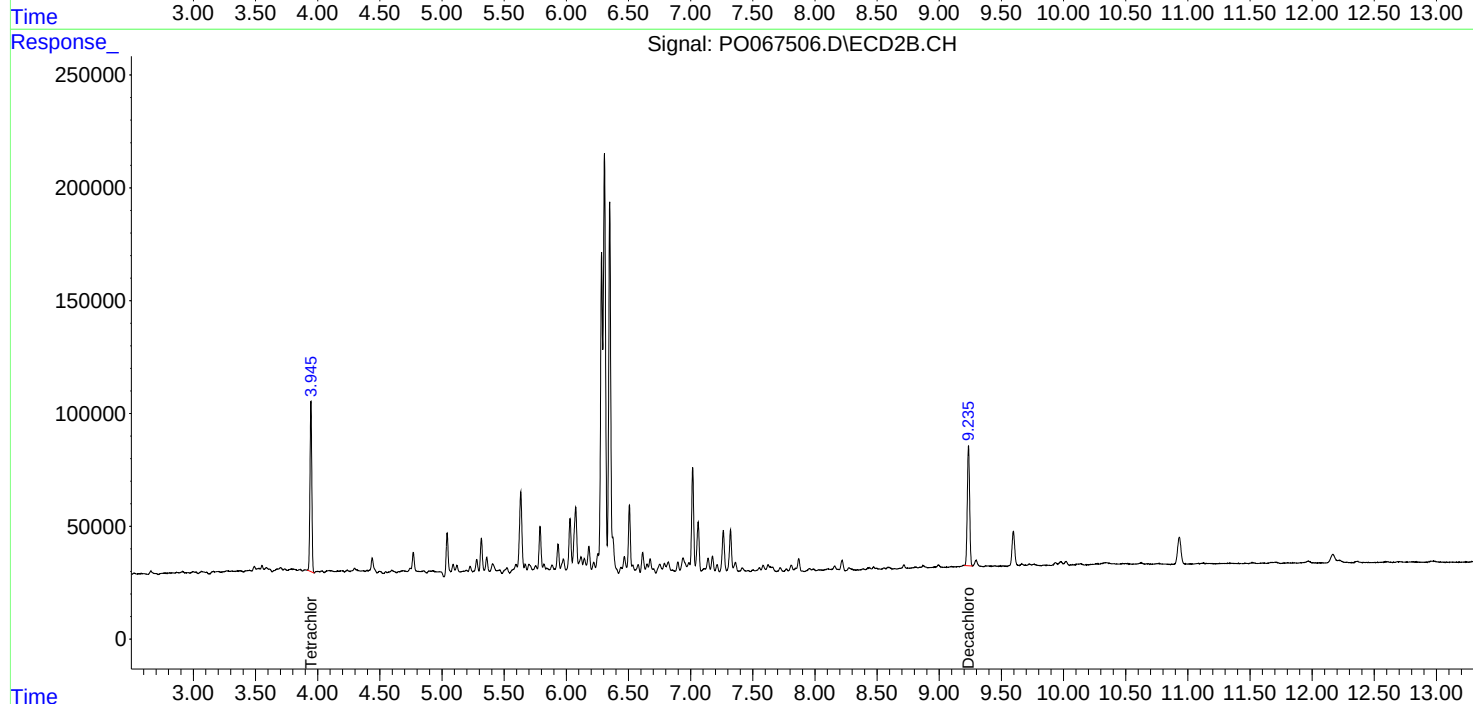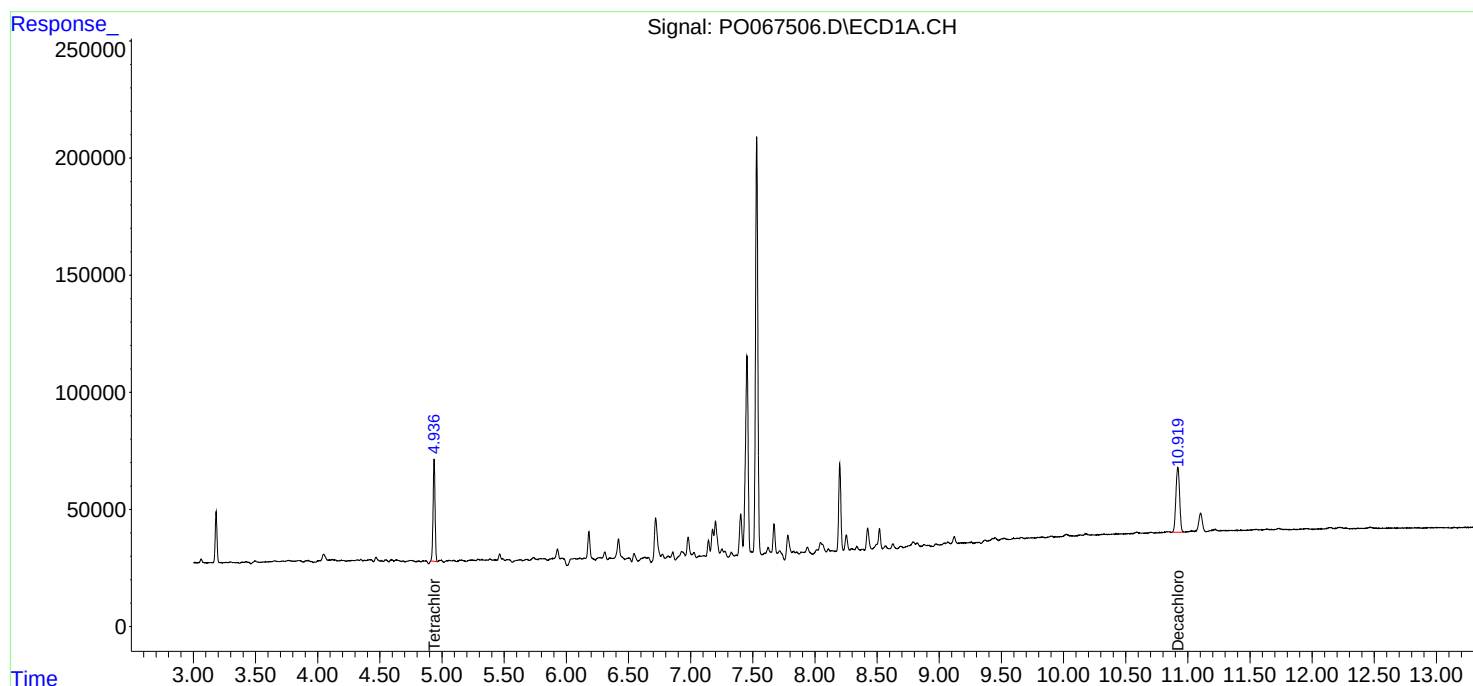

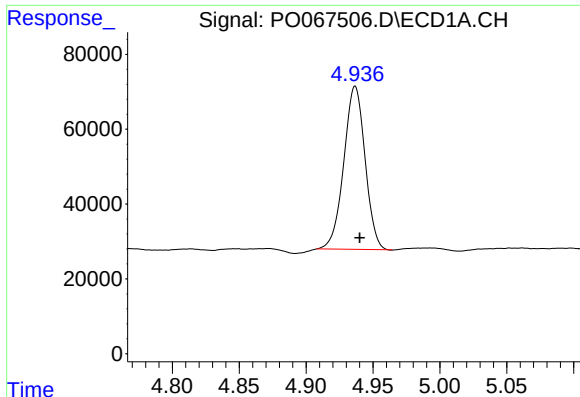


#1 Tetrachloro-m-xylene

R.T.: 4.936 min
Delta R.T.: -0.004 min
Response: 483248
Conc: 22.74 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TR-04-032720


Manual Integrations
APPROVED

Sohil
3/31/2020 4:51:00 PM

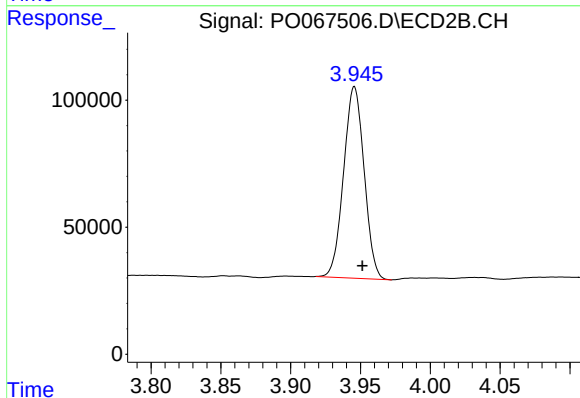


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: -0.006 min
Response: 770938
Conc: 22.05 ng/ml

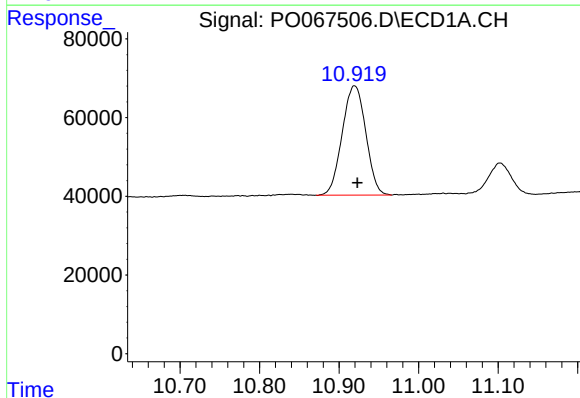

#2 Decachlorobiphenyl

R.T.: 10.919 min
Delta R.T.: -0.003 min
Response: 572032
Conc: 19.91 ng/ml

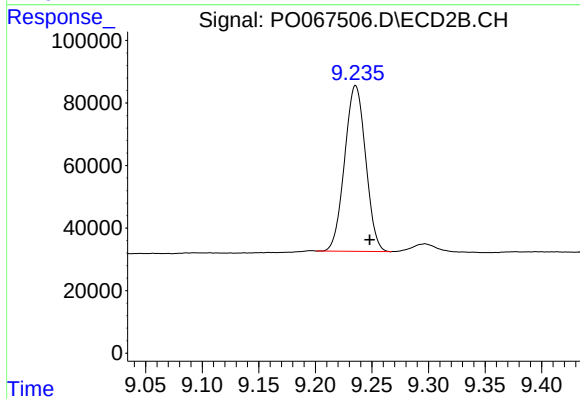

#2 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.013 min
Response: 685629
Conc: 17.58 ng/ml