

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033020\
 Data File : P0067510.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2020 17:03
 Operator : DD\AJ
 Sample : L2055-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-7-(1-3)

Manual Integrations
 APPROVED

Sohil
 3/31/2020 4:51:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 17:27:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	3.946	548740	850839	25.819	24.339
2) SA Decachlor...	10.920	9.235	589738	706163	20.525	18.104m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033020\
Data File : P0067510.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2020 17:03
Operator : DD\AJ
Sample : L2055-08
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-7-(1-3)


Manual Integrations
APPROVED

Sohil
3/31/2020 4:51:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 17:27:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

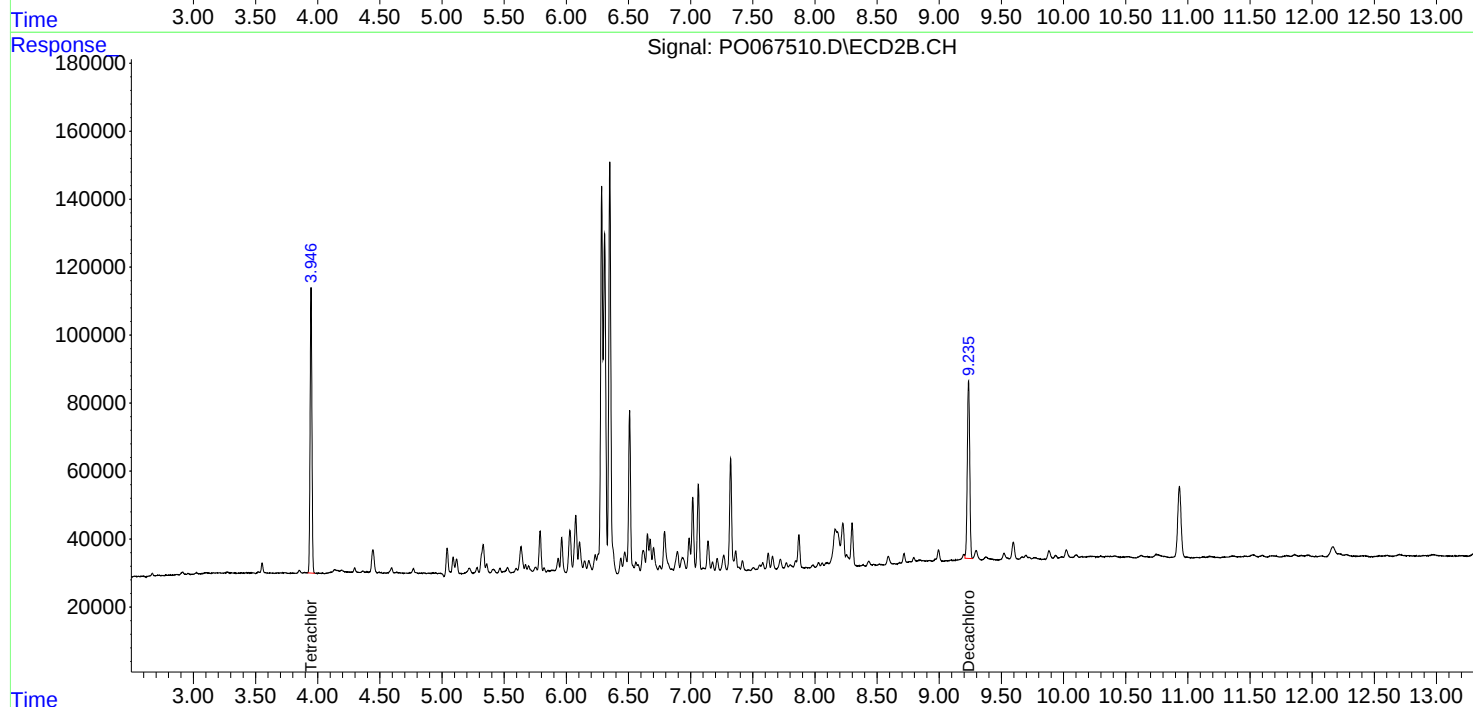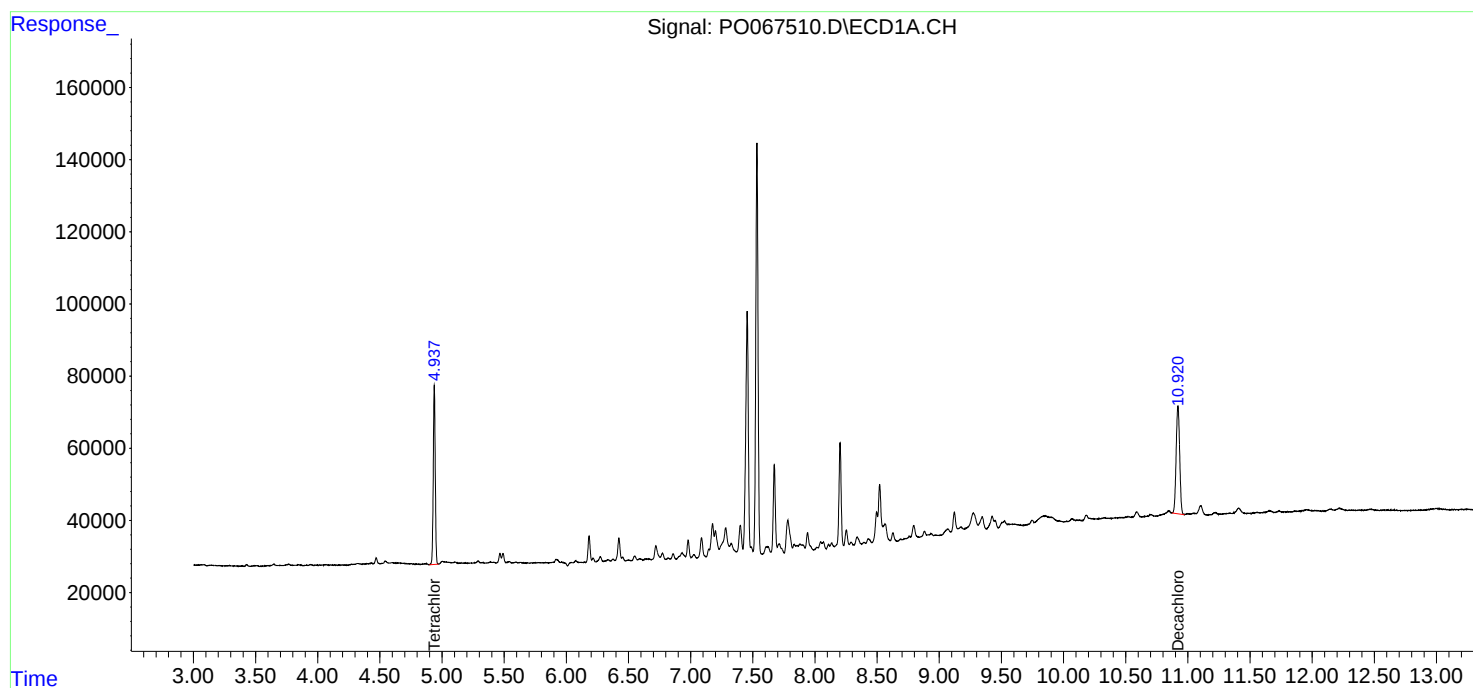

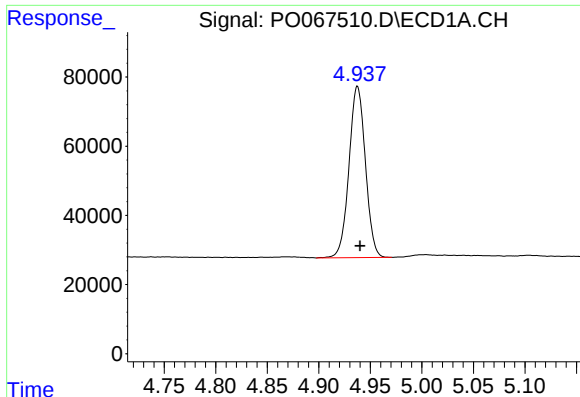


#1 Tetrachloro-m-xylene

R.T.: 4.938 min
Delta R.T.: -0.002 min
Response: 548740
Conc: 25.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-7-(1-3)


Manual Integrations
APPROVED

Sohil
3/31/2020 4:51:02 PM

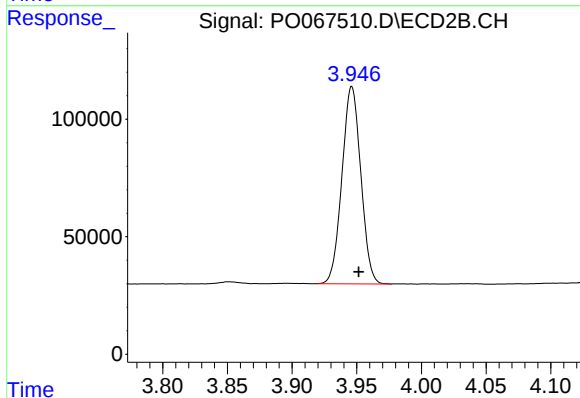


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: -0.005 min
Response: 850839
Conc: 24.34 ng/ml

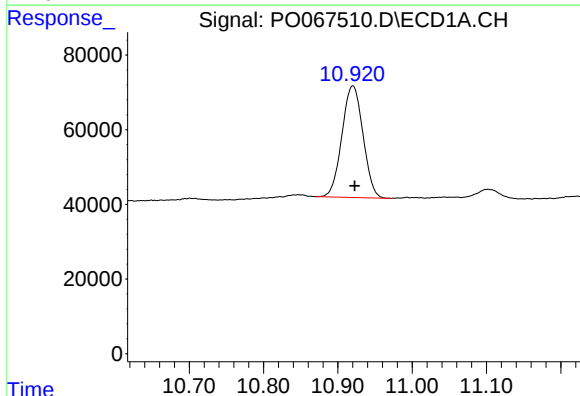

#2 Decachlorobiphenyl

R.T.: 10.920 min
Delta R.T.: -0.003 min
Response: 589738
Conc: 20.52 ng/ml

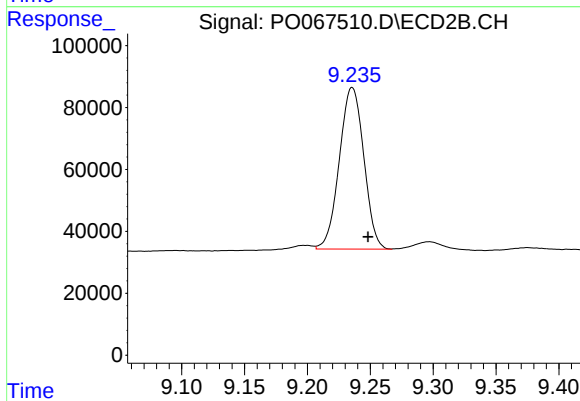

#2 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: -0.013 min
Response: 706163
Conc: 18.10 ng/ml m