

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033120\
 Data File : P0067537.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2020 20:25
 Operator : DD\AJ
 Sample : L2078-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 04:20:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.937	3.945	452330	678327	21.282	19.404
2)	SA Decachlor...	10.921	9.235	524092	635275	18.240	16.287
Target Compounds							
27)	L6 AR-1254-2	0.000	6.282	0	55834	N.D.	32.393 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033120\
Data File : P0067537.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2020 20:25
Operator : DD\AJ
Sample : L2078-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 04:20:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

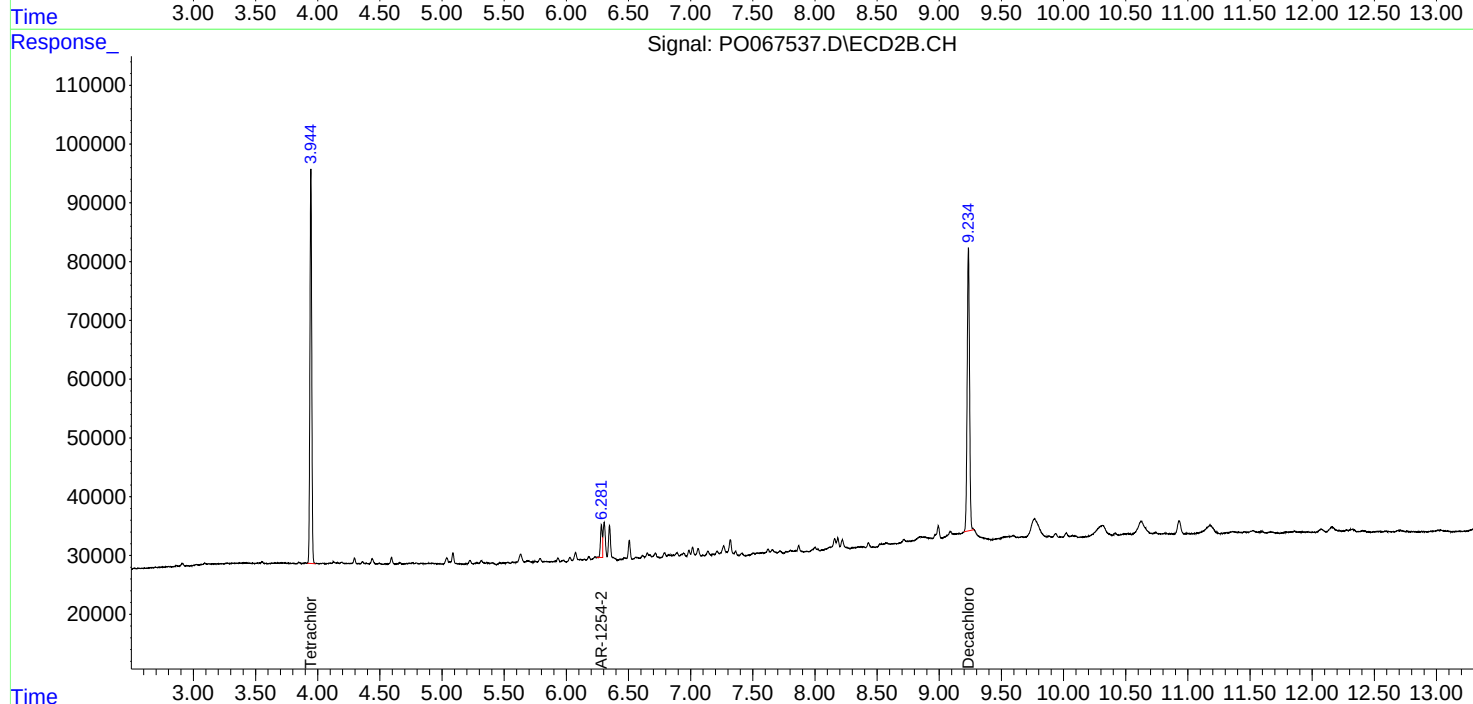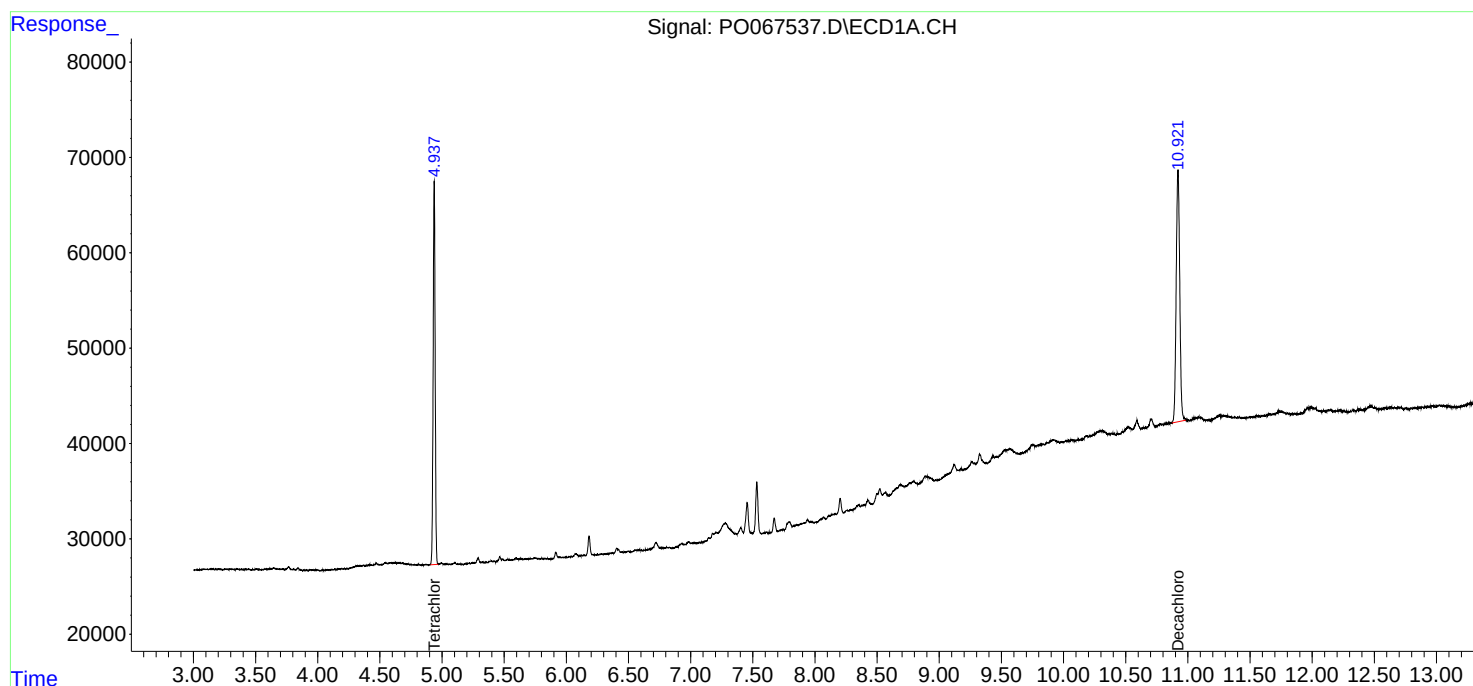


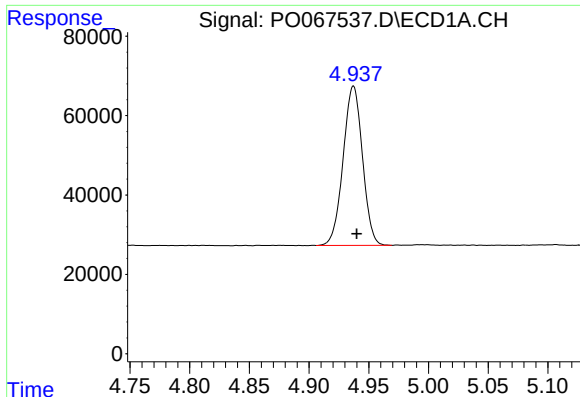

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: -0.003 min
Response: 452330
Conc: 21.28 ng/ml

Instrument :
ECD_O
ClientSampleId :

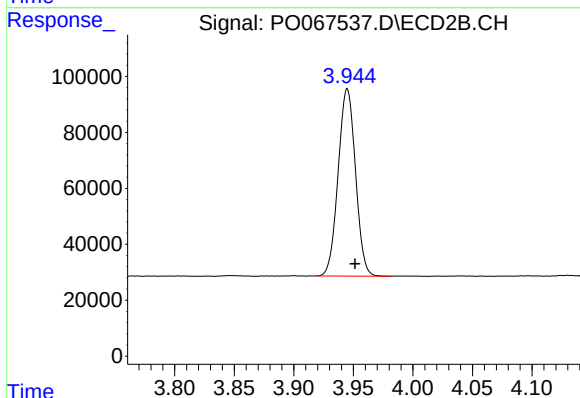


#1 Tetrachloro-m-xylene

R.T.: 3.945 min
Delta R.T.: -0.007 min
Response: 678327
Conc: 19.40 ng/ml

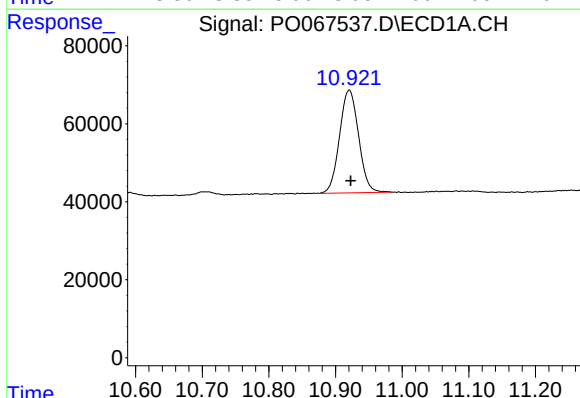


#2 Decachlorobiphenyl

R.T.: 10.921 min
Delta R.T.: -0.002 min
Response: 524092
Conc: 18.24 ng/ml

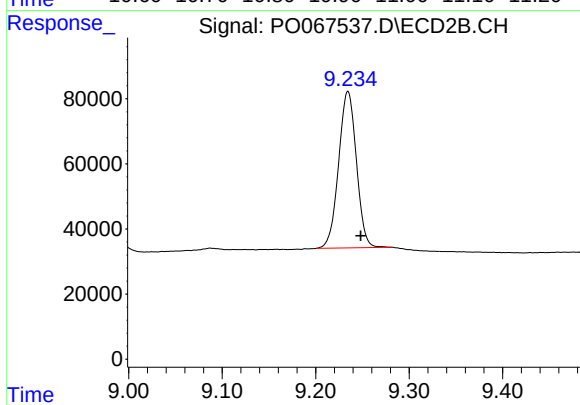

#2 Decachlorobiphenyl


R.T.: 9.235 min
Delta R.T.: -0.014 min
Response: 635275
Conc: 16.29 ng/ml

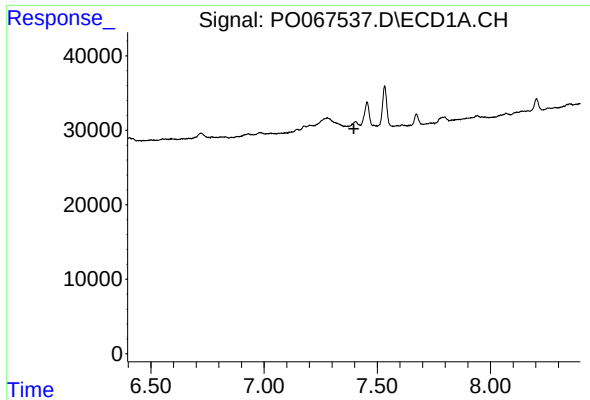

#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 7.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

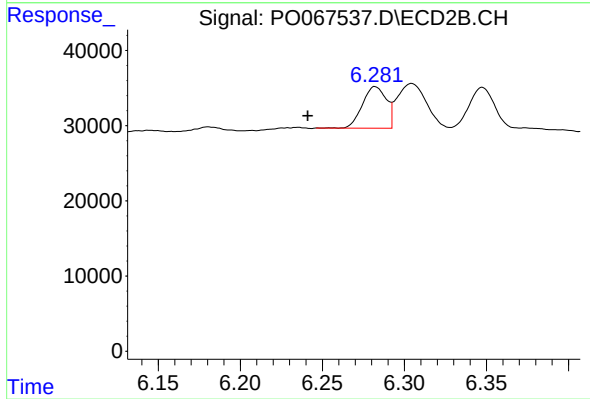

#27 AR-1254-2

R.T.: 6.282 min
Delta R.T.: 0.041 min
Response: 55834
Conc: 32.39 ng/ml