

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033120\
 Data File : P0067532.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2020 19:00
 Operator : DD\AJ
 Sample : L2075-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S2-03-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 04:18:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.937	3.945	480149	716803	22.591	20.504
2) SA Decachlor...	10.920	9.235	557405	697232	19.399	17.875

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033120\
Data File : P0067532.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2020 19:00
Operator : DD\AJ
Sample : L2075-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S2-03-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 04:18:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

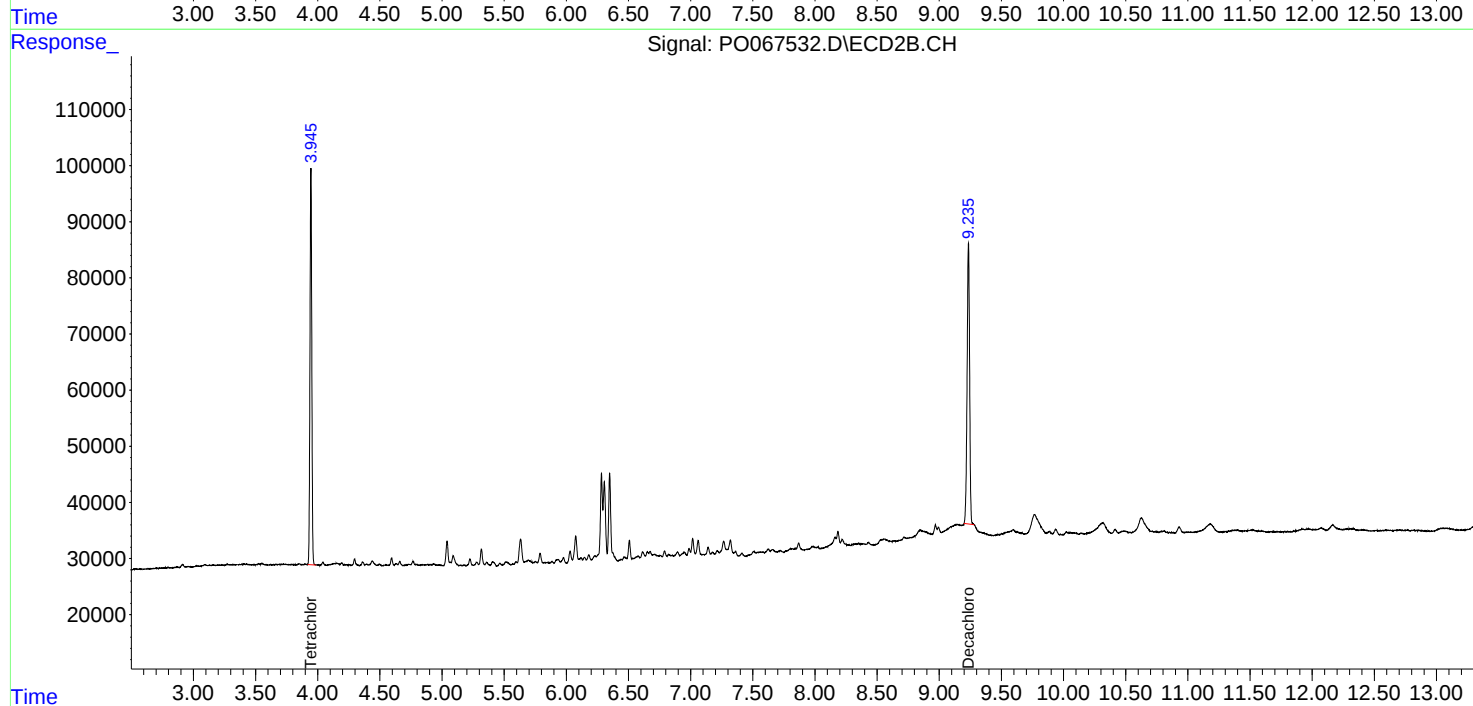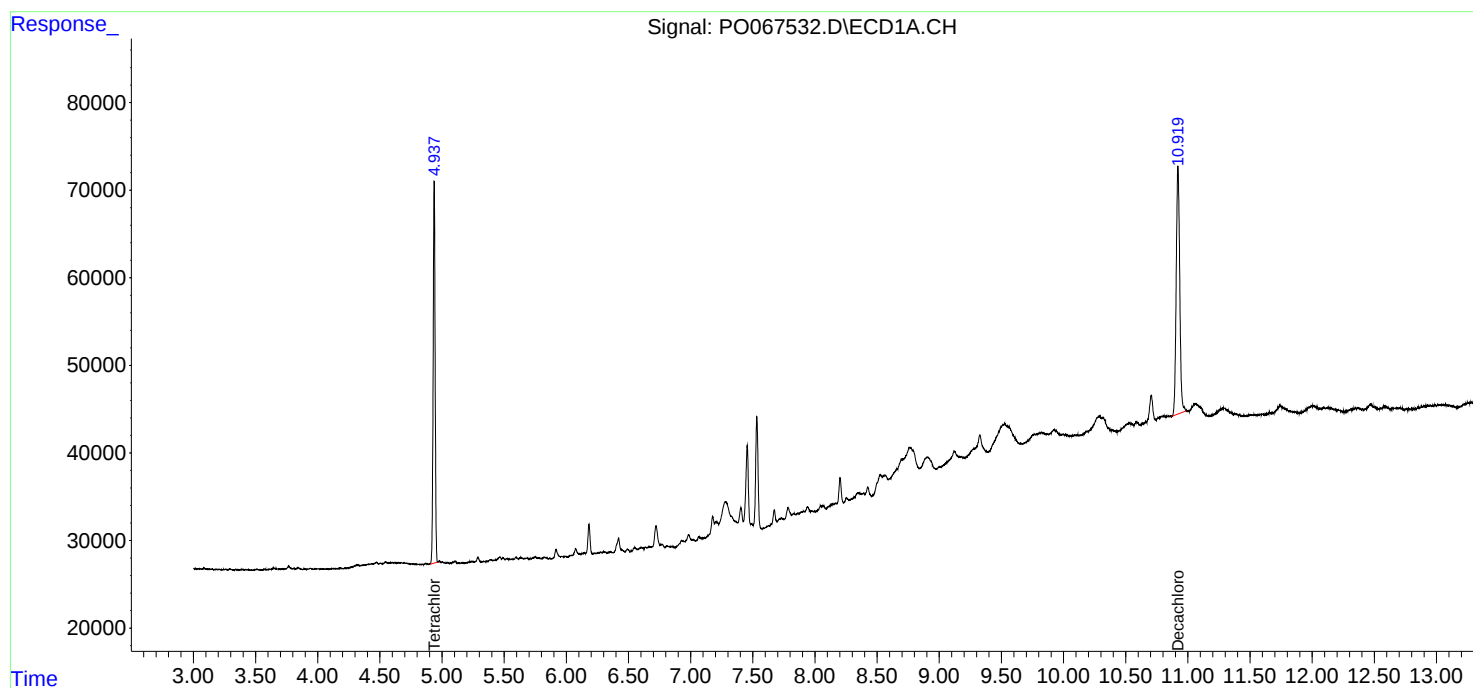


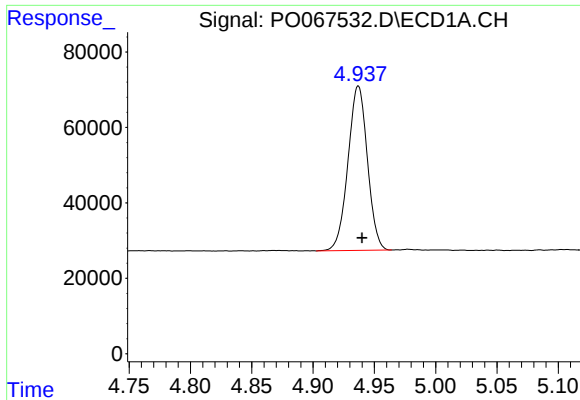

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: -0.003 min
Response: 480149
Conc: 22.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-03-A

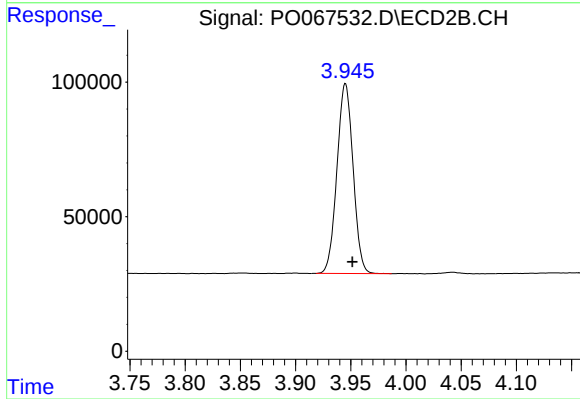


#1 Tetrachloro-m-xylene

R.T.: 3.945 min
Delta R.T.: -0.006 min
Response: 716803
Conc: 20.50 ng/ml

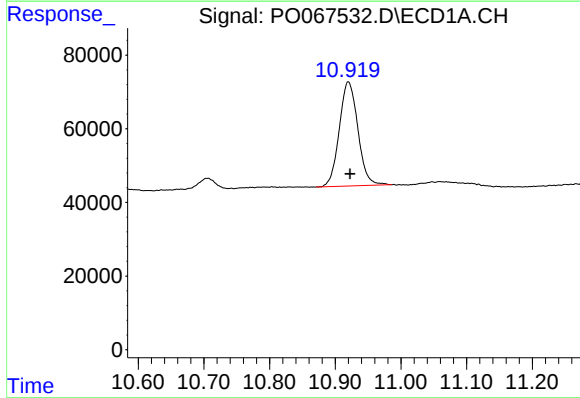

#2 Decachlorobiphenyl

R.T.: 10.920 min
Delta R.T.: -0.003 min
Response: 557405
Conc: 19.40 ng/ml

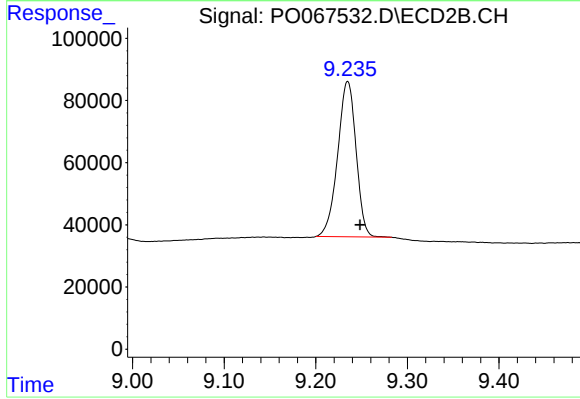

#2 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: -0.013 min
Response: 697232
Conc: 17.87 ng/ml