

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033120\
 Data File : P0067533.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2020 19:17
 Operator : DD\AJ
 Sample : L2075-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S2-04-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 04:19:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.937	3.944	468975	691111	22.066	19.769
2)	SA Decachlor...	10.920	9.234	452560	556727	15.750	14.273

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033120\
Data File : P0067533.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2020 19:17
Operator : DD\AJ
Sample : L2075-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S2-04-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 04:19:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

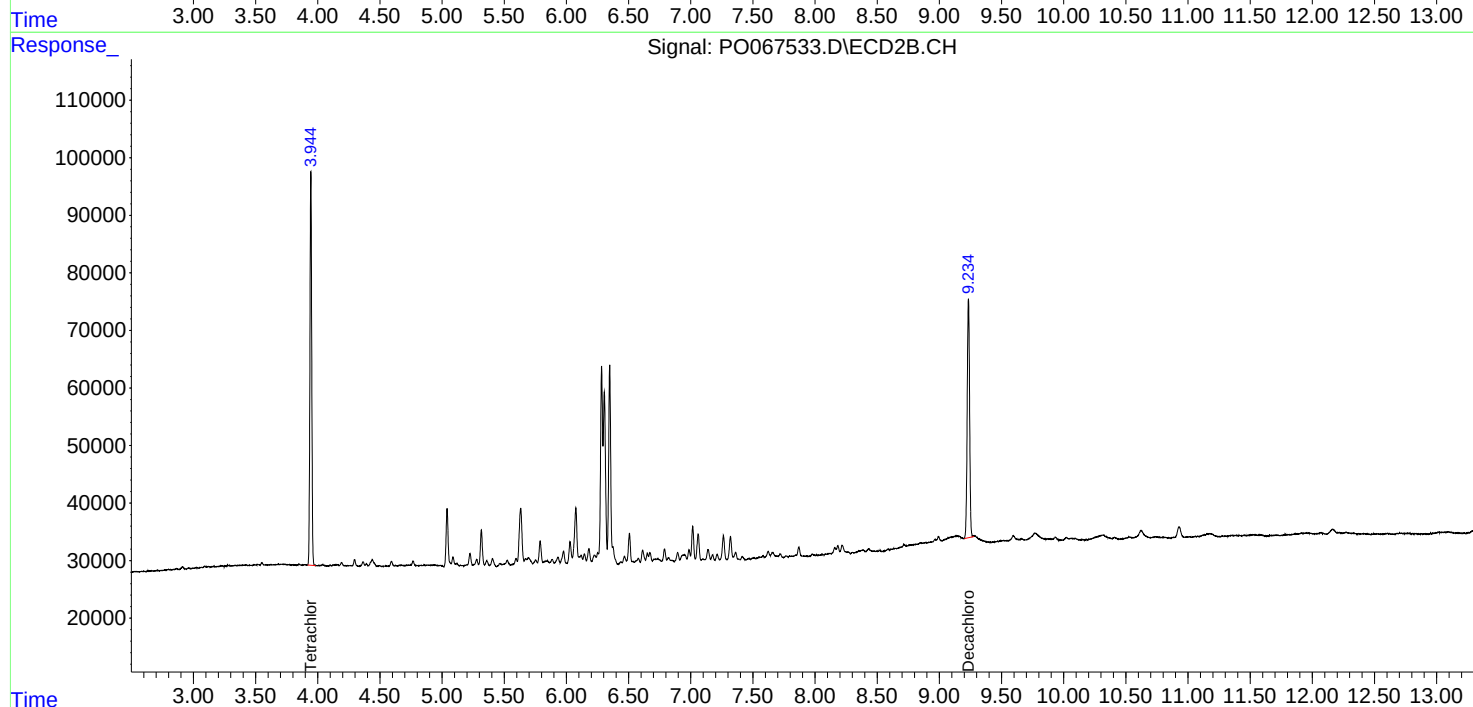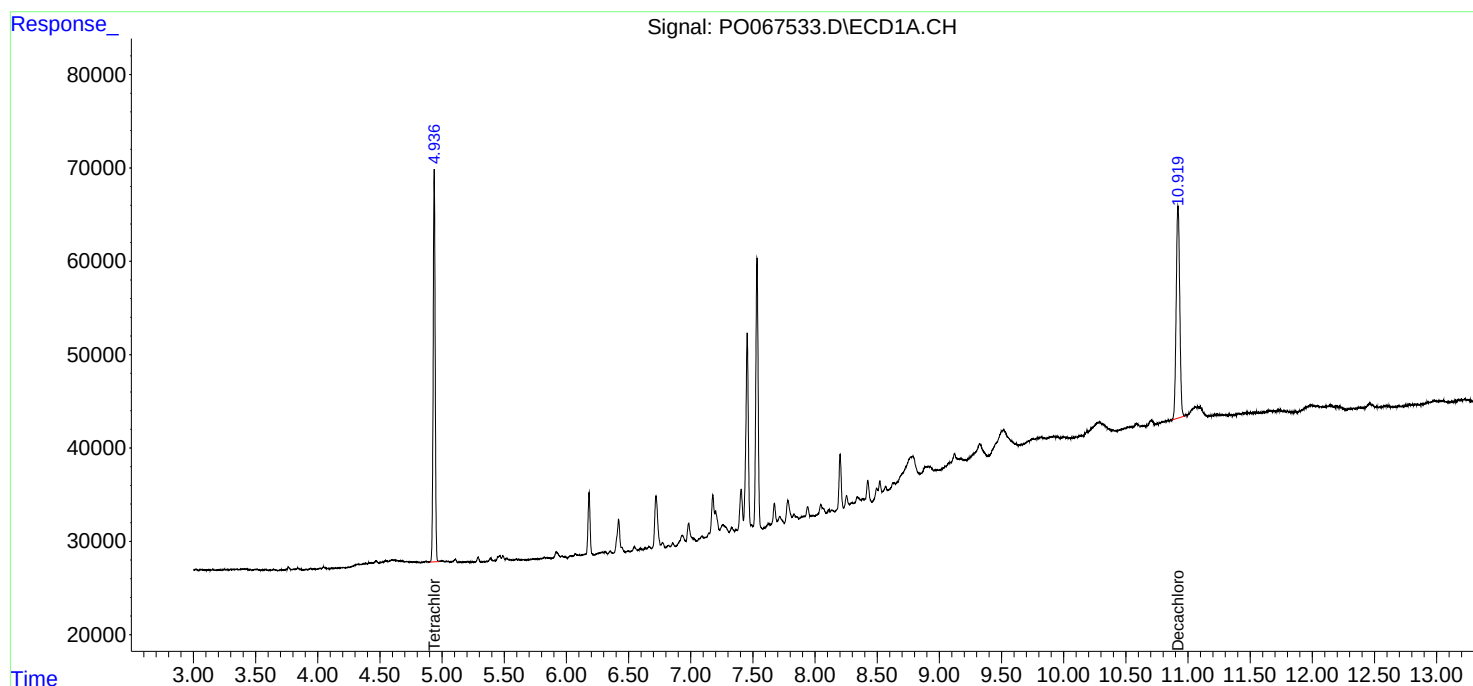


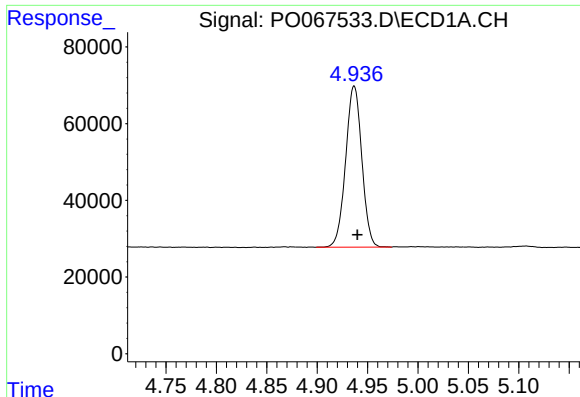

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: -0.003 min
Response: 468975
Conc: 22.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-04-A

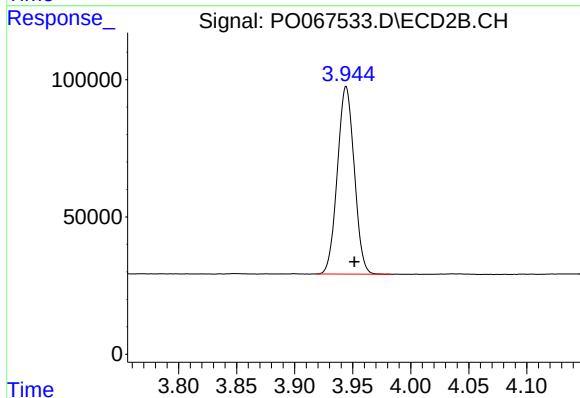


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: -0.007 min
Response: 691111
Conc: 19.77 ng/ml

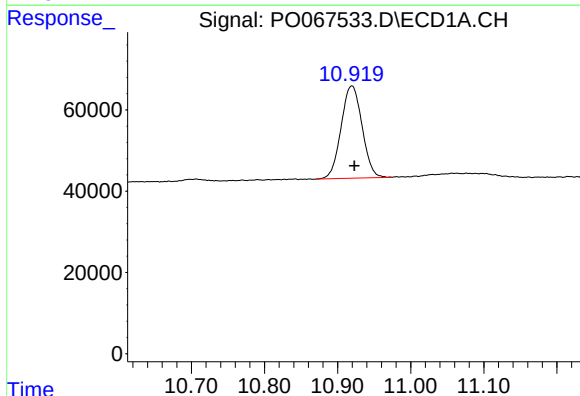

#2 Decachlorobiphenyl

R.T.: 10.920 min
Delta R.T.: -0.003 min
Response: 452560
Conc: 15.75 ng/ml

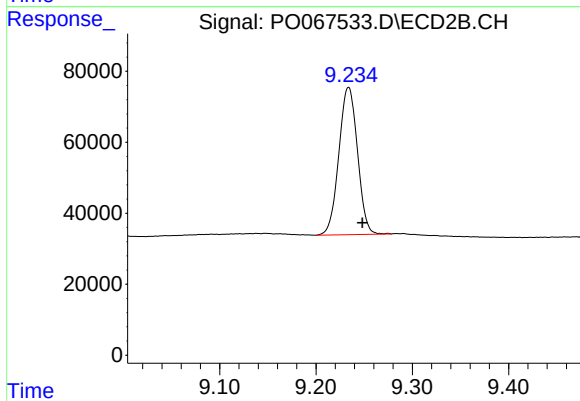

#2 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: -0.014 min
Response: 556727
Conc: 14.27 ng/ml