

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040120\
 Data File : P0067563.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2020 16:37
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 17:29:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 01 17:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.937	3.945	461550	702811	19.381	20.969
2) SA Decachlor...	10.921	9.234	702713	863162	20.641	20.877
Target Compounds						
32) L7 AR-1260-2	8.147	0.000	121760	0	72.125	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040120\
Data File : P0067563.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2020 16:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 17:29:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 01 17:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

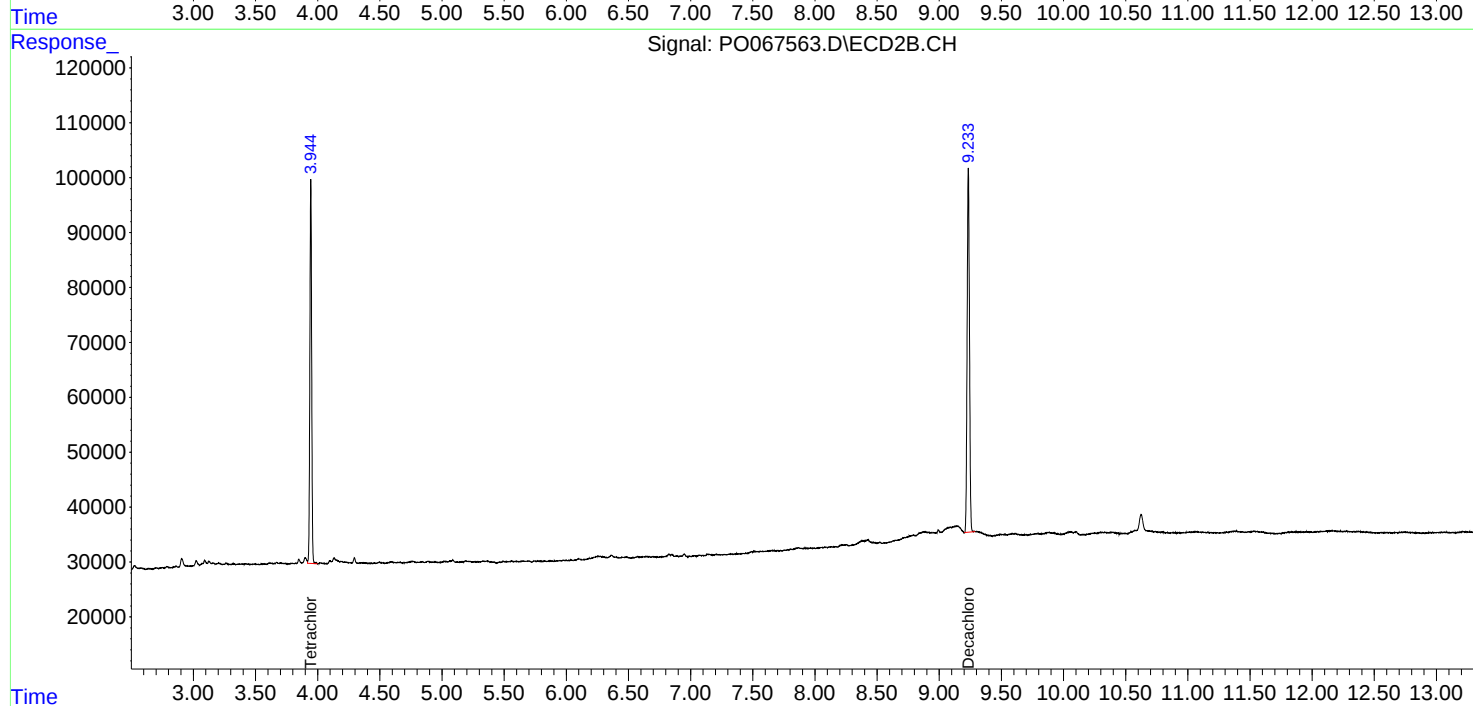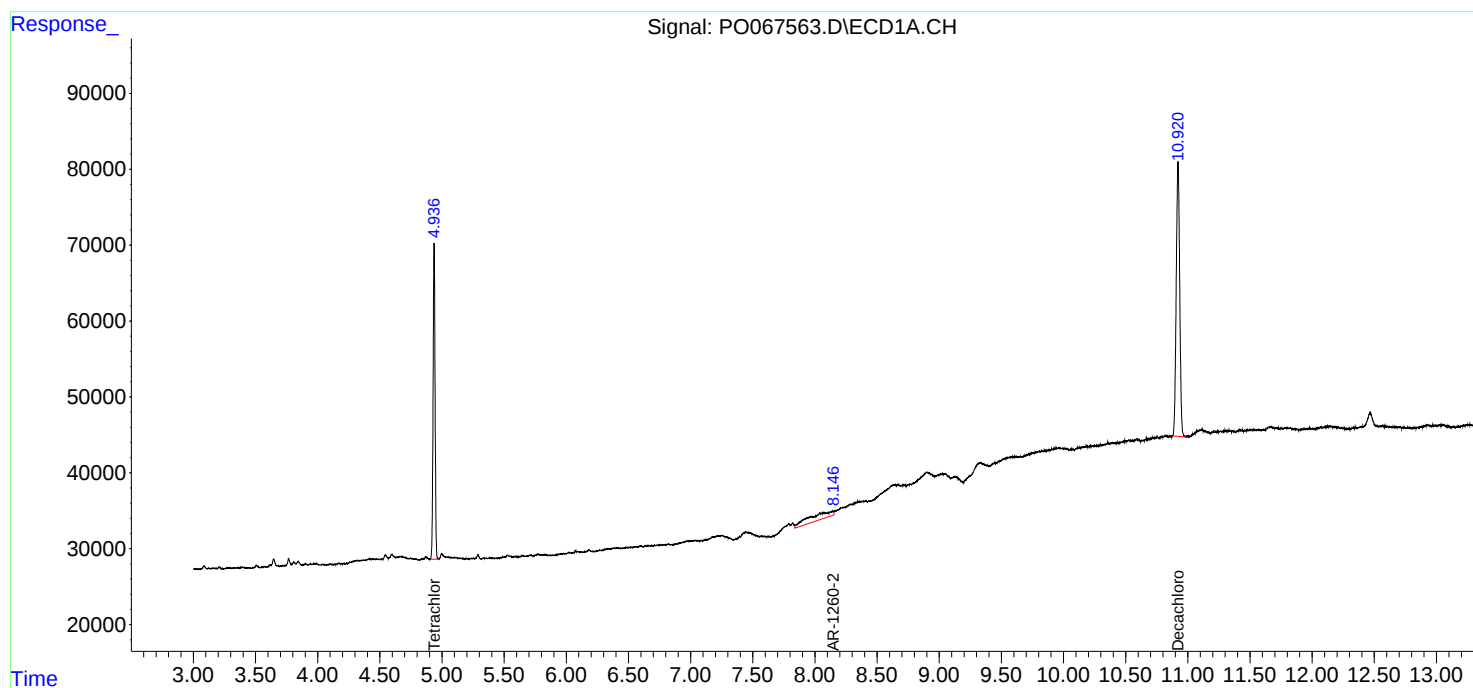


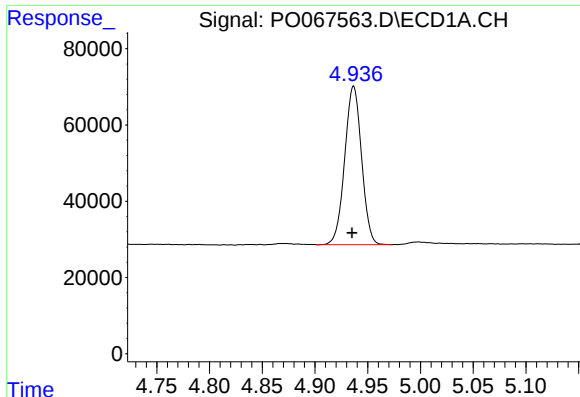

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: 0.002 min
Response: 461550
Conc: 19.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

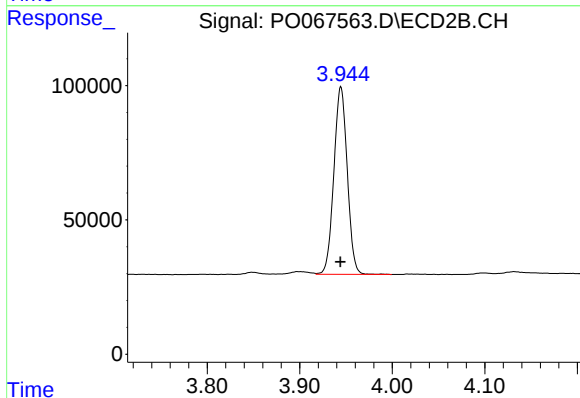


#1 Tetrachloro-m-xylene

R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 702811
Conc: 20.97 ng/ml

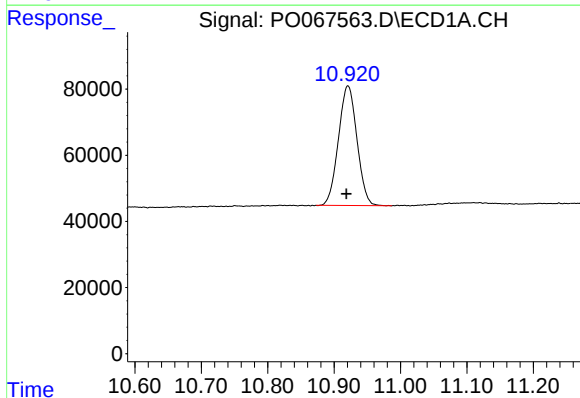


#2 Decachlorobiphenyl

R.T.: 10.921 min
Delta R.T.: 0.002 min
Response: 702713
Conc: 20.64 ng/ml

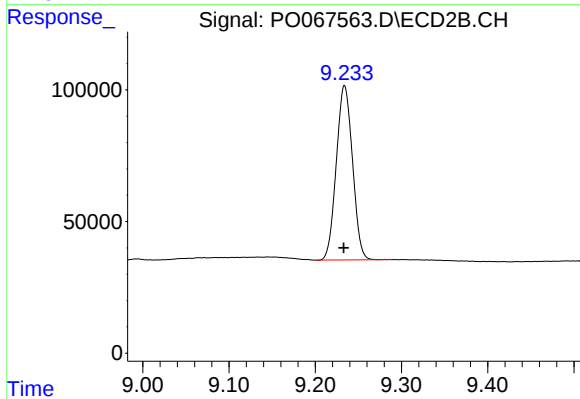

#2 Decachlorobiphenyl


R.T.: 9.234 min
Delta R.T.: 0.000 min
Response: 863162
Conc: 20.88 ng/ml

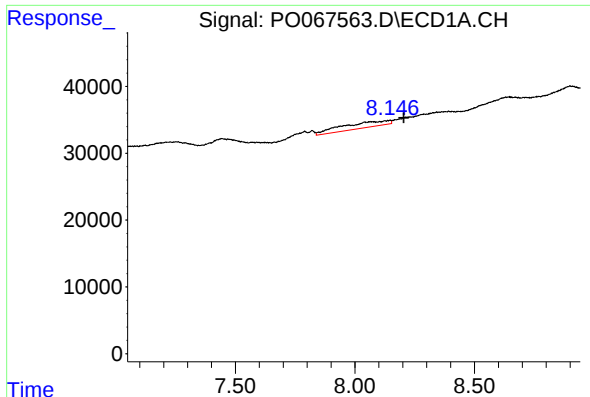

#32 AR-1260-2

R.T.: 8.147 min
Delta R.T.: -0.058 min
Response: 121760
Conc: 72.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

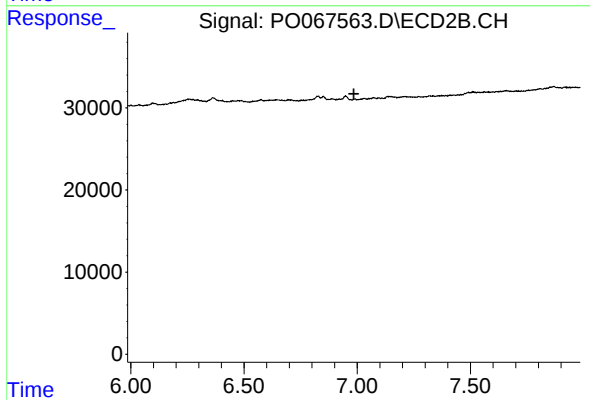

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.985 min
Response: 0
Conc: N.D.