

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040120\
 Data File : P0067585.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2020 23:09
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 03:00:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 01 17:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.935	3.944	517614	799369	21.736	23.850
2)	SA Decachlor...	10.918	9.232	722521	902536	21.223	21.829
Target Compounds							
33)	L7 AR-1260-3	8.574	0.000	25253	0	19.374	N.D. #
34)	L7 AR-1260-4	8.749	0.000	126892	0	82.569	N.D. #
36)	L8 AR-1262-1	8.574	0.000	25253	0	15.063	N.D. #
40)	L8 AR-1262-5	10.206	0.000	346849	0	294.170	N.D. #
43)	L9 AR-1268-3	9.745	0.000	256715	0	88.408	N.D. #
44)	L9 AR-1268-4	10.206	0.000	346849	0	249.851	N.D. #
45)	L9 AR-1268-5	10.589	0.000	136992	0	13.817	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040120\
Data File : PO067585.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2020 23:09
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 03:00:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 01 17:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

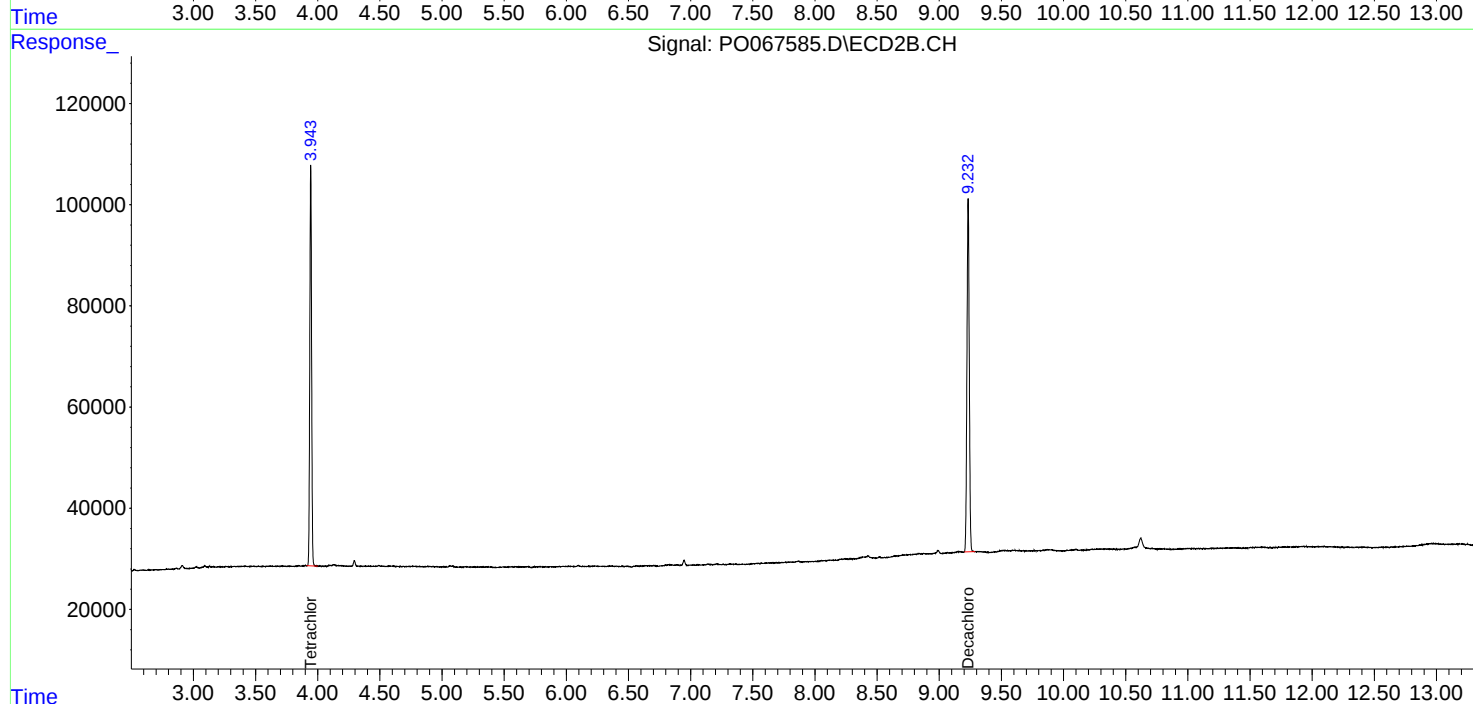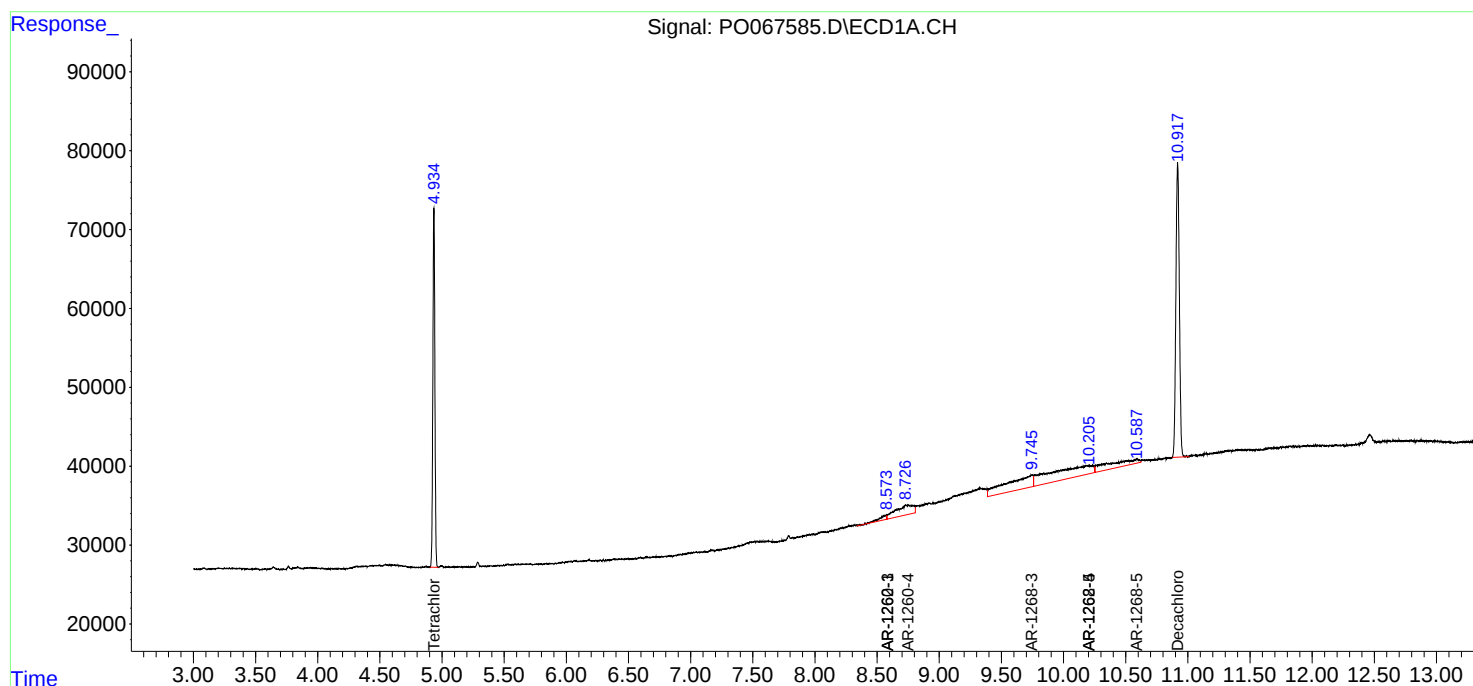


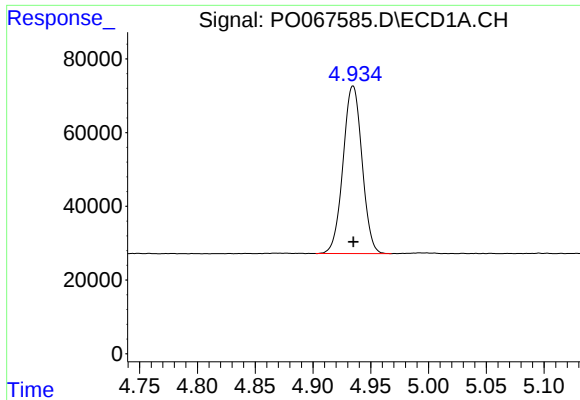

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 517614
Conc: 21.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

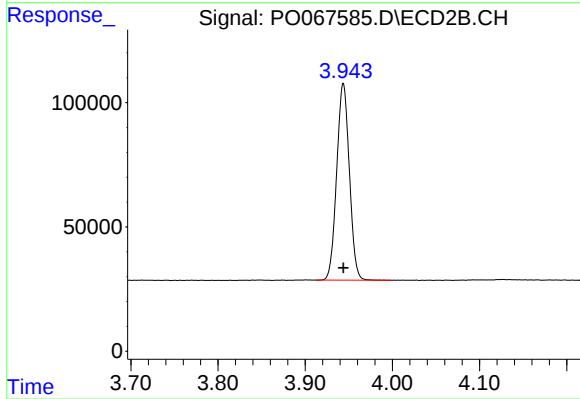


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 799369
Conc: 23.85 ng/ml

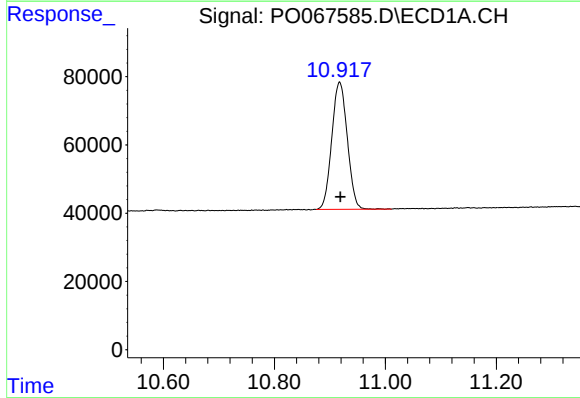


#2 Decachlorobiphenyl

R.T.: 10.918 min
Delta R.T.: -0.001 min
Response: 722521
Conc: 21.22 ng/ml

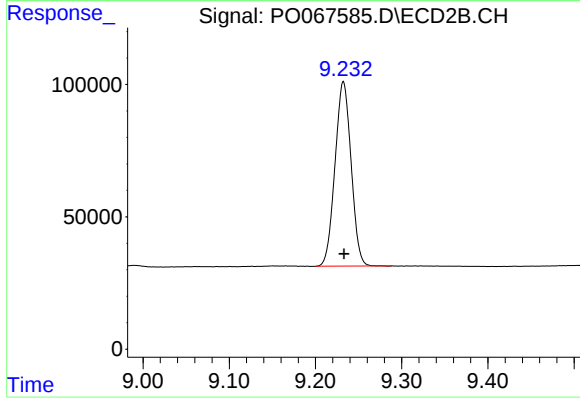

#2 Decachlorobiphenyl


R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 902536
Conc: 21.83 ng/ml

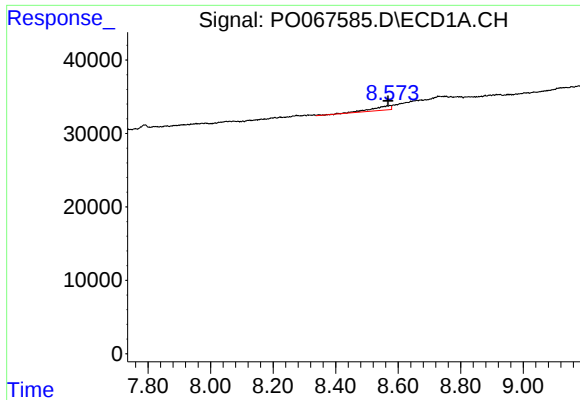

#33 AR-1260-3


R.T.: 8.574 min
Delta R.T.: 0.007 min
Response: 25253
Conc: 19.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

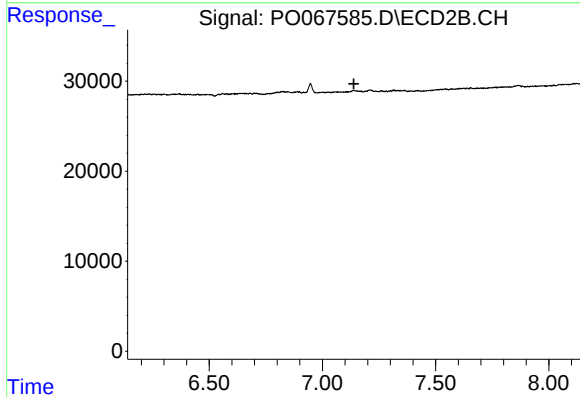


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.139 min
Response: 0
Conc: N.D.

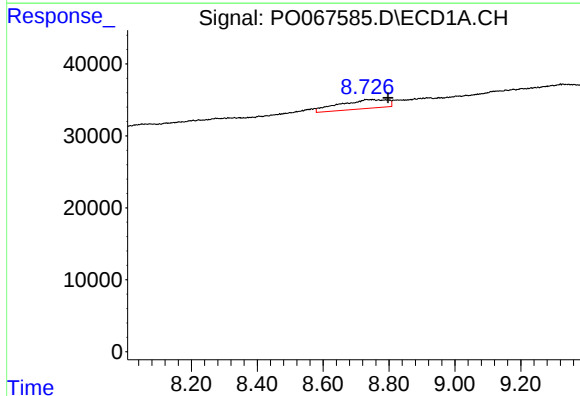


#34 AR-1260-4

R.T.: 8.749 min
Delta R.T.: -0.048 min
Response: 126892
Conc: 82.57 ng/ml

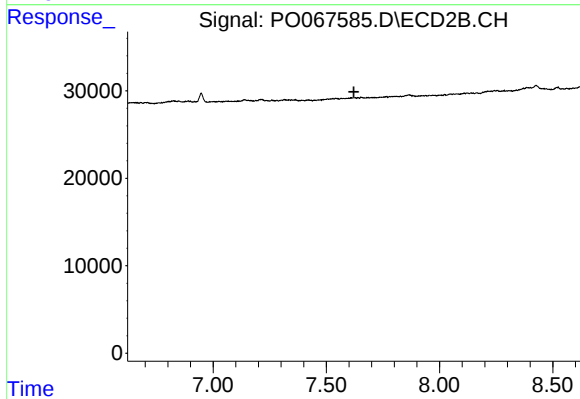

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.621 min
Response: 0
Conc: N.D.

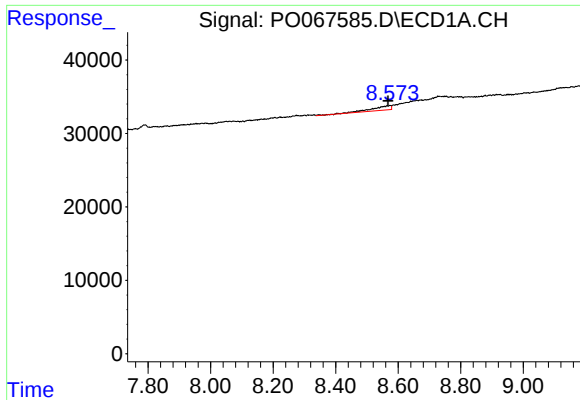

#36 AR-1262-1


R.T.: 8.574 min
Delta R.T.: 0.006 min
Response: 25253
Conc: 15.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

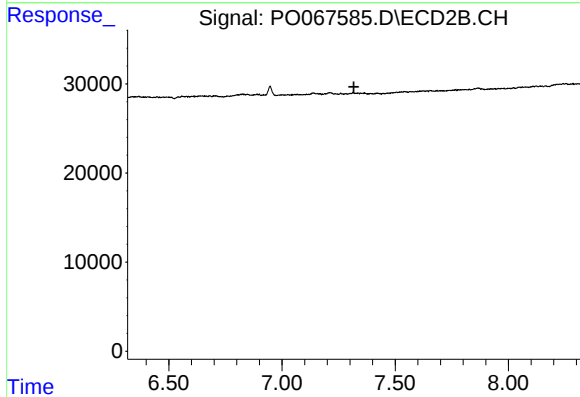


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.317 min
Response: 0
Conc: N.D.

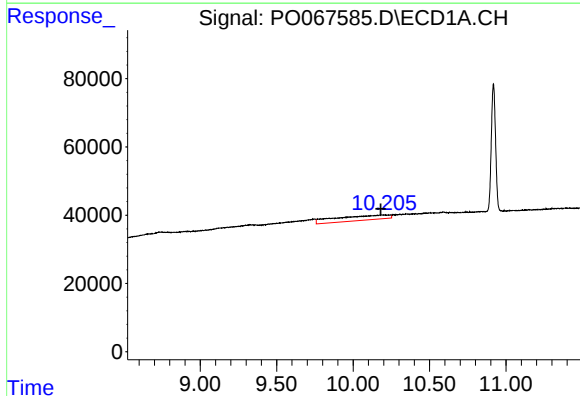


#40 AR-1262-5

R.T.: 10.206 min
Delta R.T.: 0.026 min
Response: 346849
Conc: 294.17 ng/ml

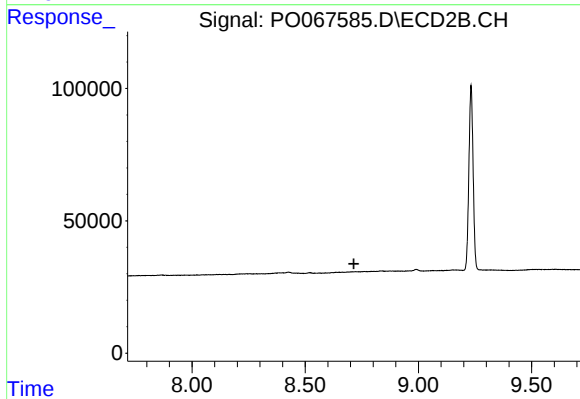

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.715 min
Response: 0
Conc: N.D.

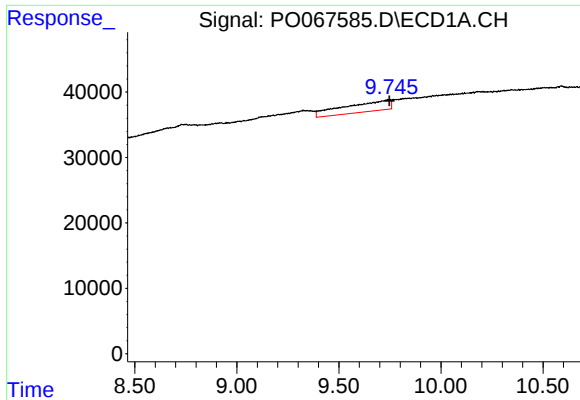

#43 AR-1268-3


R.T.: 9.745 min
Delta R.T.: 0.000 min
Response: 256715
Conc: 88.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

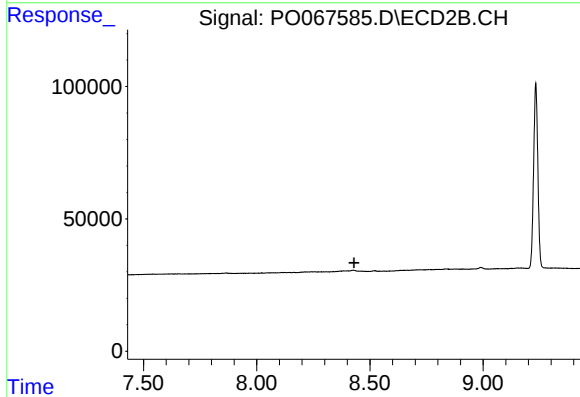


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.430 min
Response: 0
Conc: N.D.

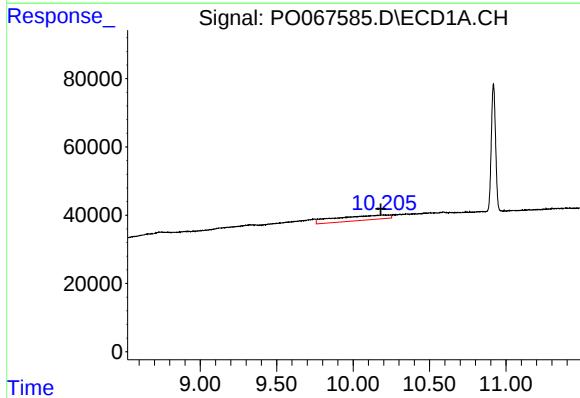


#44 AR-1268-4

R.T.: 10.206 min
Delta R.T.: 0.025 min
Response: 346849
Conc: 249.85 ng/ml

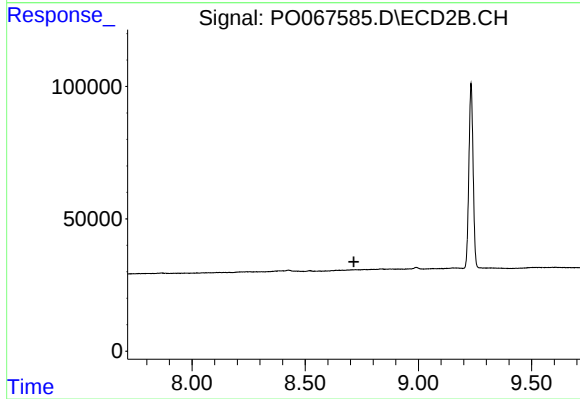

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.715 min
Response: 0
Conc: N.D.

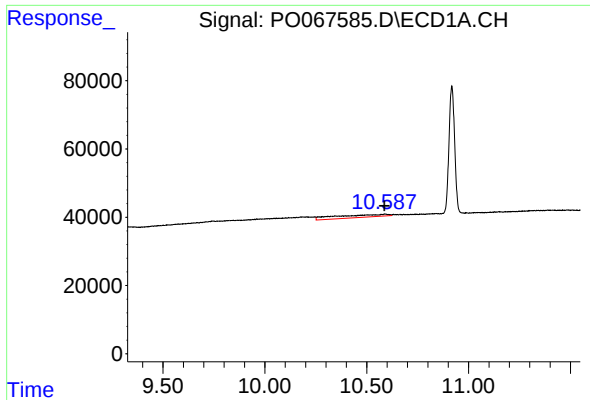

#45 AR-1268-5

R.T.: 10.589 min
Delta R.T.: 0.002 min
Response: 136992
Conc: 13.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

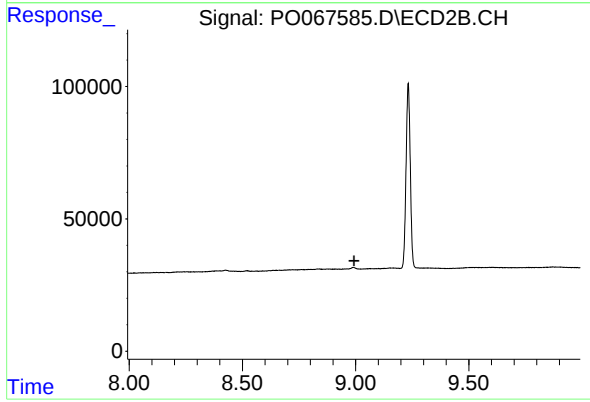

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.993 min
Response: 0
Conc: N.D.