

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040120\
 Data File : P0067597.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2020 2:49
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 04:01:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 01 17:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.934	3.943	531105	824793	22.302	24.608
2)	SA Decachlor...	10.916	9.232	733482	925373	21.545	22.381
Target Compounds							
28)	L6 AR-1254-3	7.787	0.000	30005	0	18.352	N.D. #
35)	L7 AR-1260-5	9.134	0.000	27289	0	8.651	N.D. #
37)	L8 AR-1262-2	9.134	0.000	27289	0	9.510	N.D. #
38)	L8 AR-1262-3	9.418	0.000	11253	0	5.408	N.D. #
39)	L8 AR-1262-4	9.462	0.000	13715	0	8.667	N.D. #
41)	L9 AR-1268-1	9.418	0.000	11253	0	3.045	N.D. #
42)	L9 AR-1268-2	9.462	0.000	13715	0	3.957	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040120\
Data File : P0067597.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2020 2:49
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 04:01:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 01 17:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

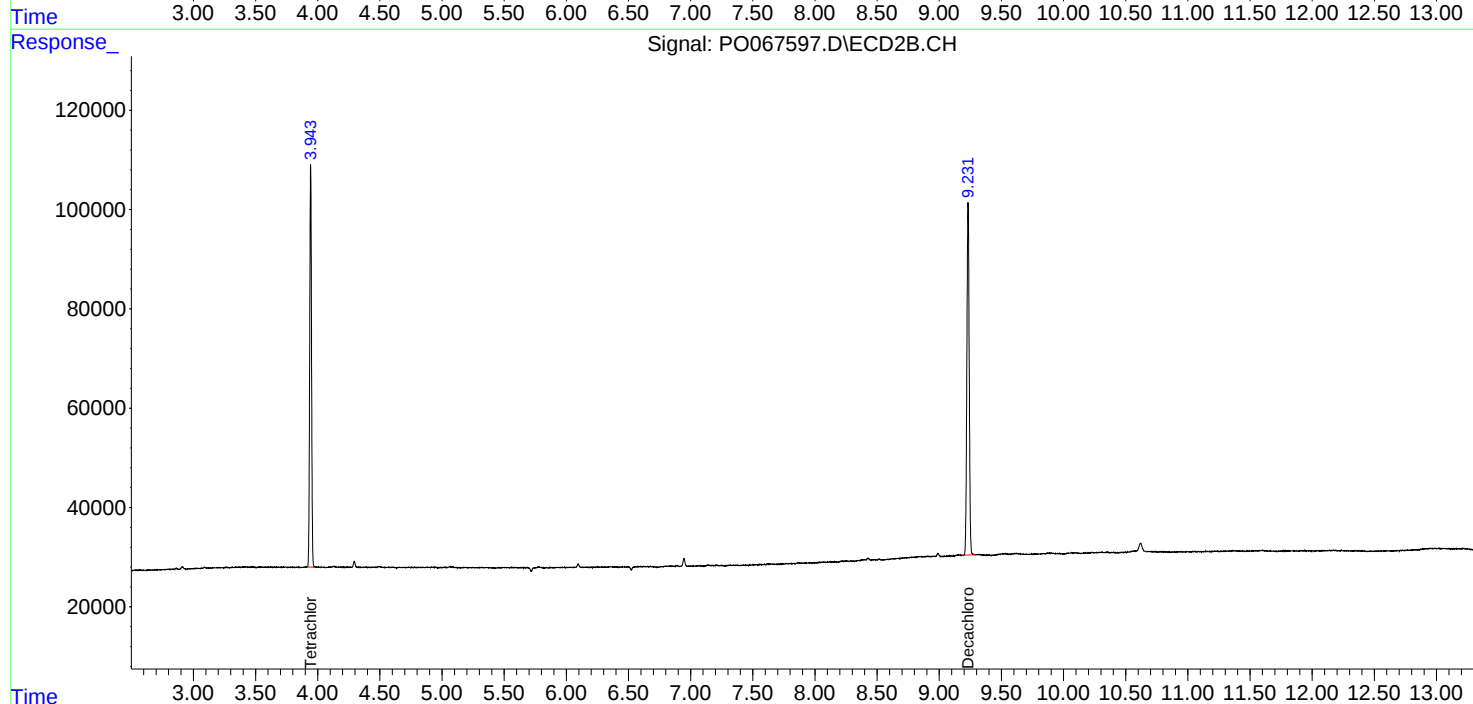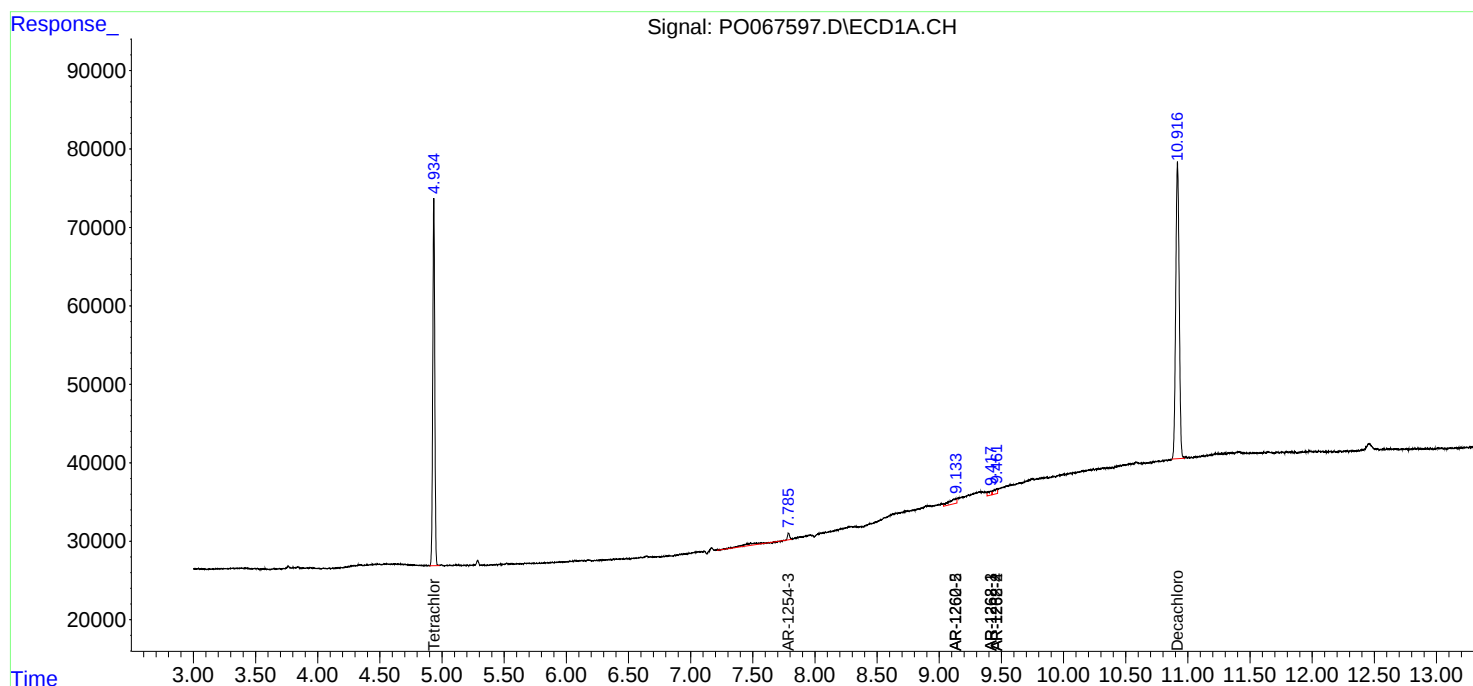


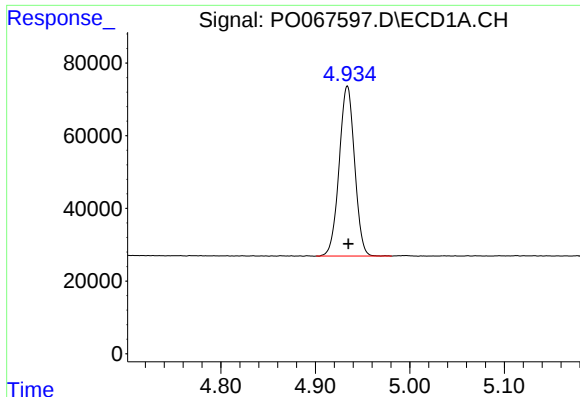

#1 Tetrachloro-m-xylene


R.T.: 4.934 min
Delta R.T.: -0.001 min
Response: 531105
Conc: 22.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

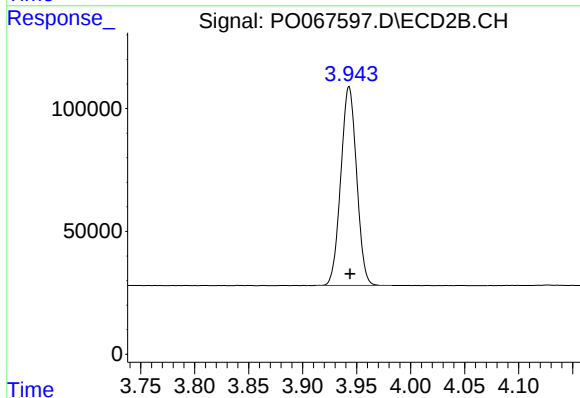


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 824793
Conc: 24.61 ng/ml

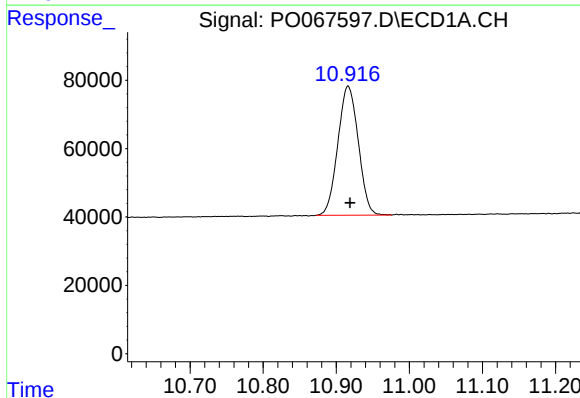


#2 Decachlorobiphenyl

R.T.: 10.916 min
Delta R.T.: -0.003 min
Response: 733482
Conc: 21.55 ng/ml

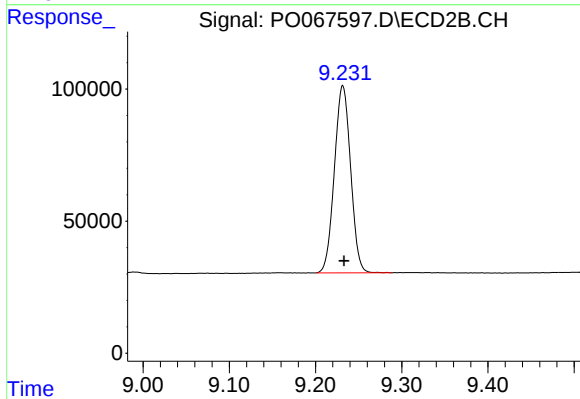

#2 Decachlorobiphenyl


R.T.: 9.232 min
Delta R.T.: -0.001 min
Response: 925373
Conc: 22.38 ng/ml

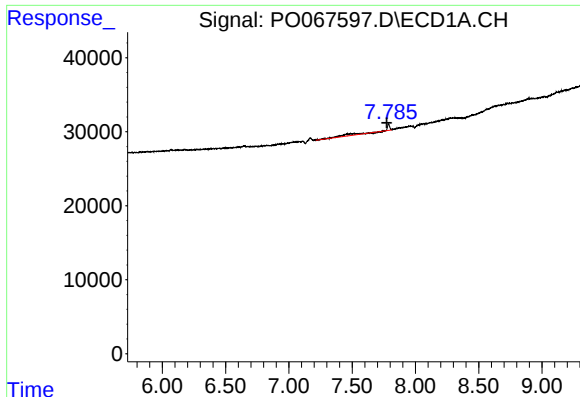

#28 AR-1254-3


R.T.: 7.787 min
Delta R.T.: 0.014 min
Response: 30005
Conc: 18.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

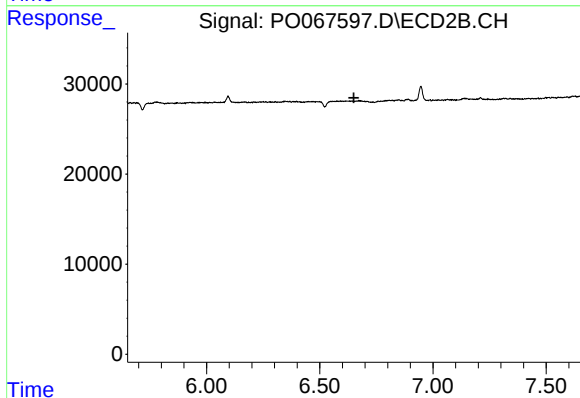


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.650 min
Response: 0
Conc: N.D.

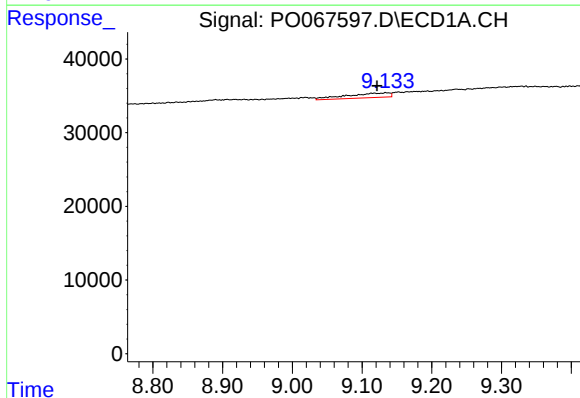


#35 AR-1260-5

R.T.: 9.134 min
Delta R.T.: 0.013 min
Response: 27289
Conc: 8.65 ng/ml

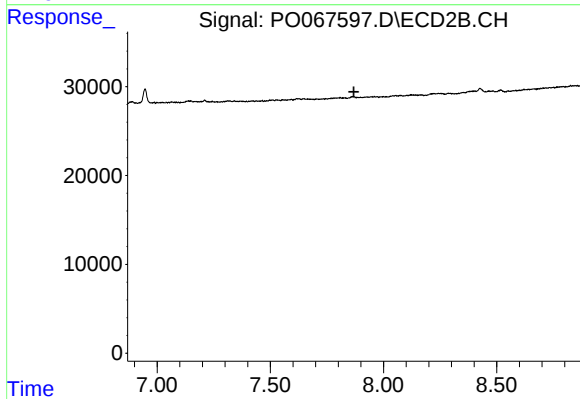

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.869 min
Response: 0
Conc: N.D.

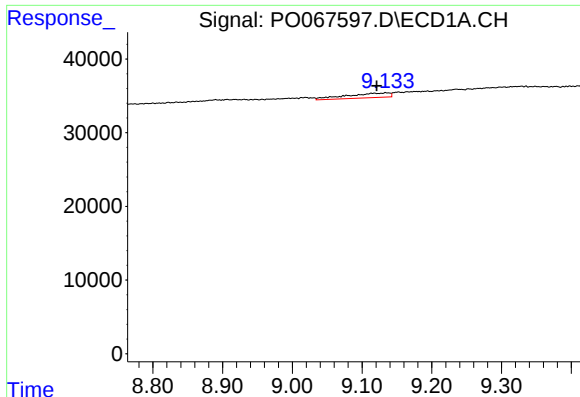

#37 AR-1262-2


R.T.: 9.134 min
Delta R.T.: 0.013 min
Response: 27289
Conc: 9.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

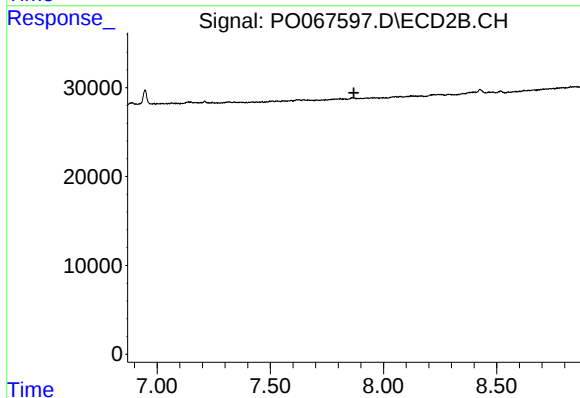


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.869 min
Response: 0
Conc: N.D.

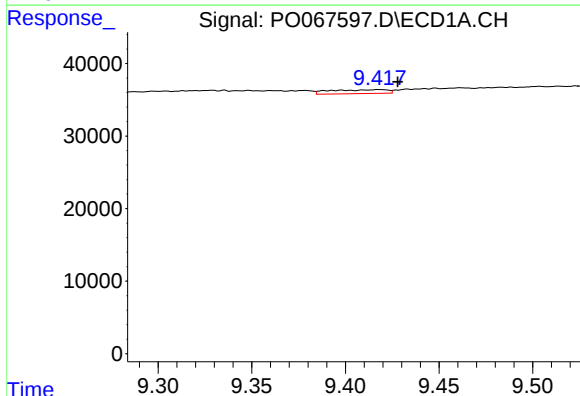


#38 AR-1262-3

R.T.: 9.418 min
Delta R.T.: -0.010 min
Response: 11253
Conc: 5.41 ng/ml

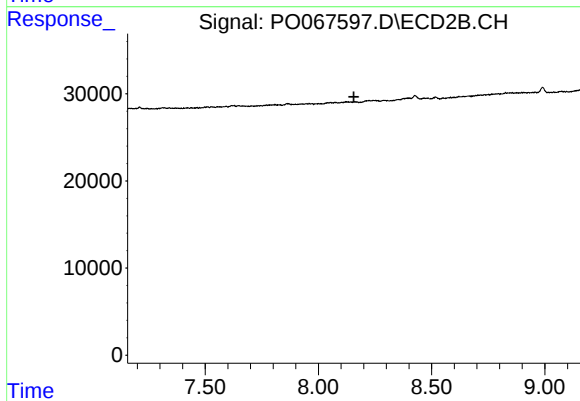

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.157 min
Response: 0
Conc: N.D.

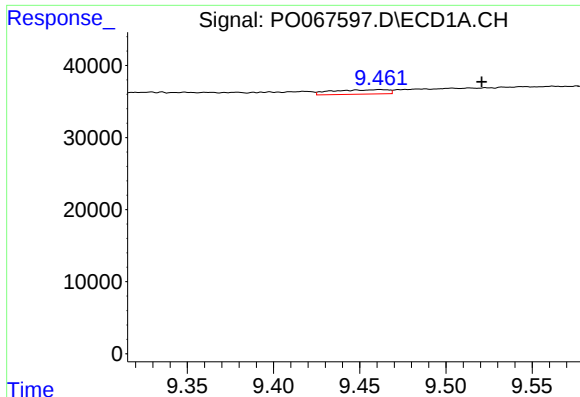

#39 AR-1262-4


R.T.: 9.462 min
Delta R.T.: -0.059 min
Response: 13715
Conc: 8.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

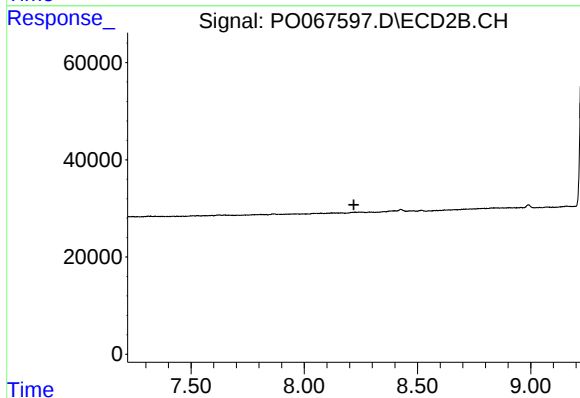


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.219 min
Response: 0
Conc: N.D.

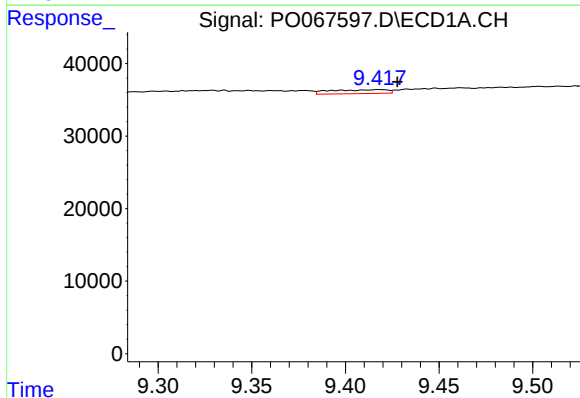


#41 AR-1268-1

R.T.: 9.418 min
Delta R.T.: -0.010 min
Response: 11253
Conc: 3.05 ng/ml

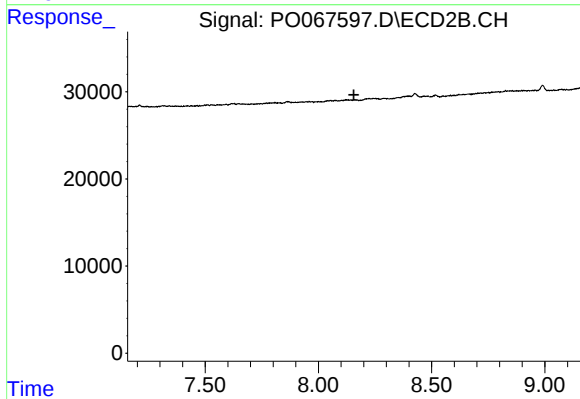

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.156 min
Response: 0
Conc: N.D.

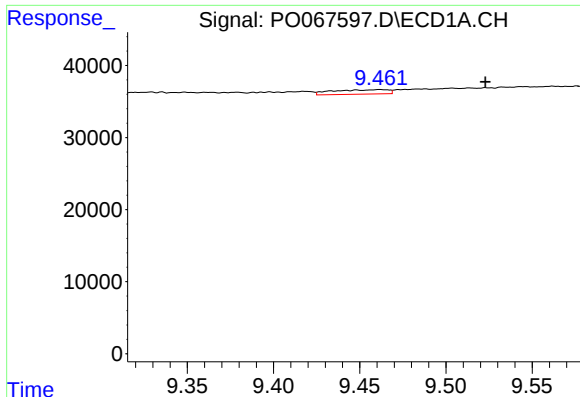

#42 AR-1268-2

R.T.: 9.462 min
Delta R.T.: -0.061 min
Response: 13715
Conc: 3.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

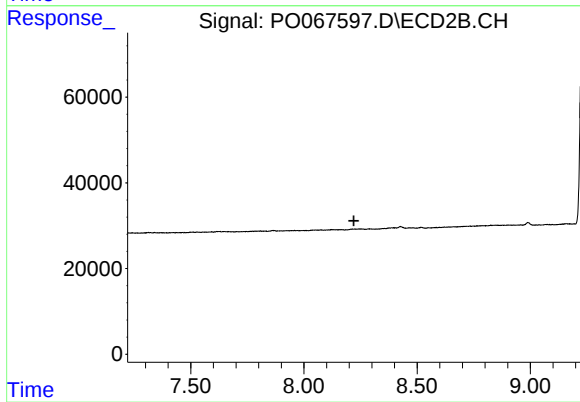

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.221 min
Response: 0
Conc: N.D.