

Data Path : P:\HPCHEM1\ECD_0\Data\P0040218\
Data File : P0043466.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2018 1:07
Operator : SM/UA
Sample : J2114-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
032718-TIDO-E-U-S

Manual Integrations
APPROVED

UGO
4/3/2018 5:08:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:25:44 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040218.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 03 01:50:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.065	3.320	9196466	12594127	16.551m	16.322
2)	SA Decachlor...	9.416	8.090	8414996	11550293	17.038	17.418

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0040218\
Data File : P0043466.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2018 1:07
Operator : SM/UA
Sample : J2114-10
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
032718-TIDO-E-U-S


Manual Integrations
APPROVED

UGO
4/3/2018 5:08:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:25:44 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040218.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 03 01:50:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

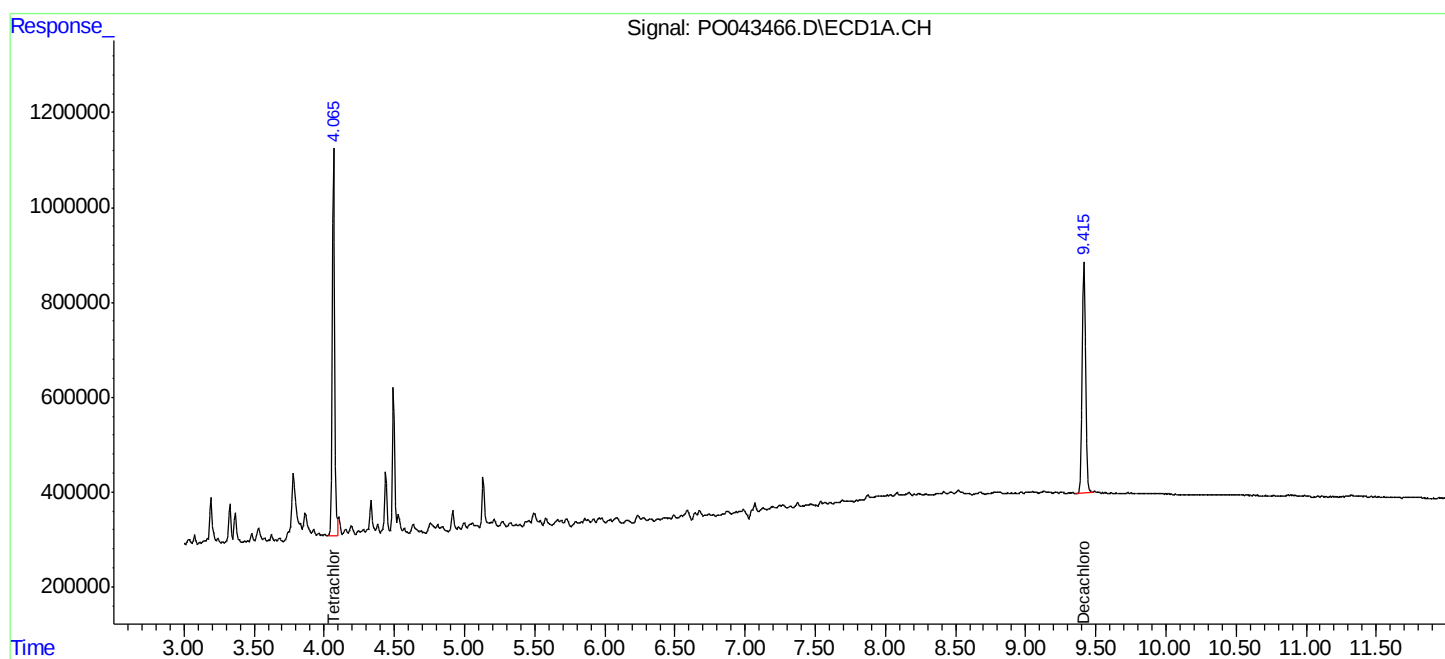

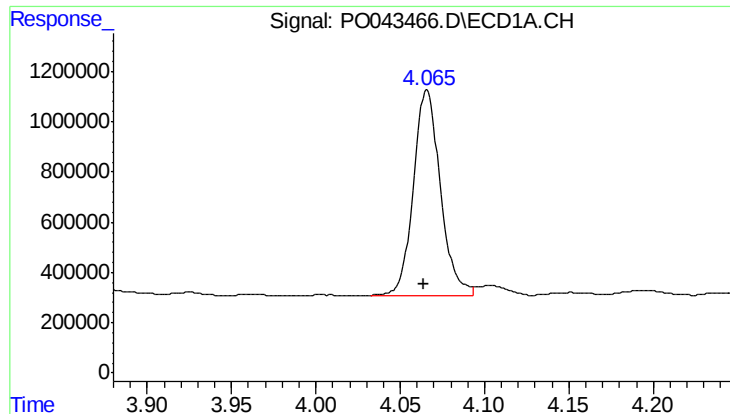


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: 0.001 min
Response: 9196466
Conc: 16.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
032718-TIDO-E-U-S


Manual Integrations
APPROVED

UGO
4/3/2018 5:08:09 PM

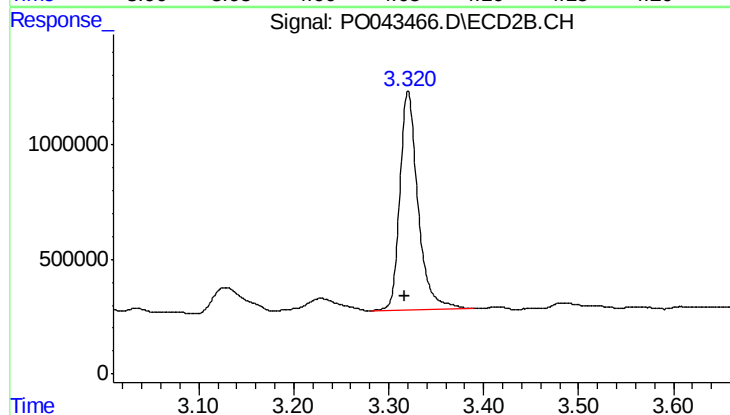


#1 Tetrachloro-m-xylene

R.T.: 3.320 min
Delta R.T.: 0.004 min
Response: 12594127
Conc: 16.32 ng/ml

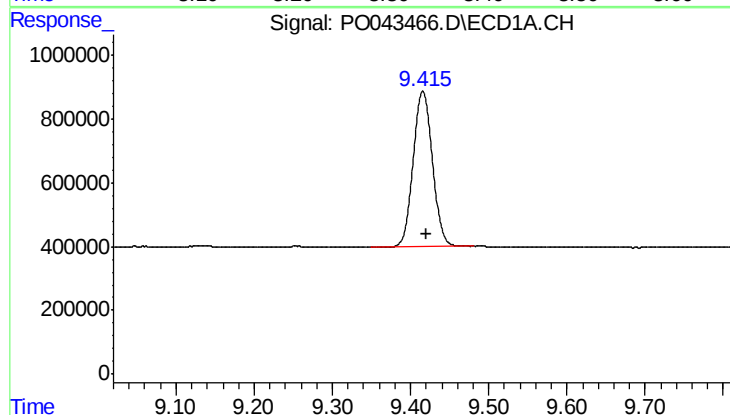

#2 Decachlorobiphenyl

R.T.: 9.416 min
Delta R.T.: -0.004 min
Response: 8414996
Conc: 17.04 ng/ml

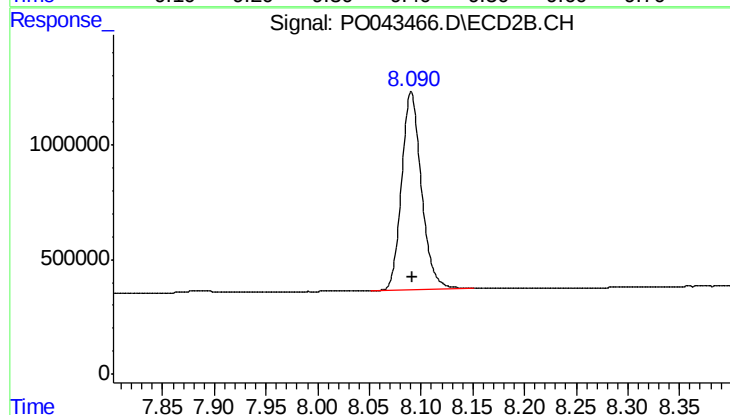

#2 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: -0.002 min
Response: 11550293
Conc: 17.42 ng/ml