

Data Path : P:\HPCHEM1\ECD_0\Data\P0040218\
Data File : P0043470.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2018 2:07
Operator : SM/UA
Sample : J2114-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
032718-SIDI-E-U-B

Manual Integrations
APPROVED

UGO
4/3/2018 5:07:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 07:14:16 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040218.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 03 01:50:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.066	3.320	8868263	12337019	15.960m	15.989
2)	SA Decachlor...	9.416	8.091	7607103	10281389	15.403	15.505

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0040218\
Data File : P0043470.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2018 2:07
Operator : SM/UA
Sample : J2114-14
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
032718-SIDI-E-U-B


Manual Integrations
APPROVED

UGO
4/3/2018 5:07:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 07:14:16 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040218.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 03 01:50:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

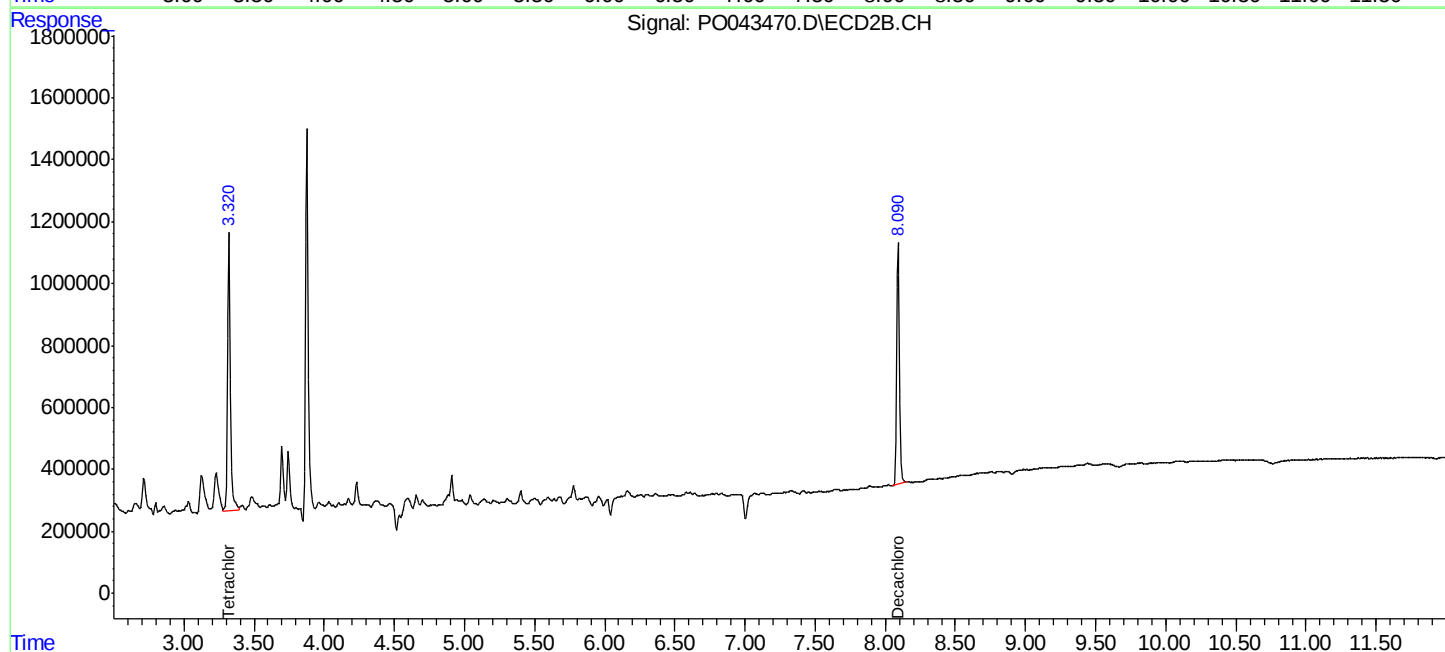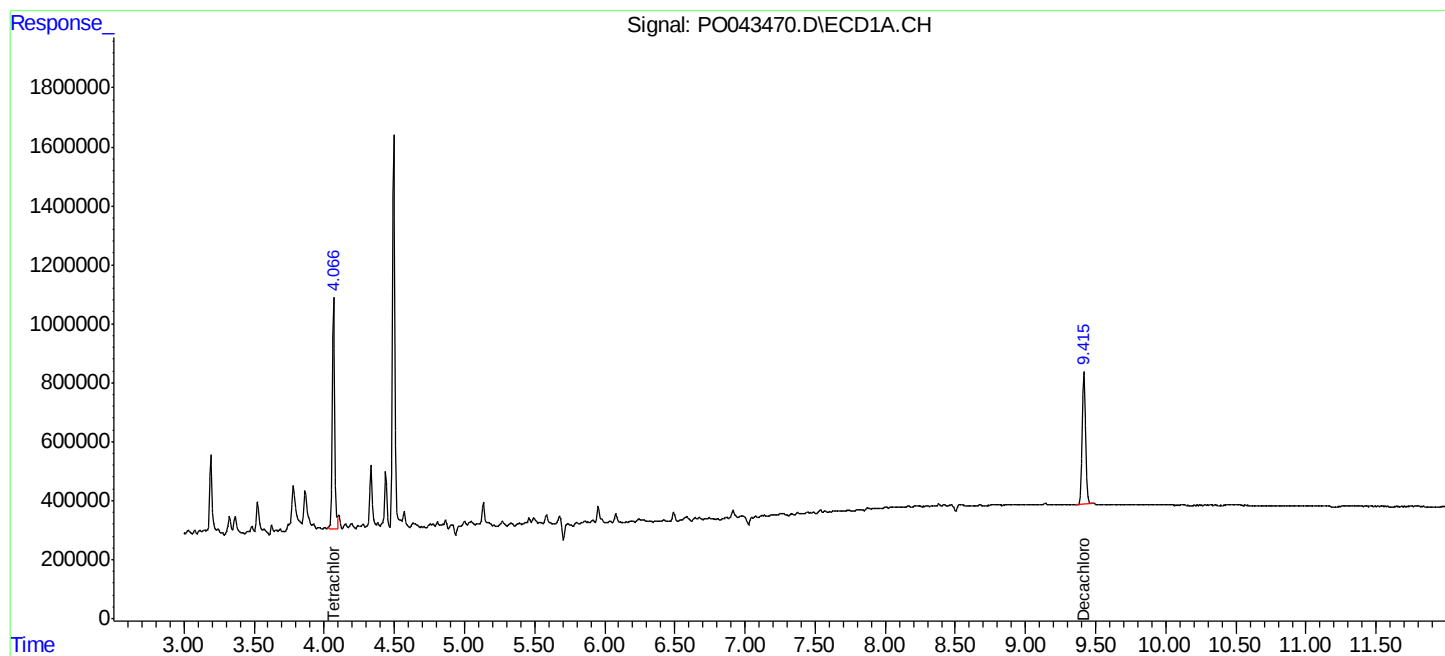

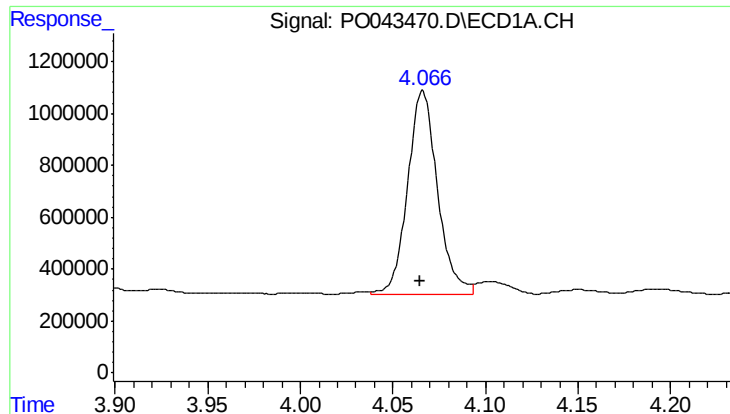


#1 Tetrachloro-m-xylene

R.T.: 4.066 min
Delta R.T.: 0.001 min
Response: 8868263
Conc: 15.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
032718-SIDI-E-U-B


Manual Integrations
APPROVED

UGO
4/3/2018 5:07:19 PM

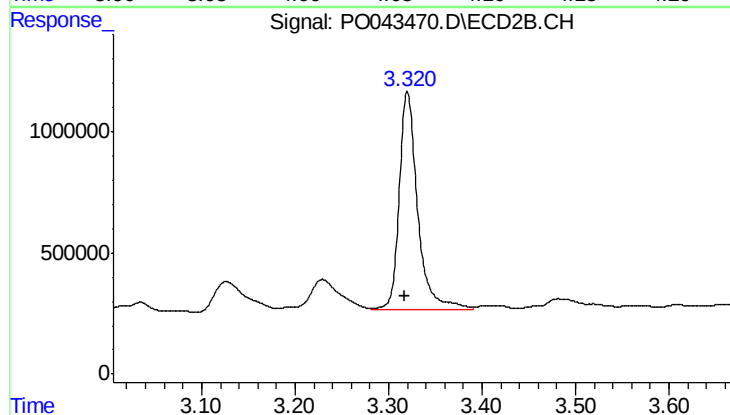


#1 Tetrachloro-m-xylene

R.T.: 3.320 min
Delta R.T.: 0.003 min
Response: 12337019
Conc: 15.99 ng/ml

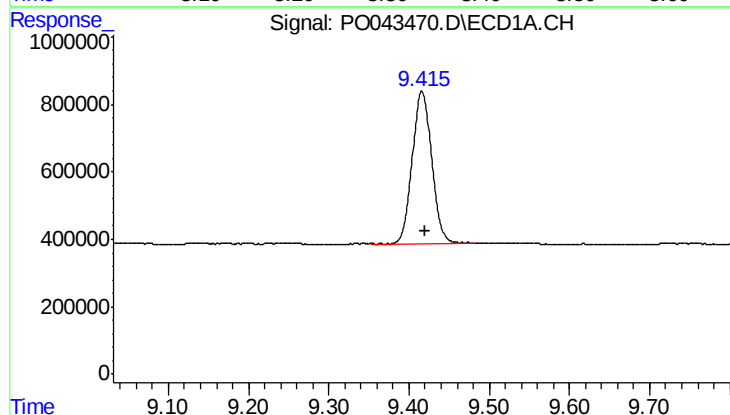

#2 Decachlorobiphenyl

R.T.: 9.416 min
Delta R.T.: -0.004 min
Response: 7607103
Conc: 15.40 ng/ml

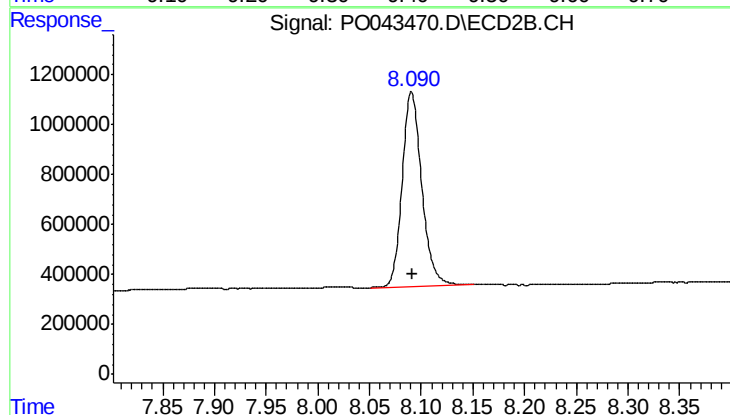

#2 Decachlorobiphenyl

R.T.: 8.091 min
Delta R.T.: -0.001 min
Response: 10281389
Conc: 15.50 ng/ml