

Data Path : P:\HPCHEM1\ECD_0\Data\P0040218\
 Data File : P0043479.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Apr 2018 4:22
 Operator : SM/UA
 Sample : J2113-02
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 032618-TIDO-E-D-S

Manual Integrations
 APPROVED

UGO
 4/3/2018 5:06:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 07:25:27 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0040218.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 03 01:50:04 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.065	3.318	10610140	14037952	19.095	18.193m
2) SA Decachlor...	9.414	8.090	9779044	13607803	19.800	20.521

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0040218\
Data File : P0043479.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2018 4:22
Operator : SM/UA
Sample : J2113-02
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
032618-TIDO-E-D-S


Manual Integrations
APPROVED

UGO
4/3/2018 5:06:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 07:25:27 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040218.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 03 01:50:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

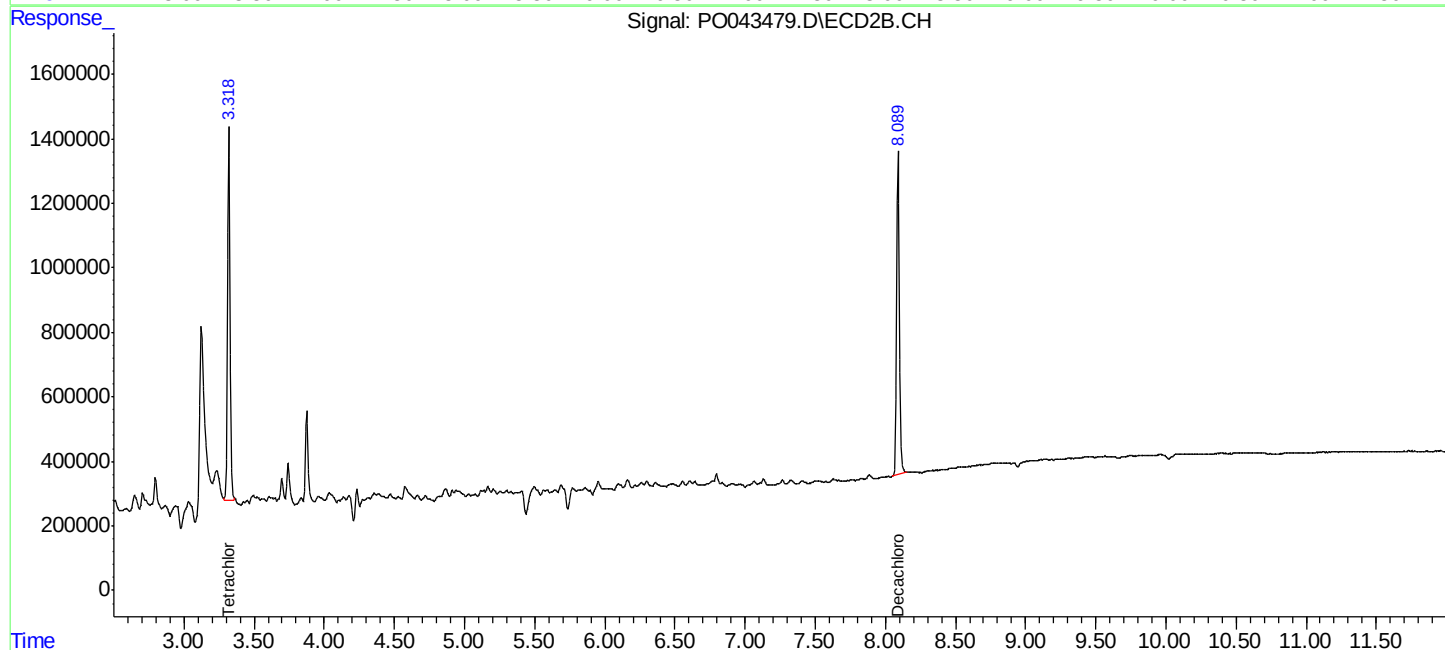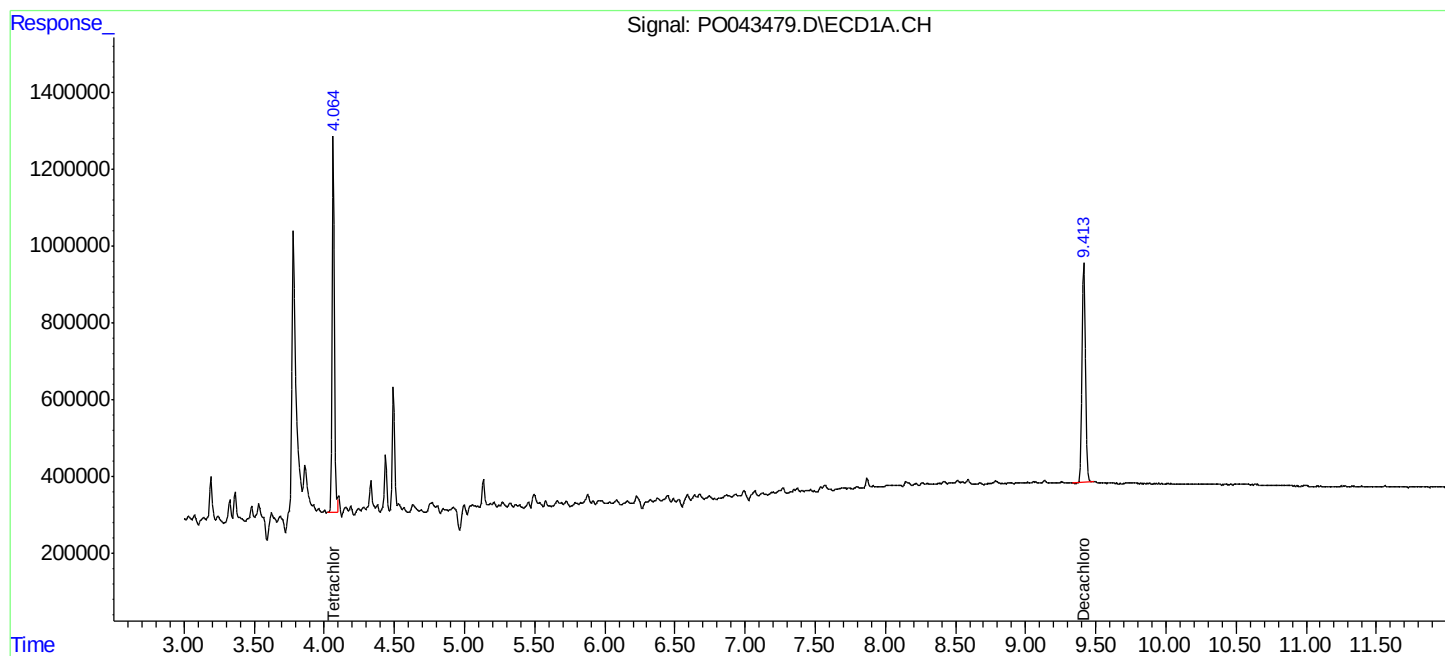

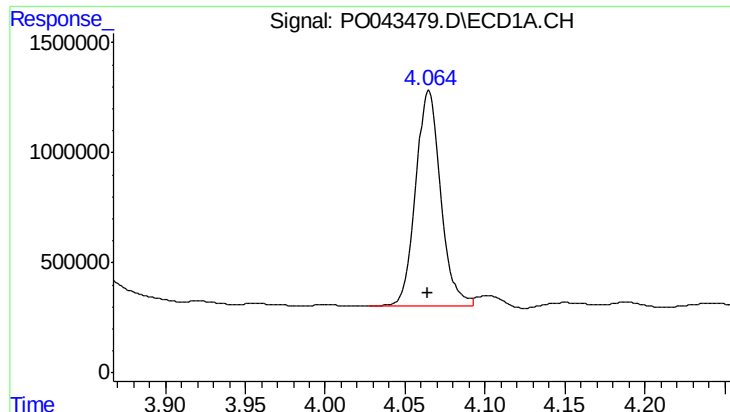


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: 0.000 min
Response: 10610140
Conc: 19.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
032618-TIDO-E-D-S


Manual Integrations
APPROVED

UGO
4/3/2018 5:06:58 PM

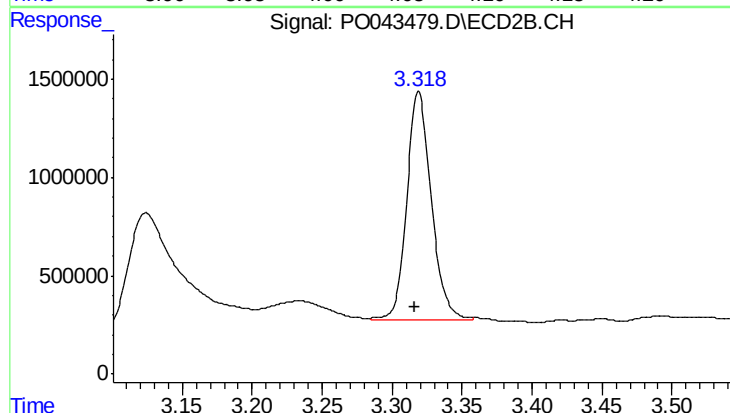


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.002 min
Response: 14037952
Conc: 18.19 ng/ml m

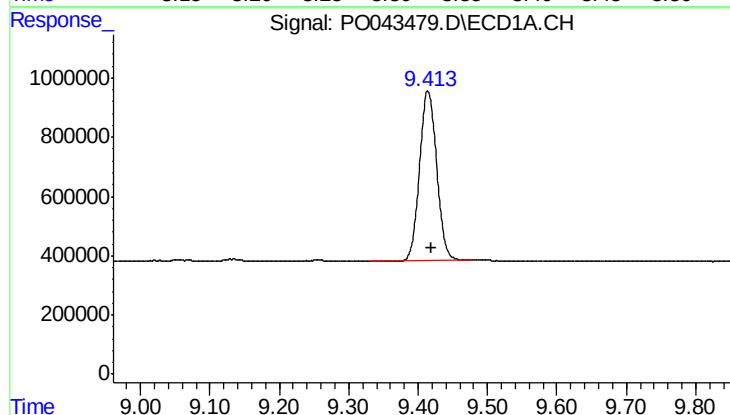

#2 Decachlorobiphenyl

R.T.: 9.414 min
Delta R.T.: -0.006 min
Response: 9779044
Conc: 19.80 ng/ml

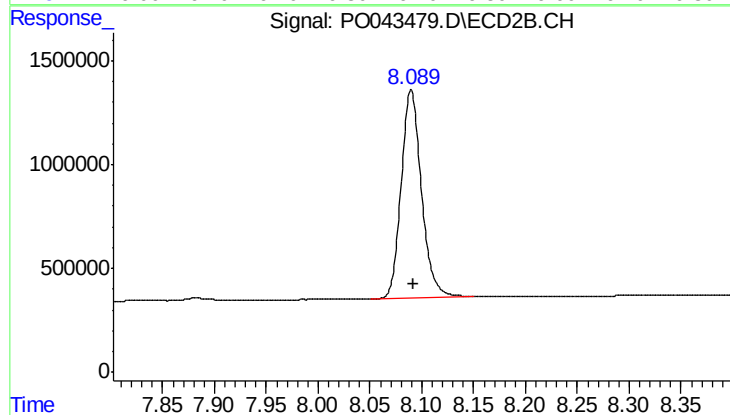

#2 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: -0.002 min
Response: 13607803
Conc: 20.52 ng/ml