

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040219\
 Data File : P0054806.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2019 11:40
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 13:49:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.302	3.618	900673	885757	25.952	27.756
2)	SA Decachlor...	9.920	8.591	824510	564203	16.725	17.715
Target Compounds							
9)	L2 AR-1221-2	0.000	3.916	0	11485	N.D.	38.311 #
20)	L4 AR-1242-5	0.000	5.519	0	9247	N.D.	7.519 #
25)	L5 AR-1248-5	0.000	5.519	0	9247	N.D.	6.202 #
26)	L6 AR-1254-1	0.000	5.519	0	9247	N.D.	4.231 #
32)	L7 AR-1260-2	0.000	6.350	0	12248	N.D.	4.450 #
35)	L7 AR-1260-5	0.000	7.219	0	8829	N.D.	1.843 #
37)	L8 AR-1262-2	0.000	7.219	0	8829	N.D.	1.801 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040219\
Data File : PO054806.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2019 11:40
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 13:49:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

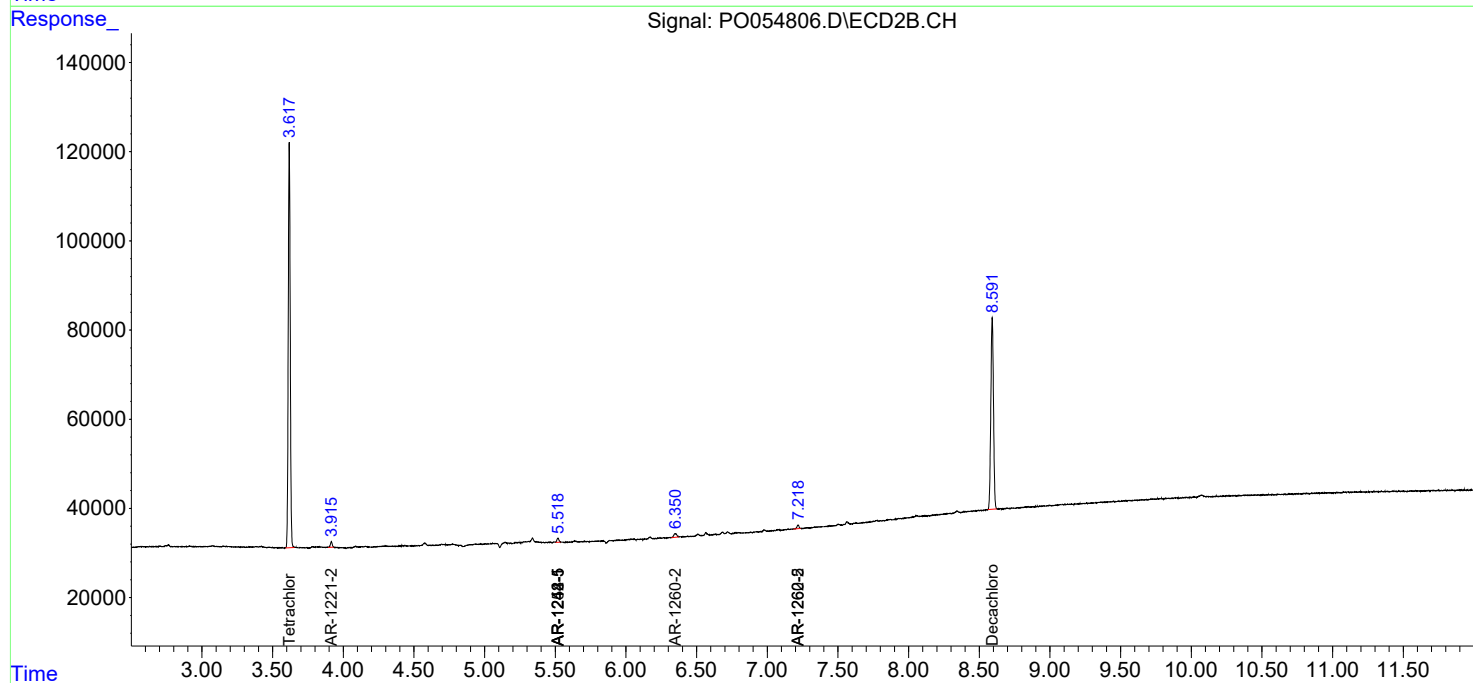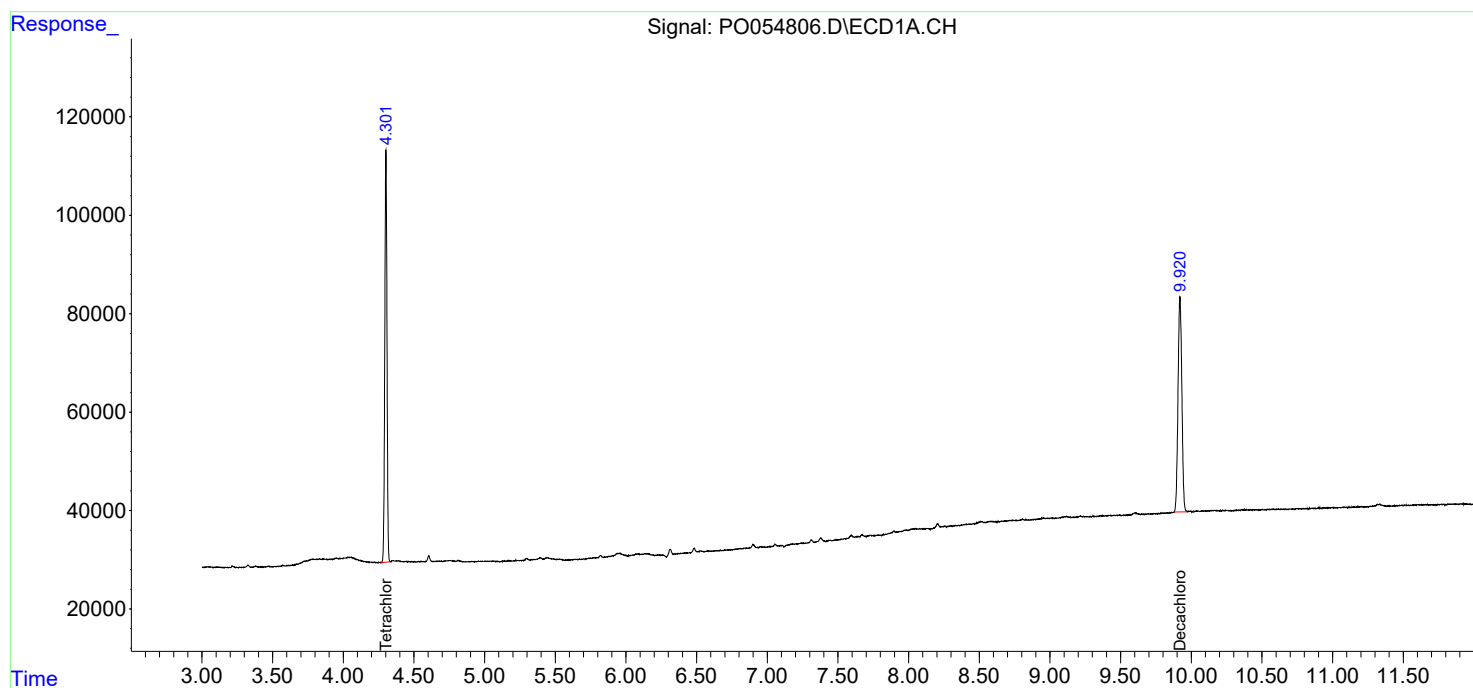


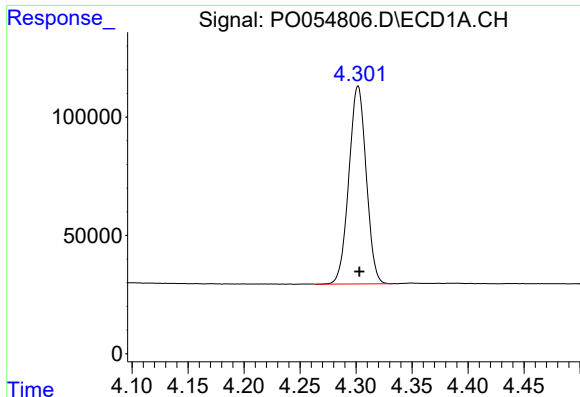

#1 Tetrachloro-m-xylene


R.T.: 4.302 min
Delta R.T.: -0.001 min
Response: 900673
Conc: 25.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

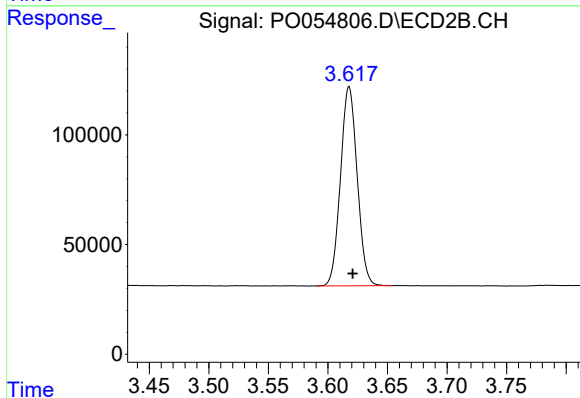


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: -0.003 min
Response: 885757
Conc: 27.76 ng/ml

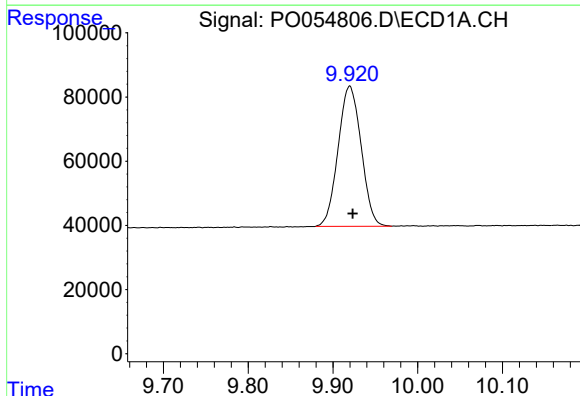


#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.003 min
Response: 824510
Conc: 16.73 ng/ml

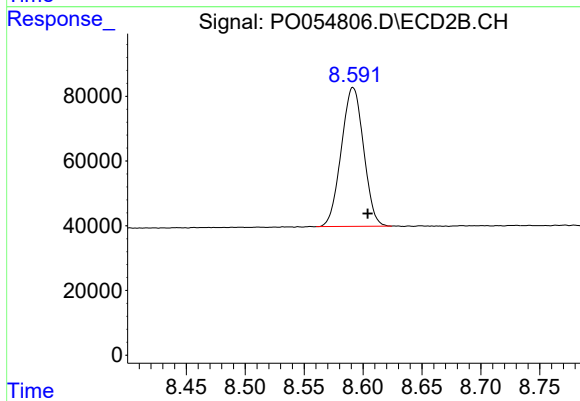

#2 Decachlorobiphenyl


R.T.: 8.591 min
Delta R.T.: -0.013 min
Response: 564203
Conc: 17.72 ng/ml

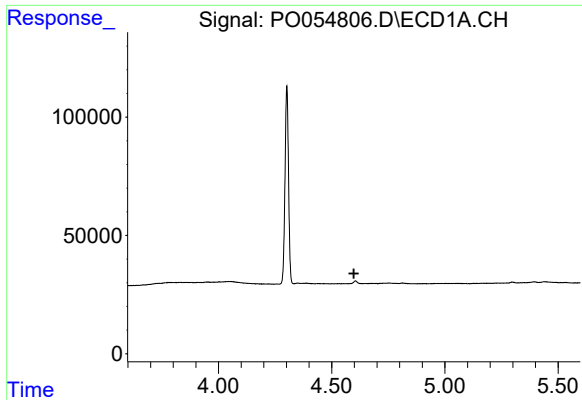

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.598 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

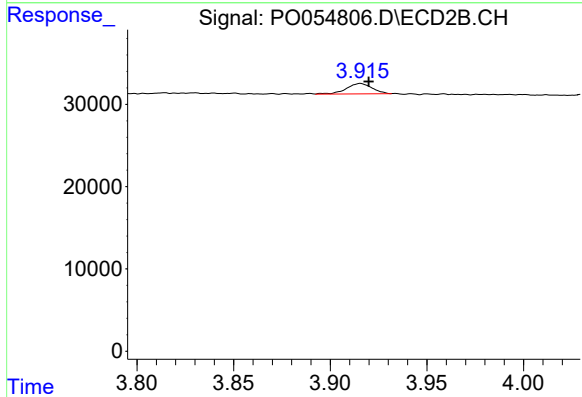


#9 AR-1221-2

R.T.: 3.916 min
Delta R.T.: -0.004 min
Response: 11485
Conc: 38.31 ng/ml

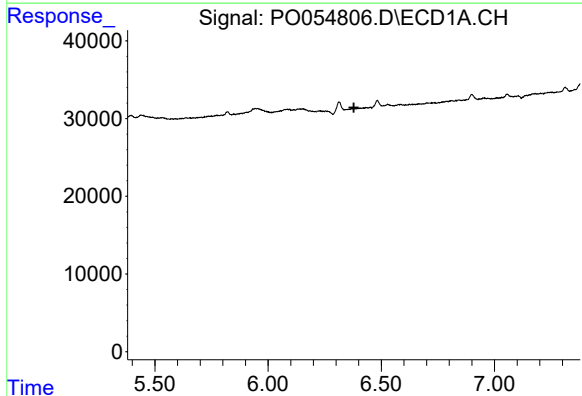


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.379 min
Response: 0
Conc: N.D.

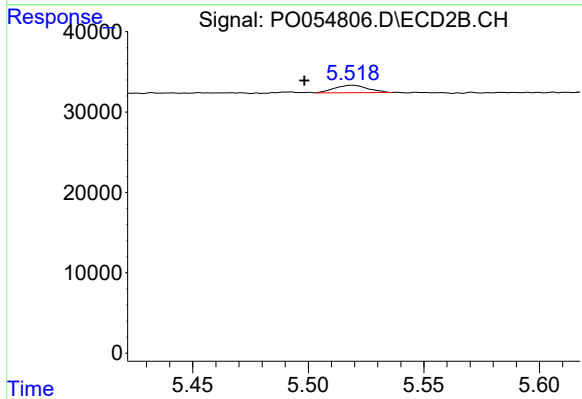

#20 AR-1242-5


R.T.: 5.519 min
Delta R.T.: 0.021 min
Response: 9247
Conc: 7.52 ng/ml

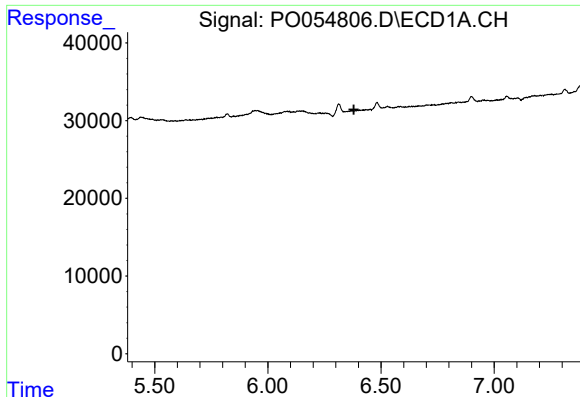

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.380 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

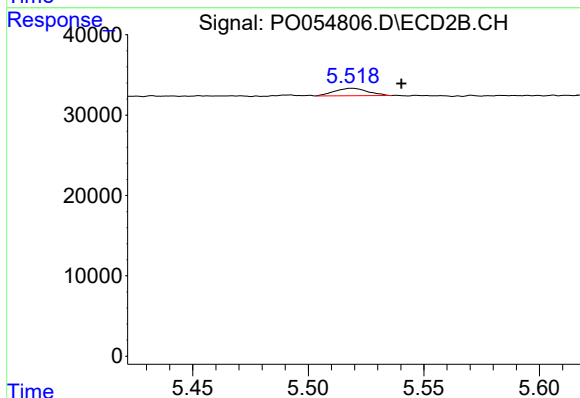


#25 AR-1248-5

R.T.: 5.519 min
Delta R.T.: -0.021 min
Response: 9247
Conc: 6.20 ng/ml

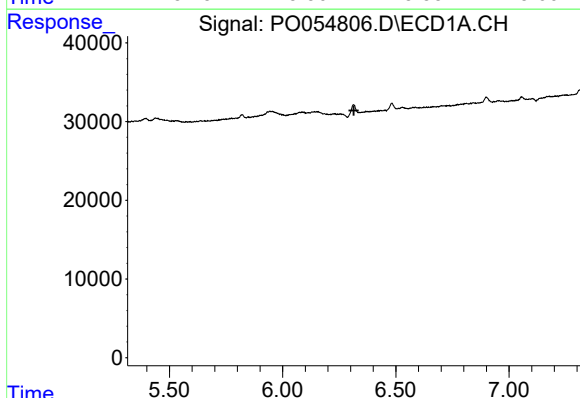


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.315 min
Response: 0
Conc: N.D.

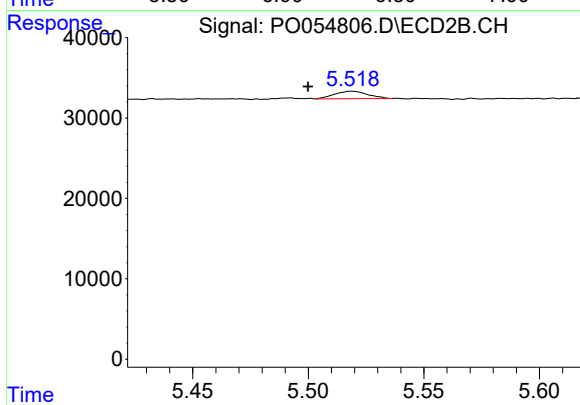

#26 AR-1254-1


R.T.: 5.519 min
Delta R.T.: 0.019 min
Response: 9247
Conc: 4.23 ng/ml

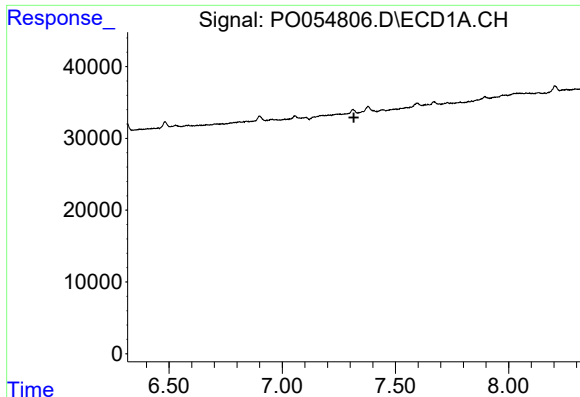

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

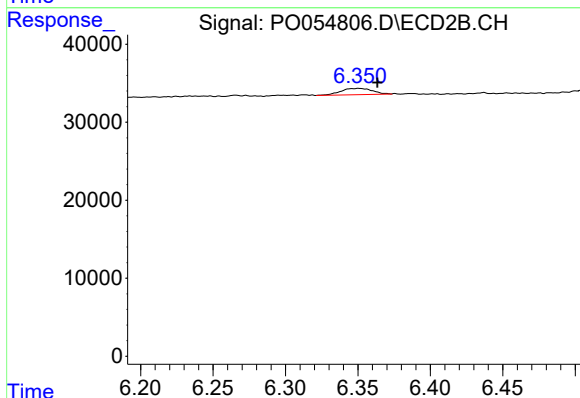


#32 AR-1260-2

R.T.: 6.350 min
Delta R.T.: -0.013 min
Response: 12248
Conc: 4.45 ng/ml

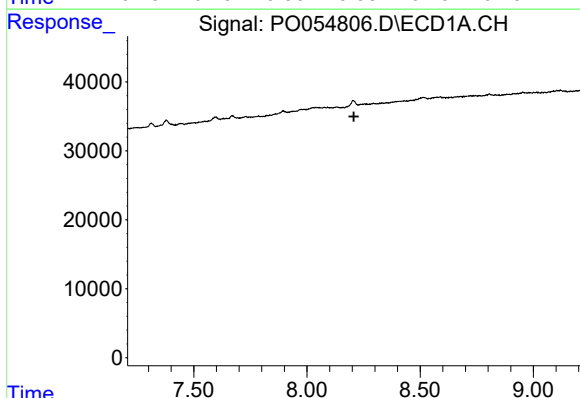


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.207 min
Response: 0
Conc: N.D.

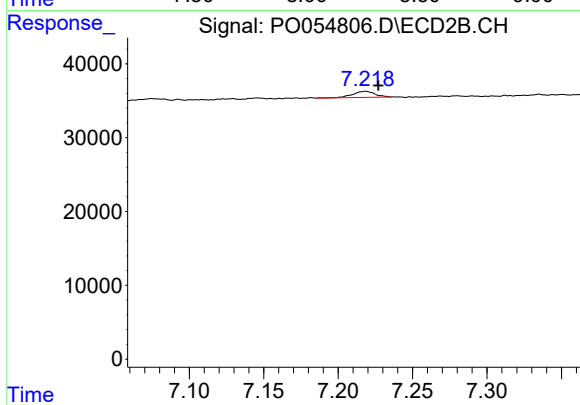

#35 AR-1260-5


R.T.: 7.219 min
Delta R.T.: -0.008 min
Response: 8829
Conc: 1.84 ng/ml

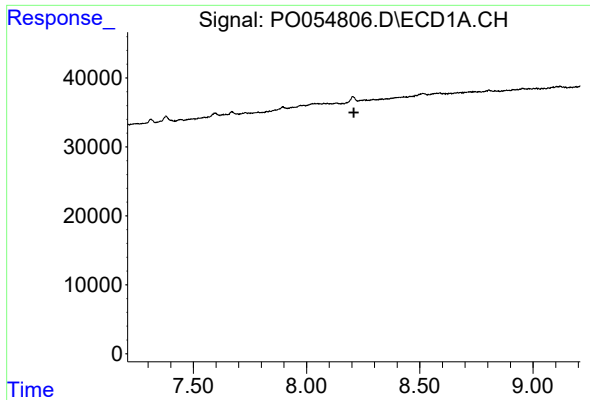

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.209 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

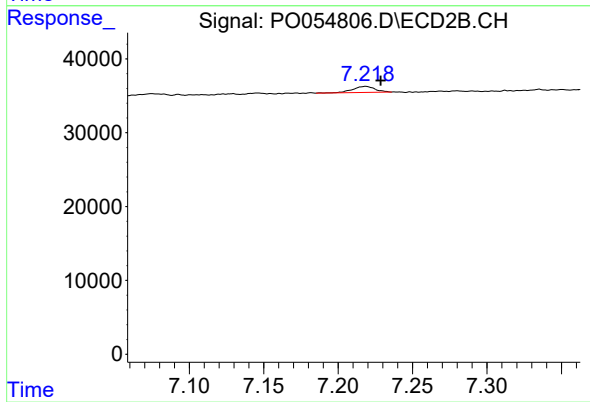

#37 AR-1262-2

R.T.: 7.219 min
Delta R.T.: -0.010 min
Response: 8829
Conc: 1.80 ng/ml