

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040219\
 Data File : P0054817.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2019 15:19
 Operator : SM/SJ
 Sample : K2208-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 INFL-3

Manual Integrations
 APPROVED

Sohil
 4/3/2019 5:47:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 15:38:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.301	3.628	585231	911836	16.863	28.573m#
2) SA Decachlor...	9.917	8.591	527591	383381	10.702m	12.038m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040219\
Data File : PO054817.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2019 15:19
Operator : SM/SJ
Sample : K2208-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
INFL-3


Manual Integrations
APPROVED

Sohil
4/3/2019 5:47:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 15:38:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

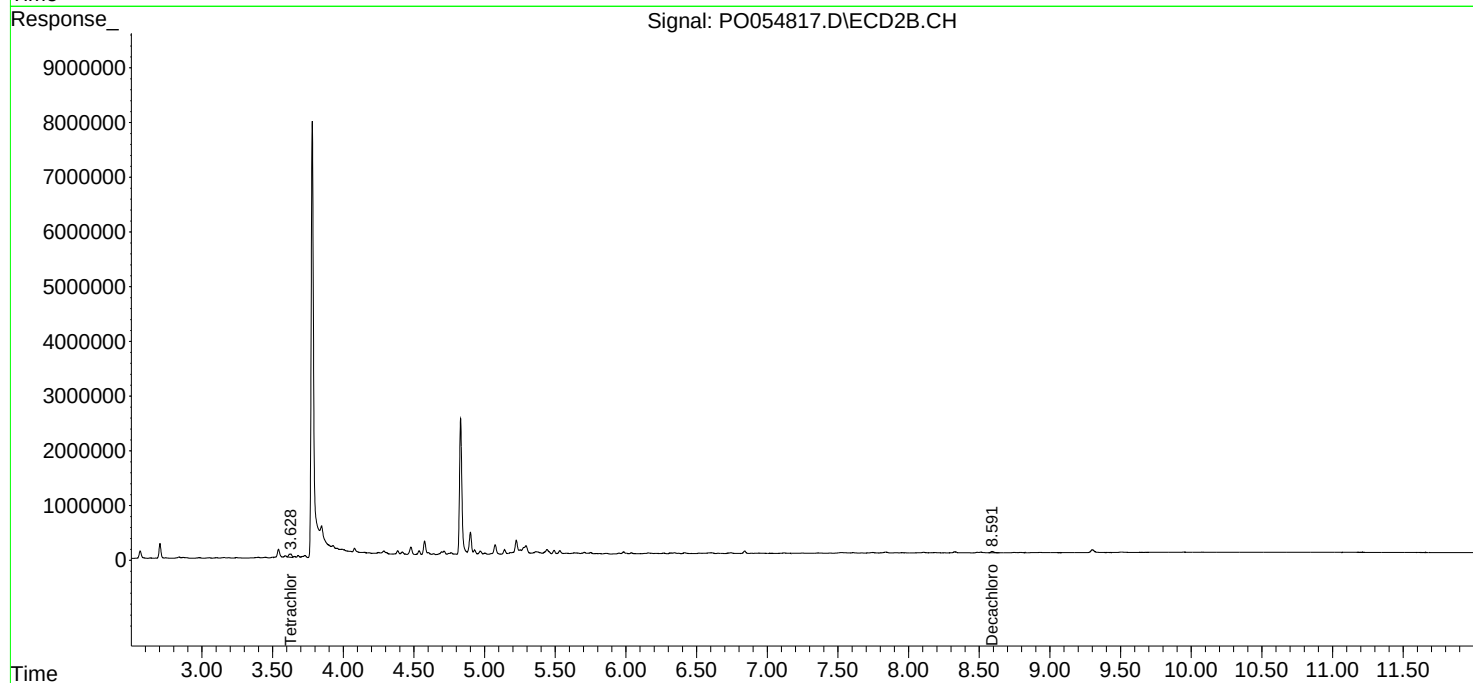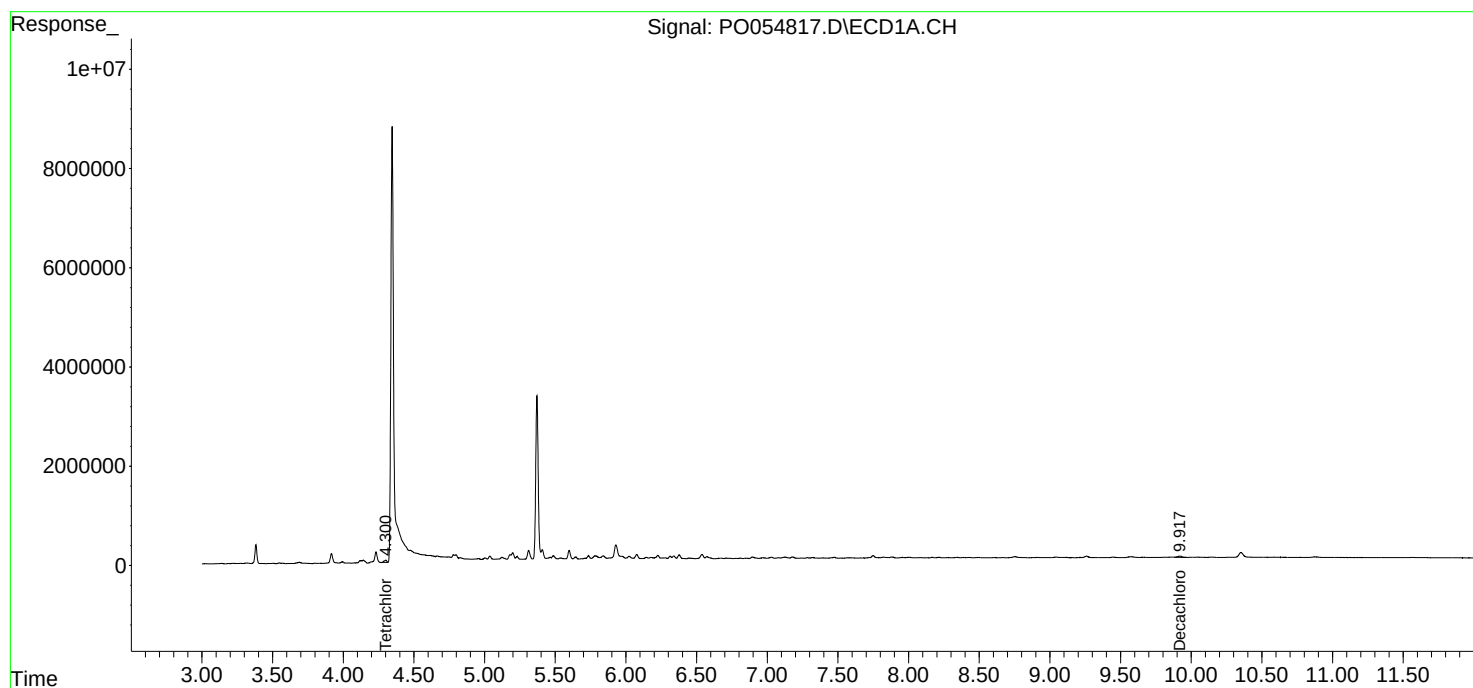

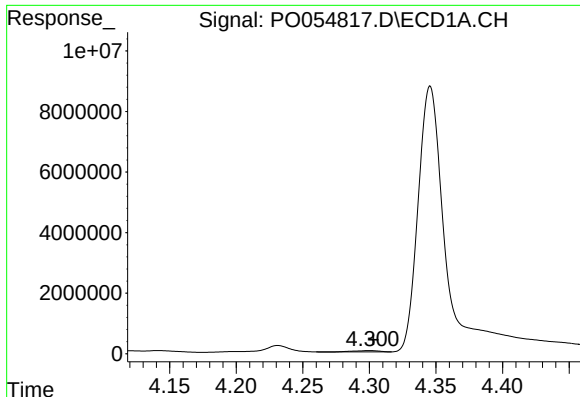


#1 Tetrachloro-m-xylene

R.T.: 4.301 min
Delta R.T.: -0.002 min
Response: 585231
Conc: 16.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
INFL-3


Manual Integrations
APPROVED

Sohil
4/3/2019 5:47:45 PM

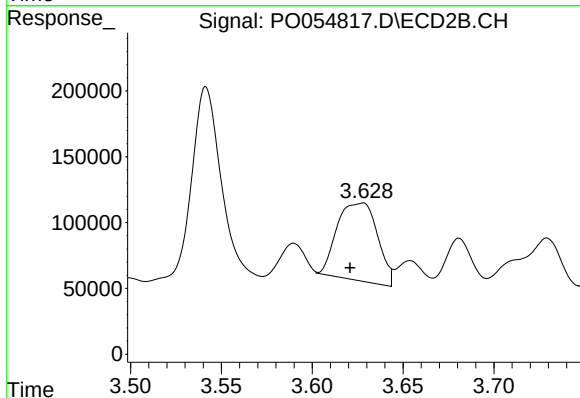


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: 0.007 min
Response: 911836
Conc: 28.57 ng/ml m

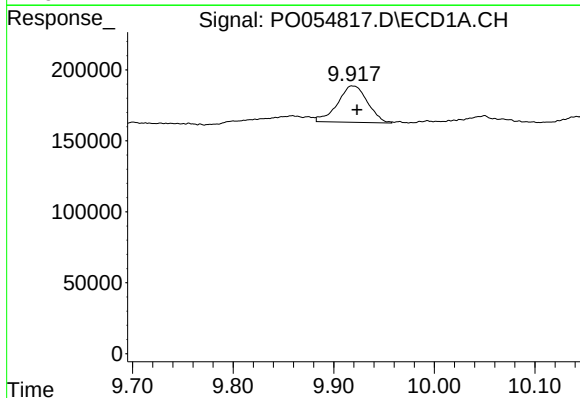

#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.006 min
Response: 527591
Conc: 10.70 ng/ml m

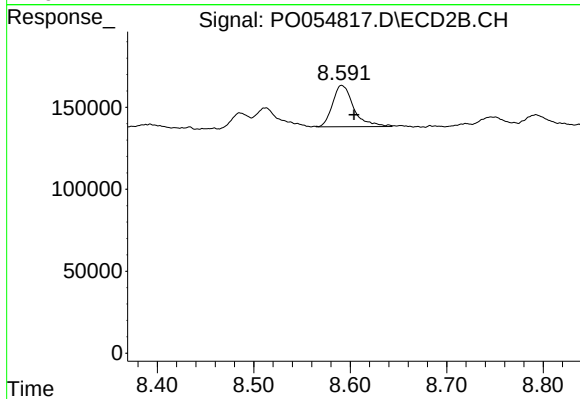

#2 Decachlorobiphenyl

R.T.: 8.591 min
Delta R.T.: -0.013 min
Response: 383381
Conc: 12.04 ng/ml m