

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040219\
 Data File : P0054868.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Apr 2019 6:07
 Operator : SM/SJ
 Sample : K2182-09
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S7C(12-20)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 07:26:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.302	3.618	1403131	1346735	40.430	42.201
2) SA Decachlor...	9.922	8.592	1177117	829143	23.878	26.034

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040219\
Data File : P0054868.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2019 6:07
Operator : SM/SJ
Sample : K2182-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S7C(12-20)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 07:26:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

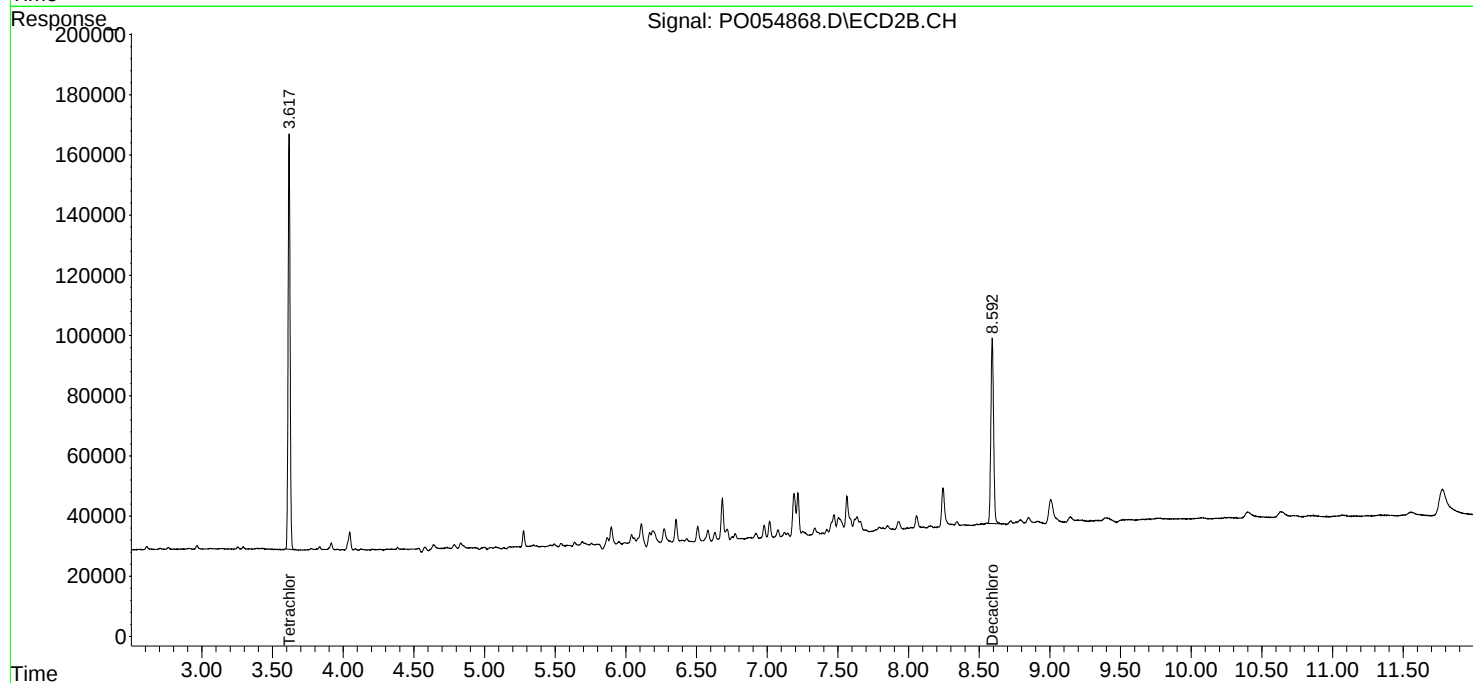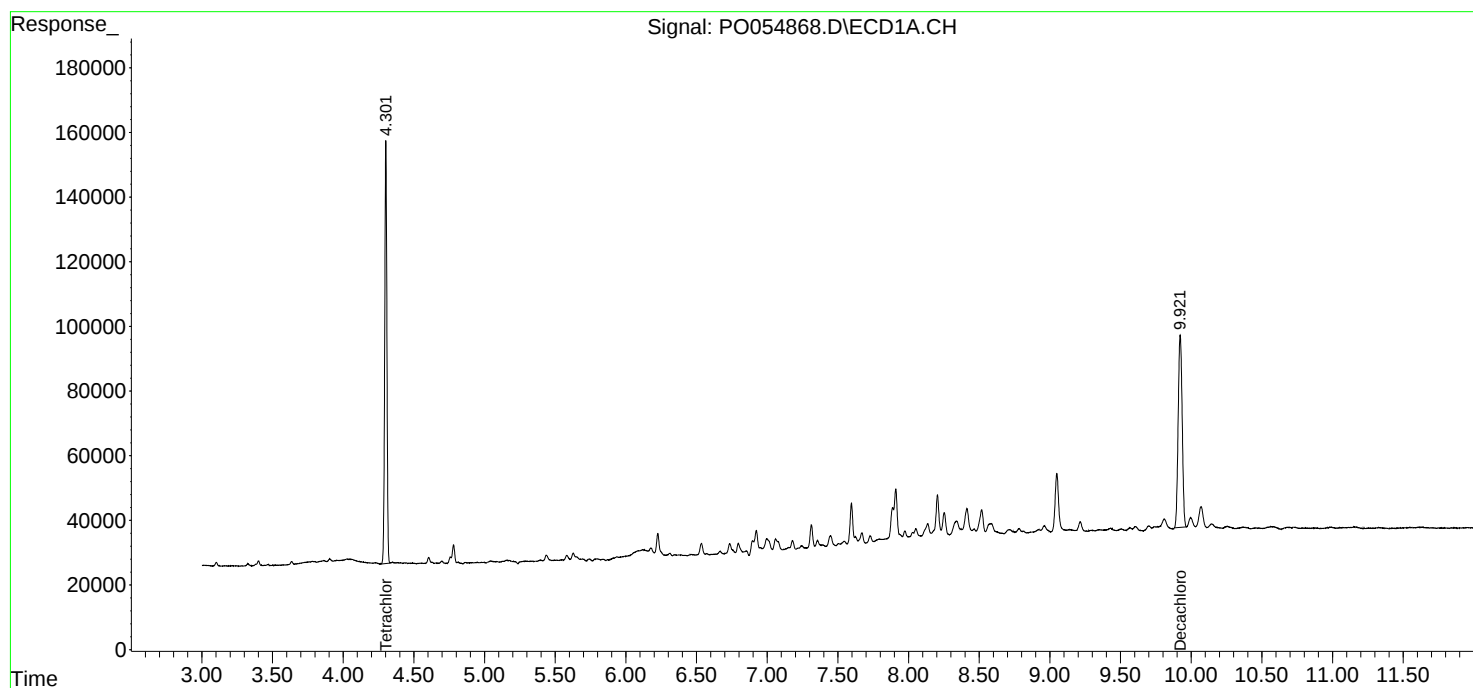


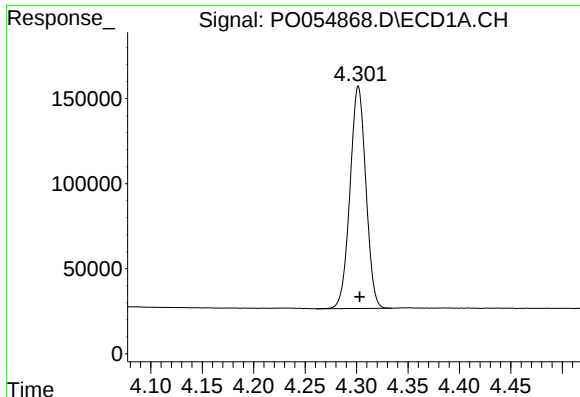

#1 Tetrachloro-m-xylene


R.T.: 4.302 min
Delta R.T.: -0.001 min
Response: 1403131
Conc: 40.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
S7C(12-20)COMP

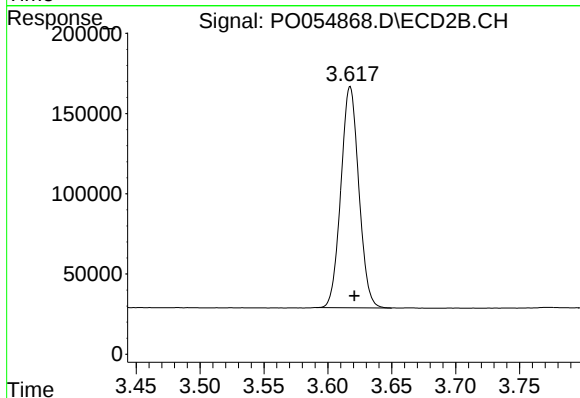


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: -0.003 min
Response: 1346735
Conc: 42.20 ng/ml

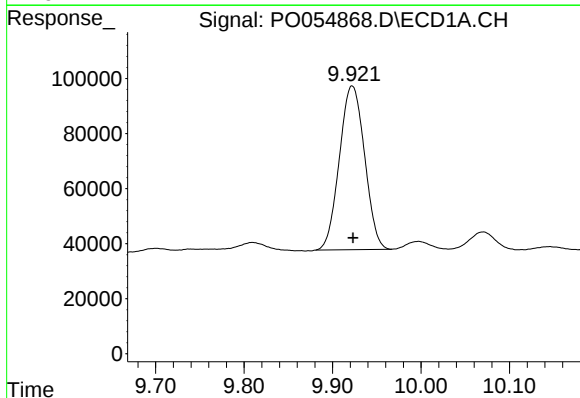

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: 0.000 min
Response: 1177117
Conc: 23.88 ng/ml

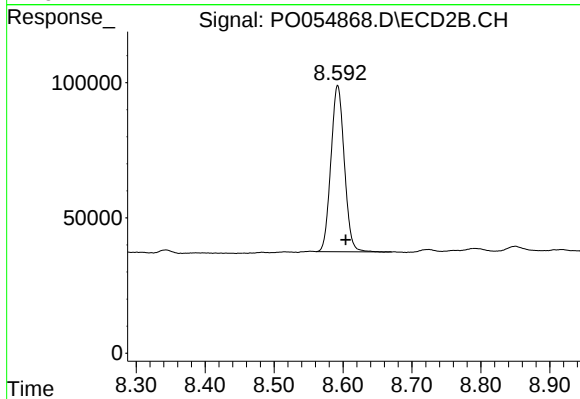

#2 Decachlorobiphenyl

R.T.: 8.592 min
Delta R.T.: -0.012 min
Response: 829143
Conc: 26.03 ng/ml