

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040220\
 Data File : P0067613.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2020 12:51
 Operator : DD\AJ
 Sample : L2085-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S12-04-A

Manual Integrations
 APPROVED

Sohil
 4/3/2020 3:22:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 14:03:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 01 17:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.935	3.943	494196	734000	20.752	21.899
2)	SA Decachlor...	10.920	9.230	461449	740145	13.555	17.901m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040220\
Data File : P0067613.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2020 12:51
Operator : DD\AJ
Sample : L2085-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S12-04-A


Manual Integrations
APPROVED

Sohil
4/3/2020 3:22:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 14:03:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 01 17:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

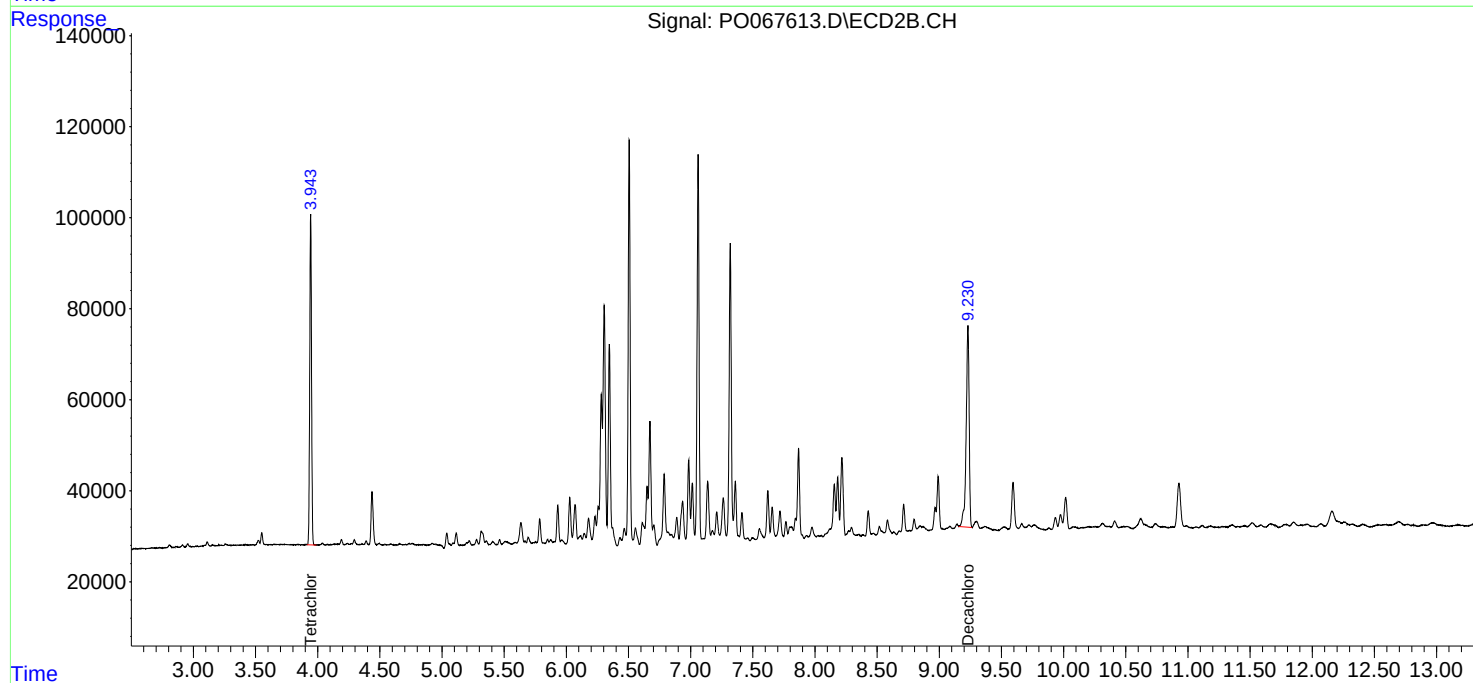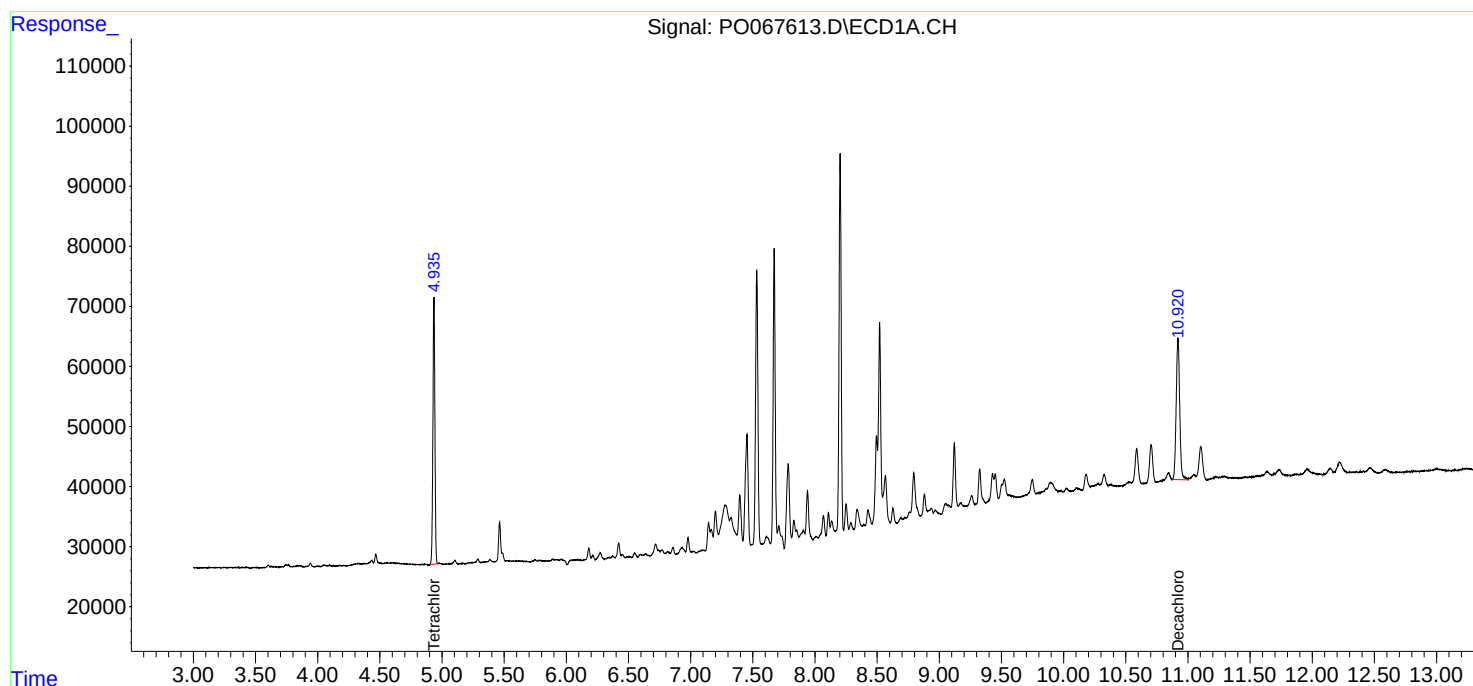

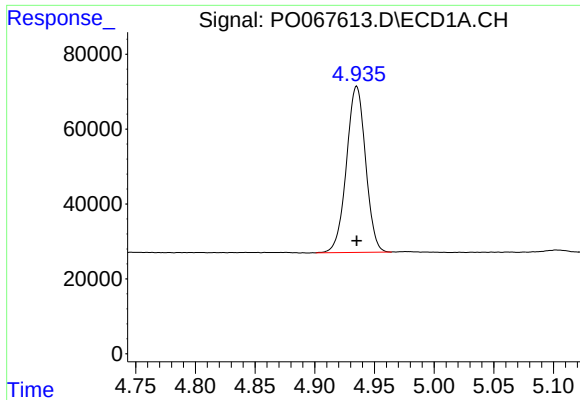


#1 Tetrachloro-m-xylene

R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 494196
Conc: 20.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-04-A


Manual Integrations
APPROVED

Sohil
4/3/2020 3:22:46 PM

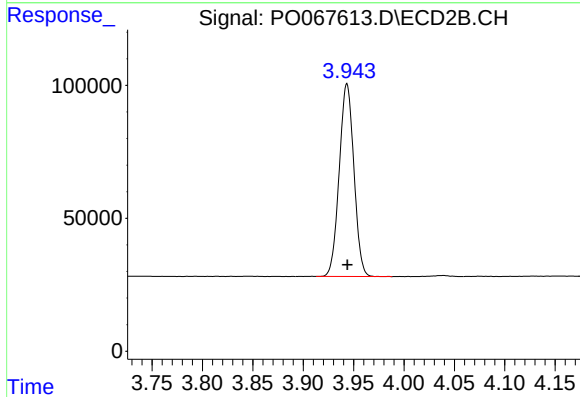


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 734000
Conc: 21.90 ng/ml

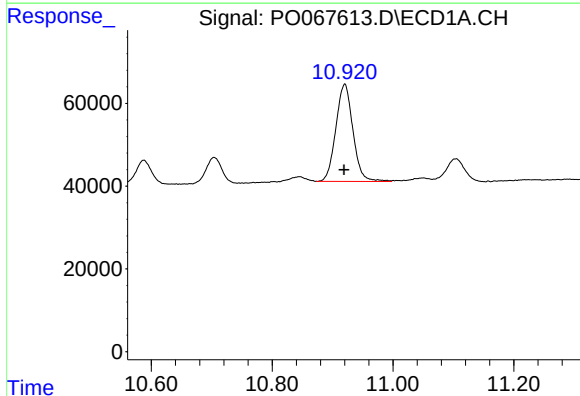

#2 Decachlorobiphenyl

R.T.: 10.920 min
Delta R.T.: 0.001 min
Response: 461449
Conc: 13.55 ng/ml

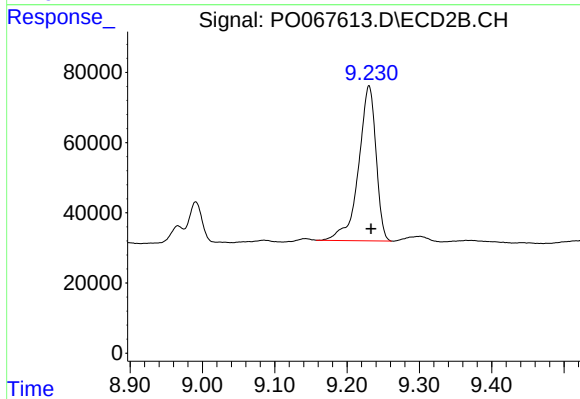

#2 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: -0.003 min
Response: 740145
Conc: 17.90 ng/ml m