

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040220\
 Data File : P0067620.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2020 14:50
 Operator : DD\AJ
 Sample : L2087-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-15

Manual Integrations
 APPROVED

Sohil
 4/3/2020 3:22:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 15:39:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 01 17:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.935	3.943	462922	665677	19.439	19.861
2) SA Decachlor...	10.921	9.231	666628	680534	19.582	16.460m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040220\
Data File : PO067620.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2020 14:50
Operator : DD\AJ
Sample : L2087-07
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DUP-15


Manual Integrations
APPROVED

Sohil
4/3/2020 3:22:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 15:39:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 01 17:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

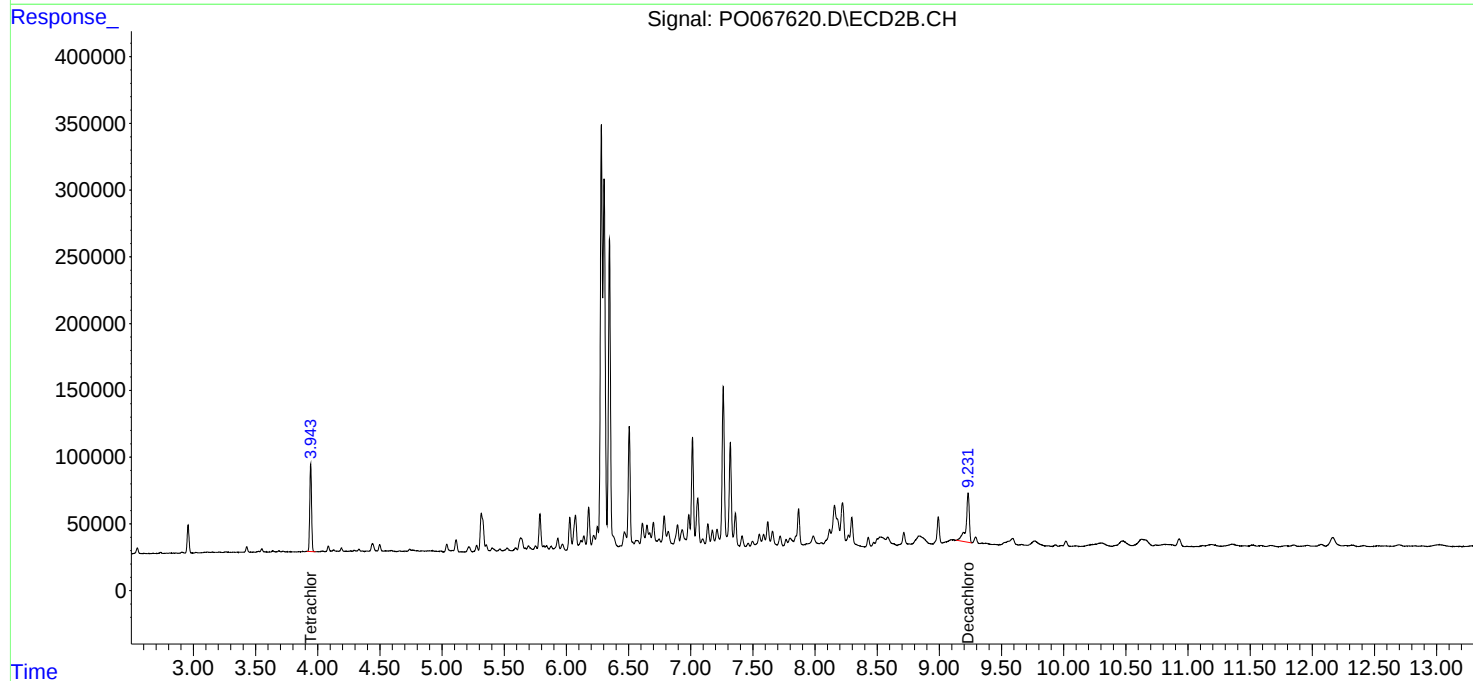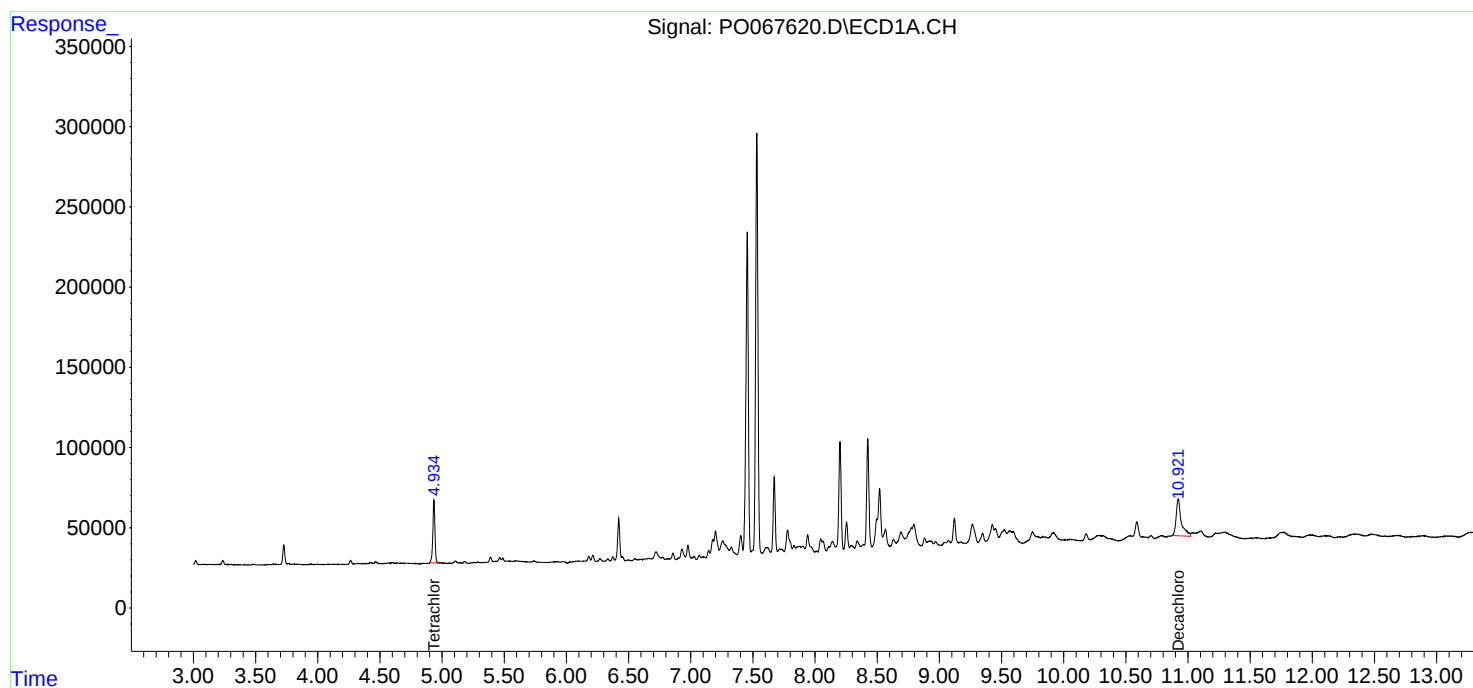

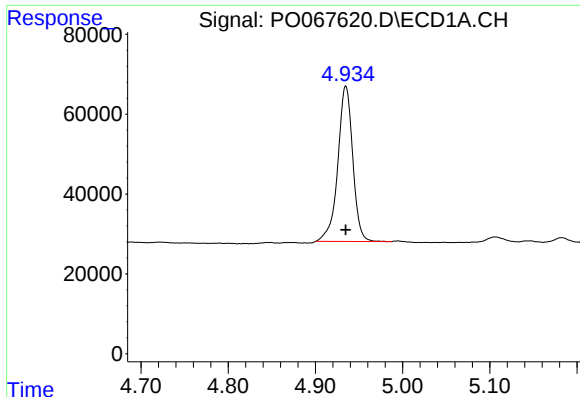


#1 Tetrachloro-m-xylene

R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 462922
Conc: 19.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-15


Manual Integrations
APPROVED

Sohil
4/3/2020 3:22:52 PM

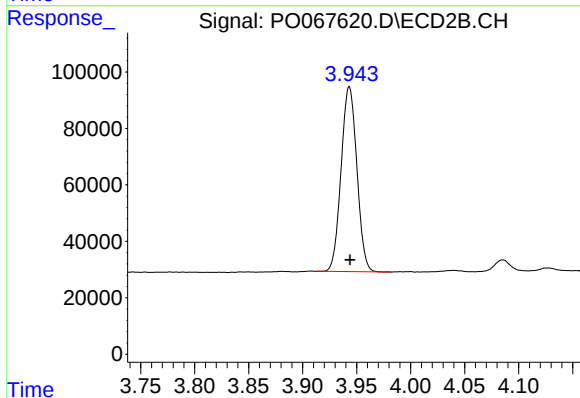


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 665677
Conc: 19.86 ng/ml

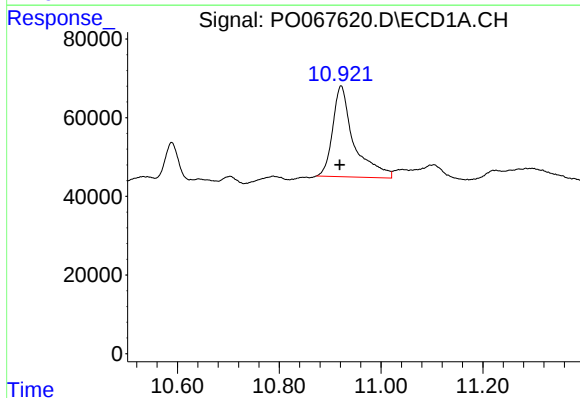

#2 Decachlorobiphenyl

R.T.: 10.921 min
Delta R.T.: 0.003 min
Response: 666628
Conc: 19.58 ng/ml

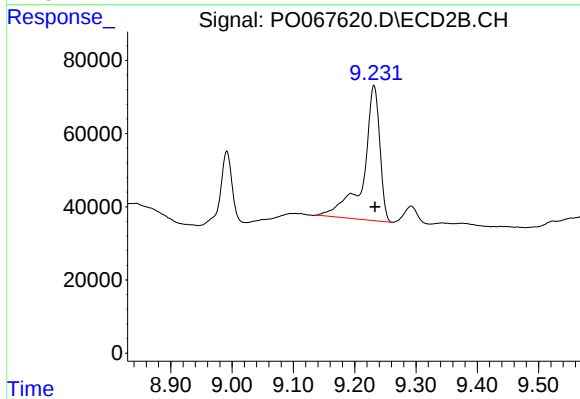

#2 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: -0.002 min
Response: 680534
Conc: 16.46 ng/ml m