

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040220\
 Data File : P0067627.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2020 16:59
 Operator : DD\AJ
 Sample : L2100-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 239-05060708-0-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 05:46:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 01 17:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.935	3.944	520039	785941	21.837	23.449
2)	SA Decachlor...	10.920	9.232	641953	702266	18.857	16.985

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040220\
Data File : P0067627.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2020 16:59
Operator : DD\AJ
Sample : L2100-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
239-05060708-0-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 05:46:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 01 17:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

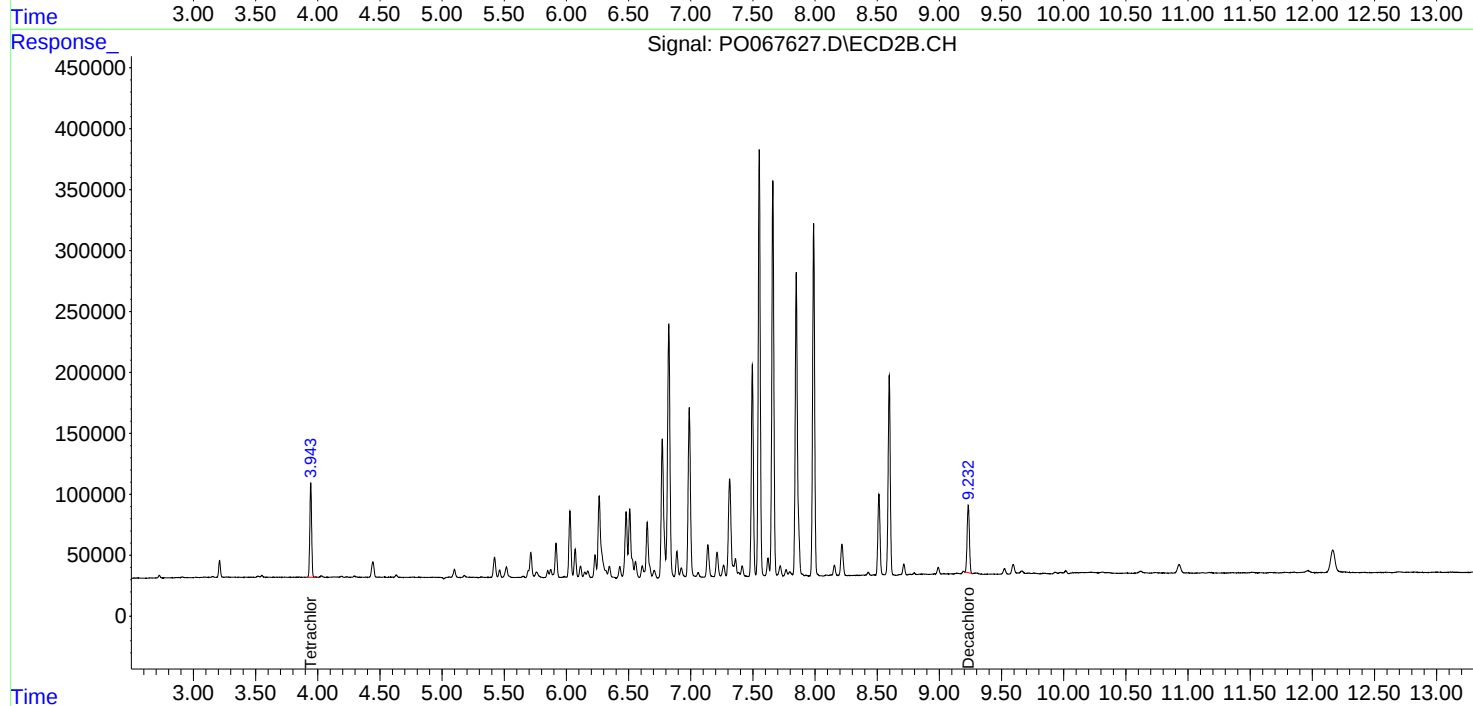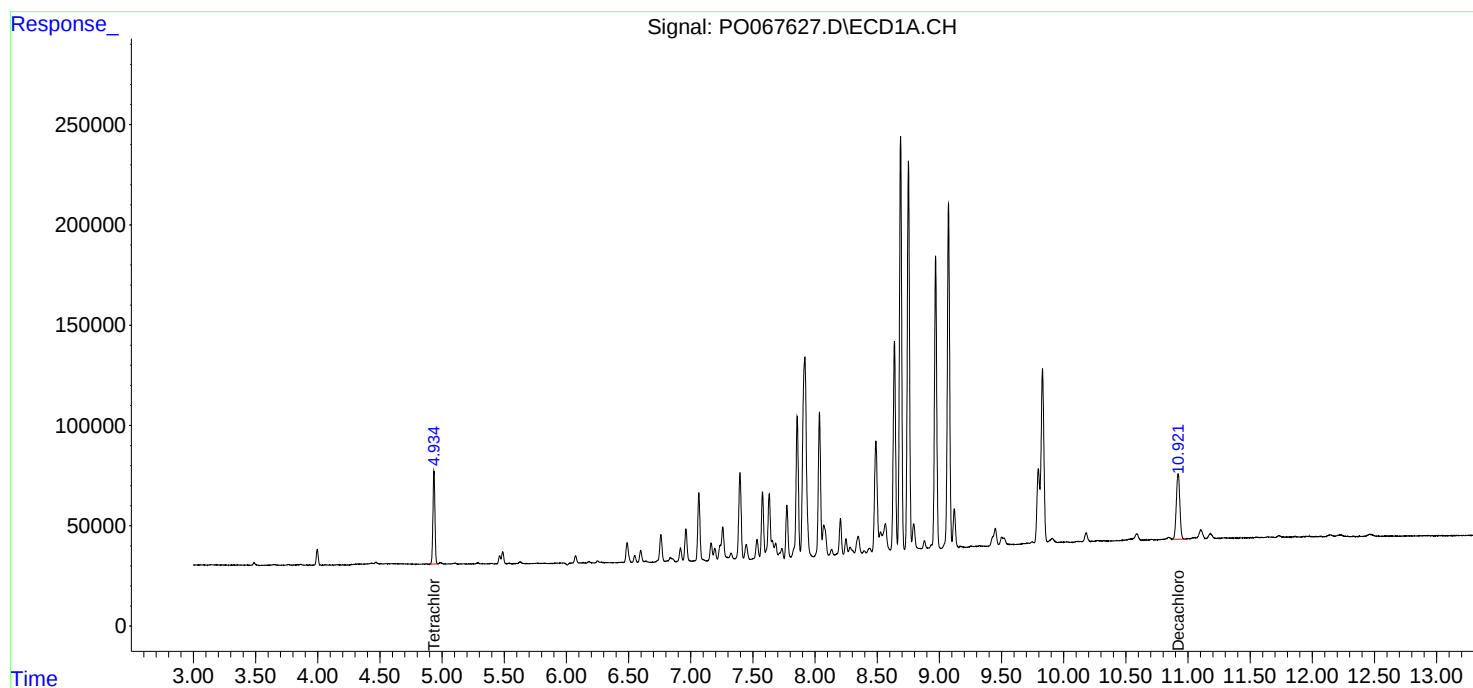


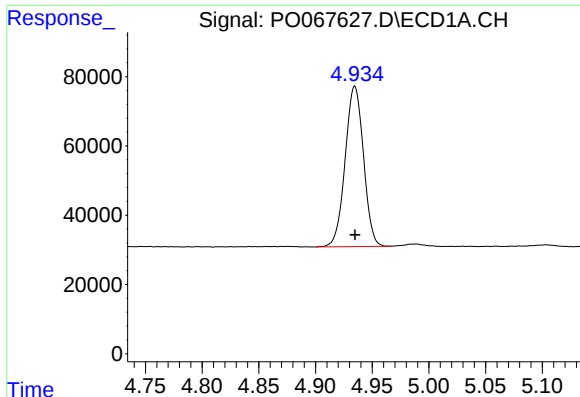

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 520039
Conc: 21.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
239-05060708-0-6

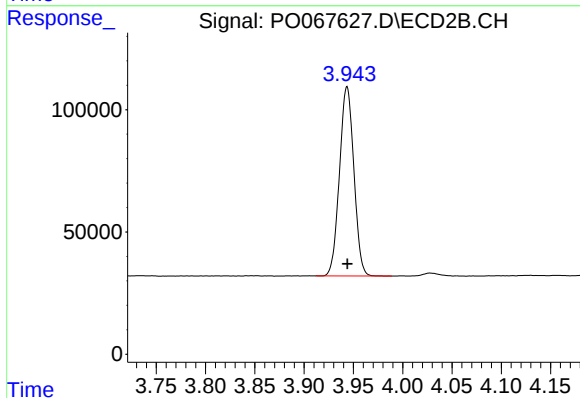


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 785941
Conc: 23.45 ng/ml

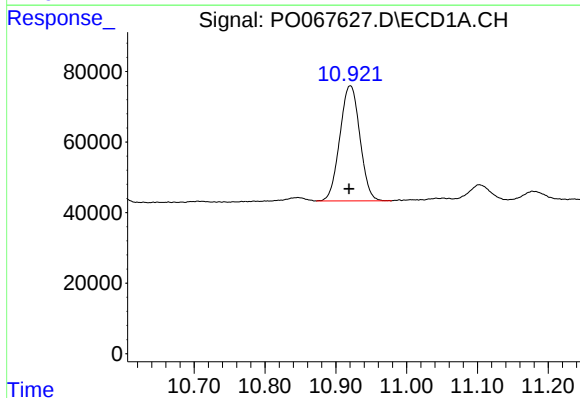

#2 Decachlorobiphenyl

R.T.: 10.920 min
Delta R.T.: 0.002 min
Response: 641953
Conc: 18.86 ng/ml

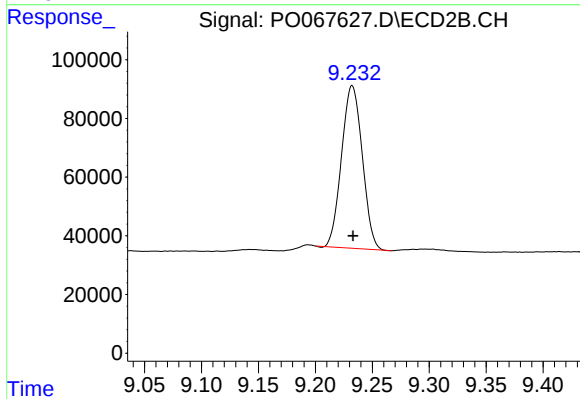

#2 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 702266
Conc: 16.99 ng/ml