

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040419\
 Data File : P0054943.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Apr 2019 22:42
 Operator : SM/SJ
 Sample : K2245-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 00:55:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.298	3.612	669072	636495	19.279	19.945
2) SA Decachlor...	9.913	8.583	636449	448611	12.910	14.086
Target Compounds						
9) L2 AR-1221-2	0.000	3.912	0	13789	N.D.	45.996 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040419\
Data File : PO054943.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Apr 2019 22:42
Operator : SM/SJ
Sample : K2245-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-3D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 00:55:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

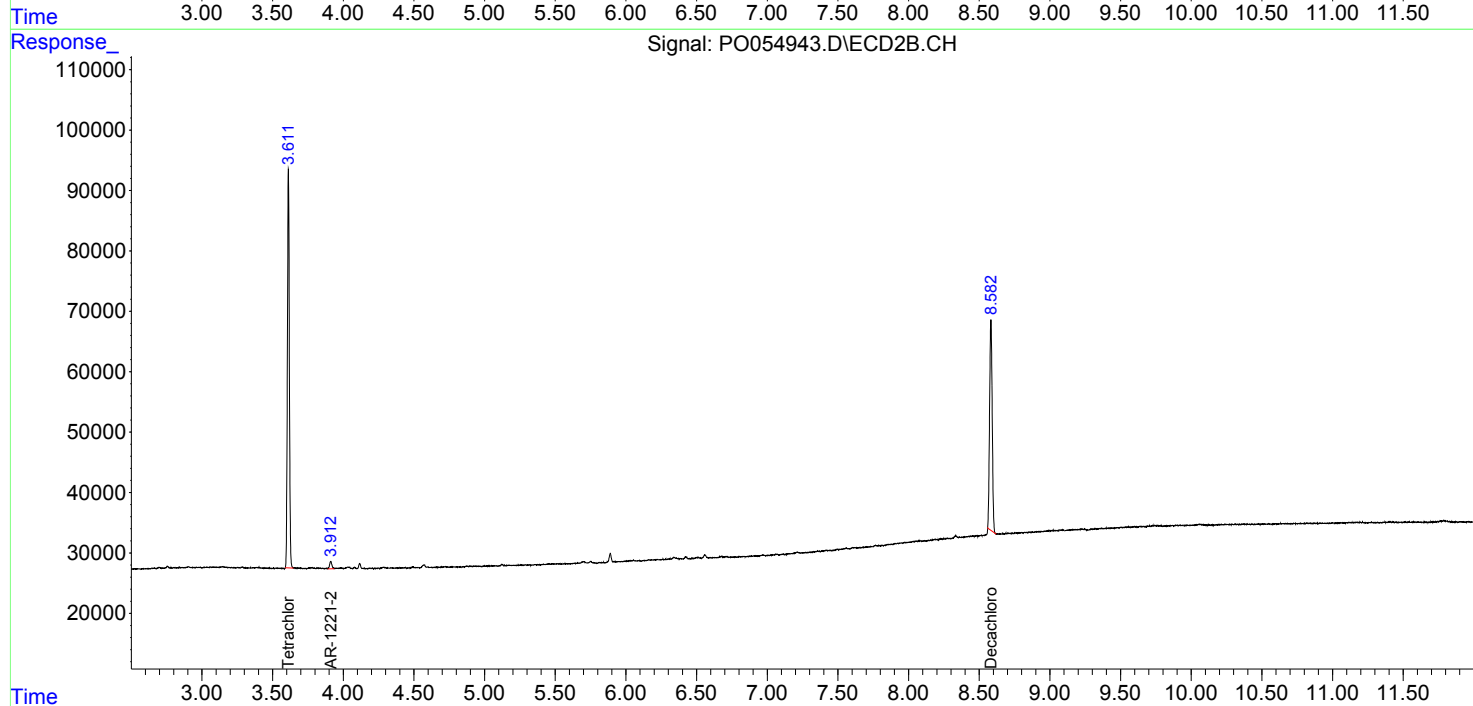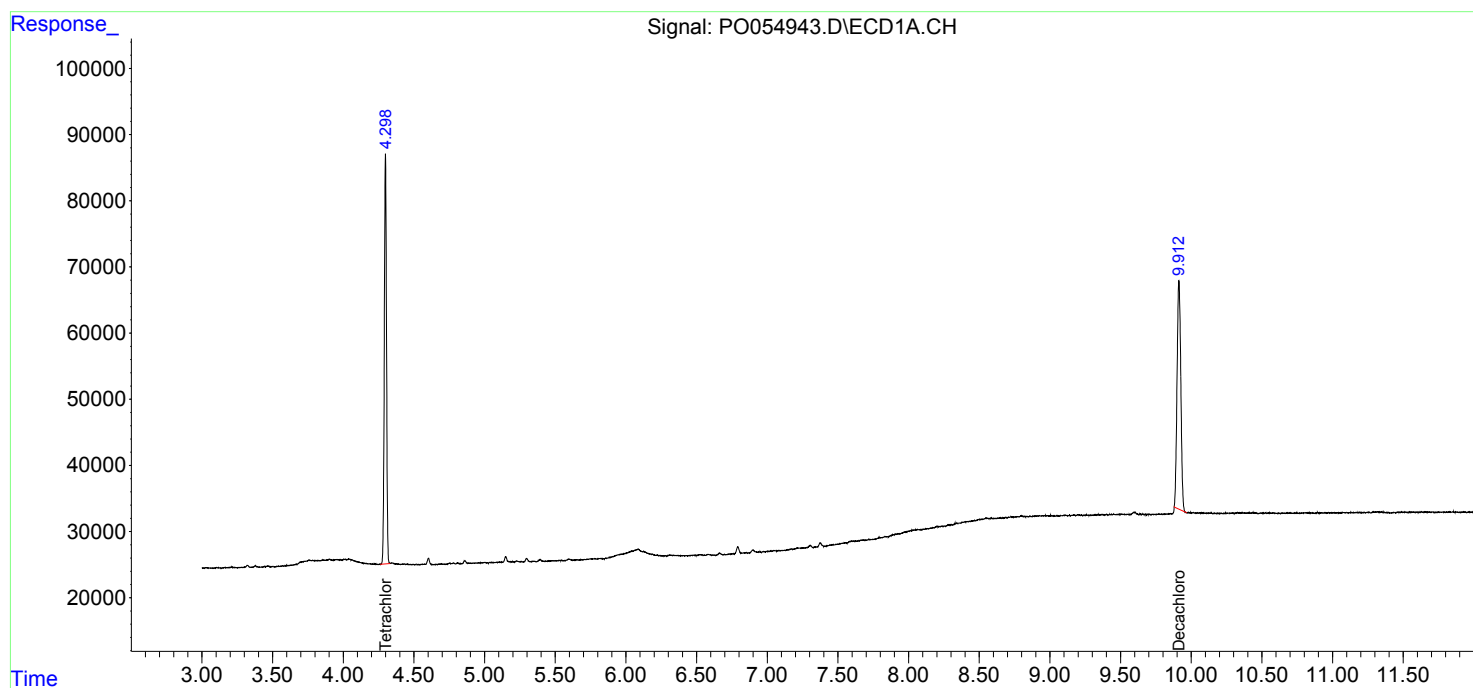


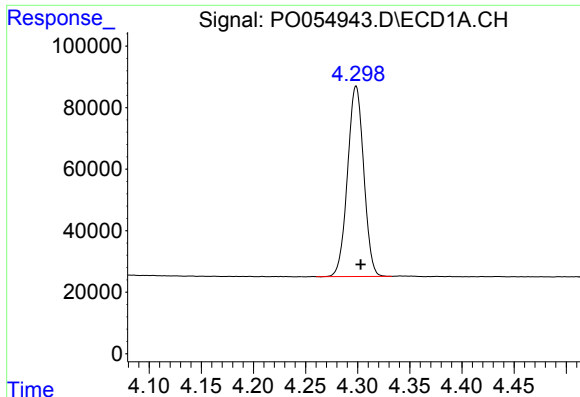

#1 Tetrachloro-m-xylene


R.T.: 4.298 min
Delta R.T.: -0.005 min
Response: 669072
Conc: 19.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3D

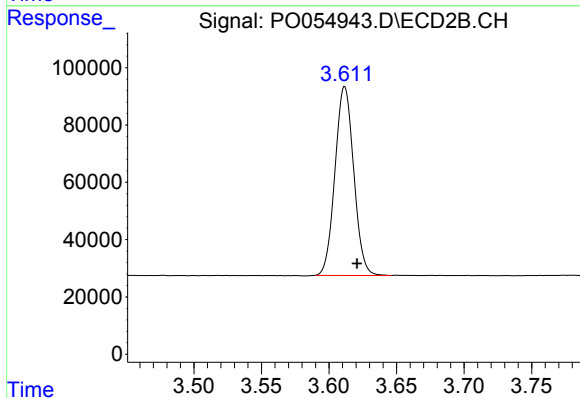


#1 Tetrachloro-m-xylene

R.T.: 3.612 min
Delta R.T.: -0.009 min
Response: 636495
Conc: 19.95 ng/ml

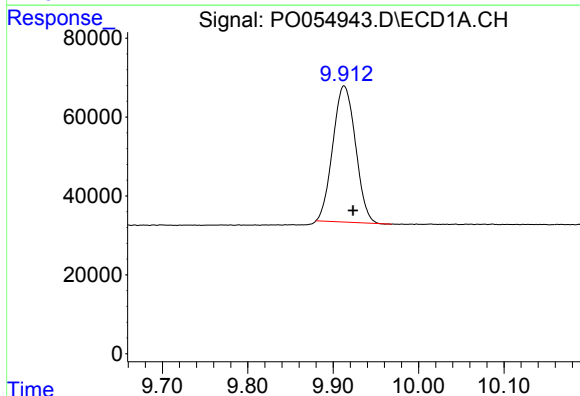


#2 Decachlorobiphenyl

R.T.: 9.913 min
Delta R.T.: -0.010 min
Response: 636449
Conc: 12.91 ng/ml

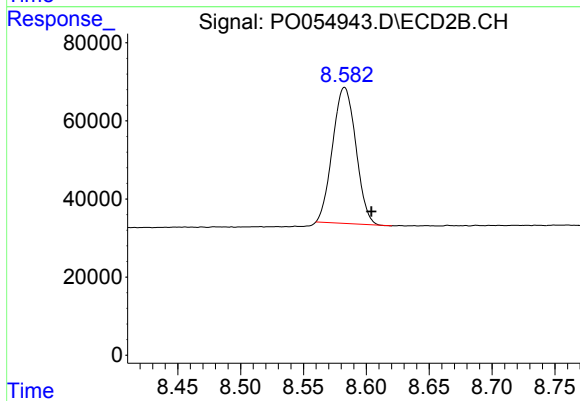

#2 Decachlorobiphenyl


R.T.: 8.583 min
Delta R.T.: -0.021 min
Response: 448611
Conc: 14.09 ng/ml

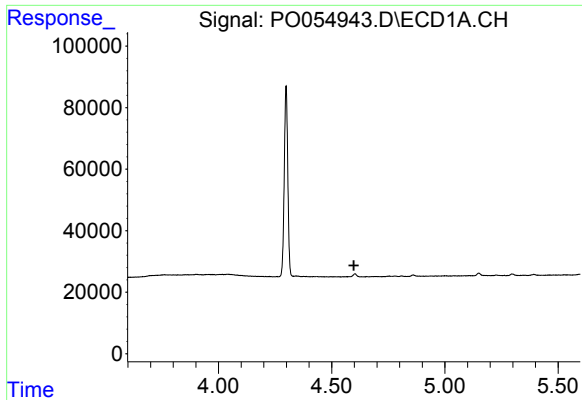

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.598 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-3D

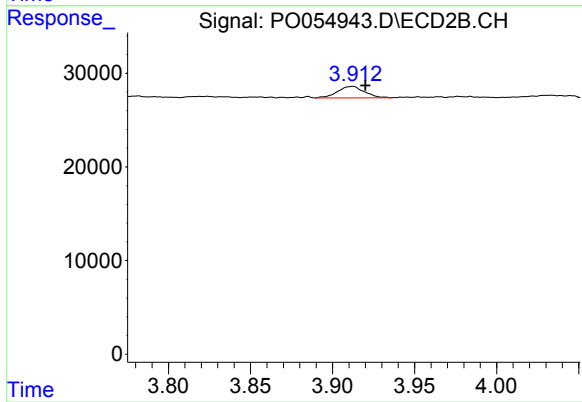

#9 AR-1221-2

R.T.: 3.912 min
Delta R.T.: -0.007 min
Response: 13789
Conc: 46.00 ng/ml