

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040419\
 Data File : P0054927.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Apr 2019 18:10
 Operator : SM/SJ
 Sample : K2193-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HR-06-040319-C

Manual Integrations
 APPROVED

Sohil
 4/5/2019 11:31:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:40:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.300	3.614	613210	606430	17.669	19.003
2) SA Decachlor...	9.917	8.585	578087	401085	11.726m	12.594

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040419\
Data File : P0054927.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Apr 2019 18:10
Operator : SM/SJ
Sample : K2193-05
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HR-06-040319-C


Manual Integrations
APPROVED

Sohil
4/5/2019 11:31:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:40:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

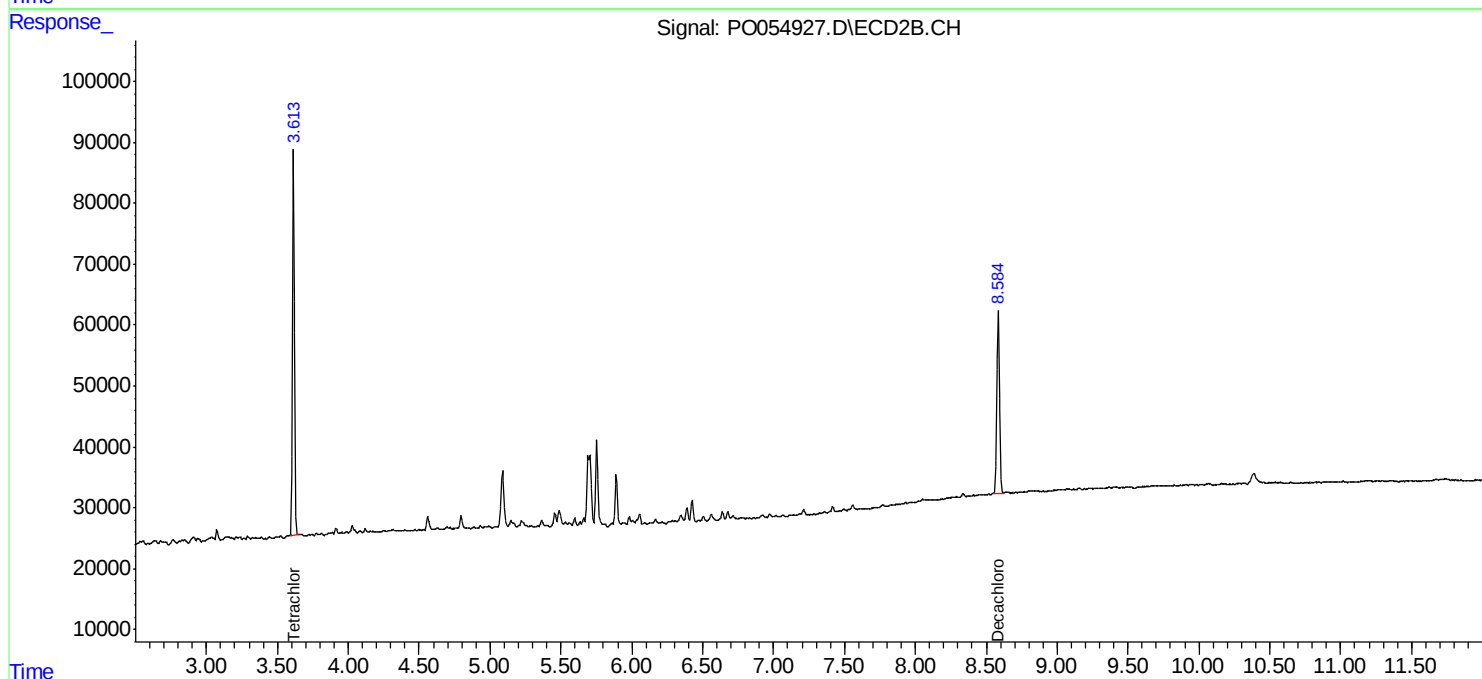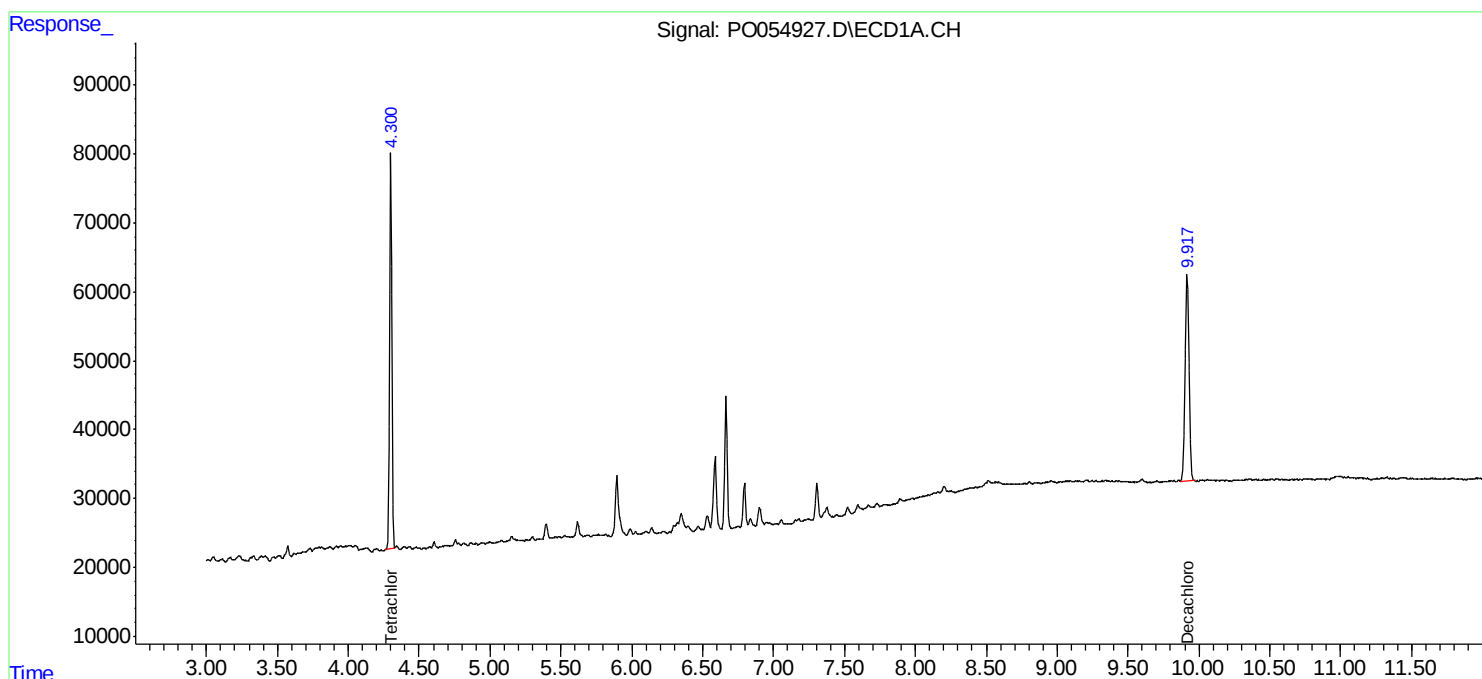

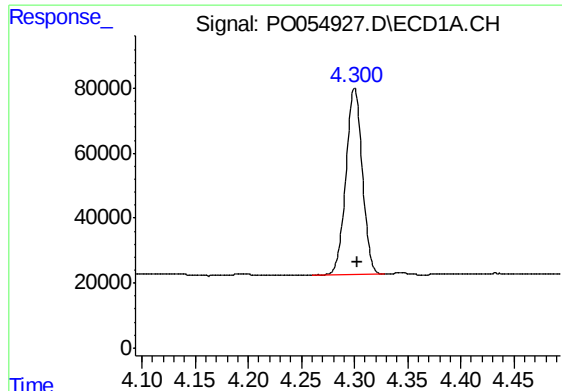


#1 Tetrachloro-m-xylene

R.T.: 4.300 min
Delta R.T.: -0.003 min
Response: 613210
Conc: 17.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
HR-06-040319-C


Manual Integrations
APPROVED

Sohil
4/5/2019 11:31:20 AM

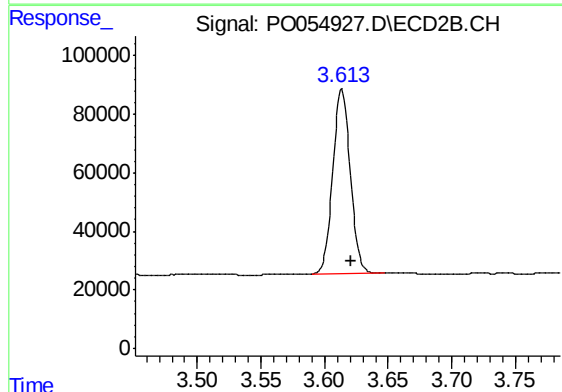


#1 Tetrachloro-m-xylene

R.T.: 3.614 min
Delta R.T.: -0.007 min
Response: 606430
Conc: 19.00 ng/ml

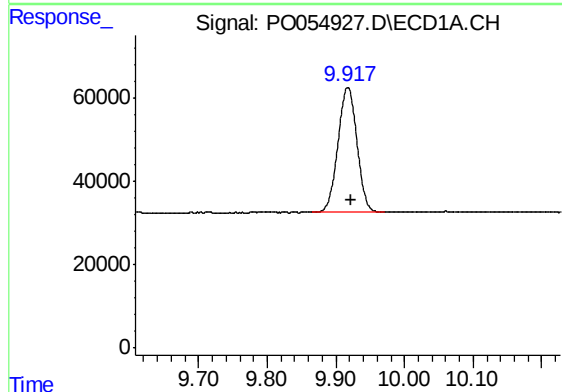

#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.006 min
Response: 578087
Conc: 11.73 ng/ml m

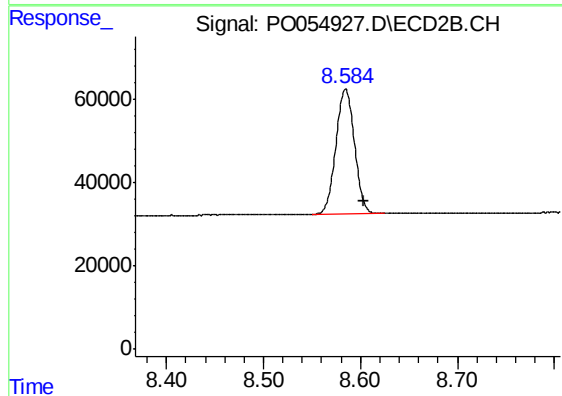

#2 Decachlorobiphenyl

R.T.: 8.585 min
Delta R.T.: -0.019 min
Response: 401085
Conc: 12.59 ng/ml