

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040419\
 Data File : P0054929.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Apr 2019 18:44
 Operator : SM/SJ
 Sample : K2221-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S10B(2-10)COMP

Manual Integrations
 APPROVED

Sohil
 4/5/2019 11:31:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:41:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.300	3.614	671829	678482	19.358	21.261
2) SA Decachlor...	9.915	8.585	515954	363253	10.466m	11.406

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040419\
Data File : PO054929.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Apr 2019 18:44
Operator : SM/SJ
Sample : K2221-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S10B(2-10)COMP


Manual Integrations
APPROVED

Sohil
4/5/2019 11:31:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:41:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

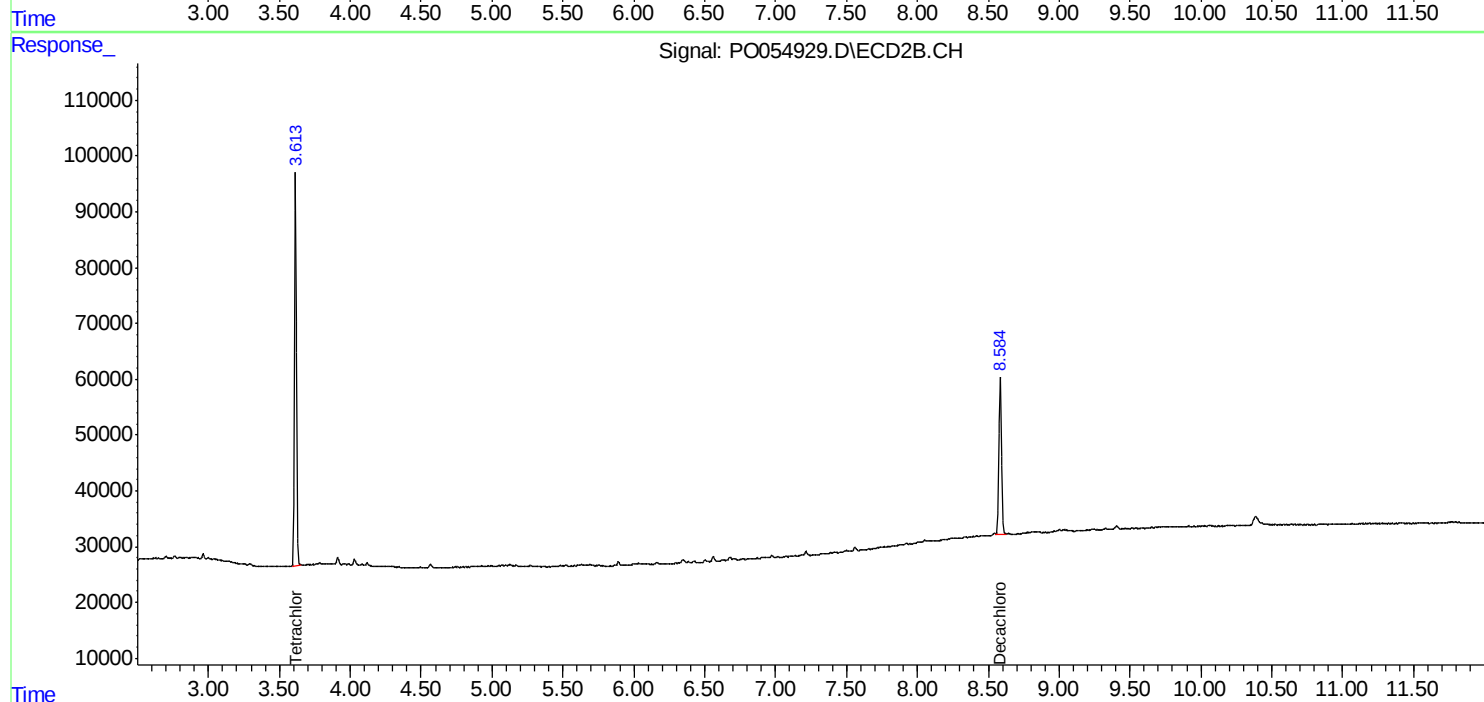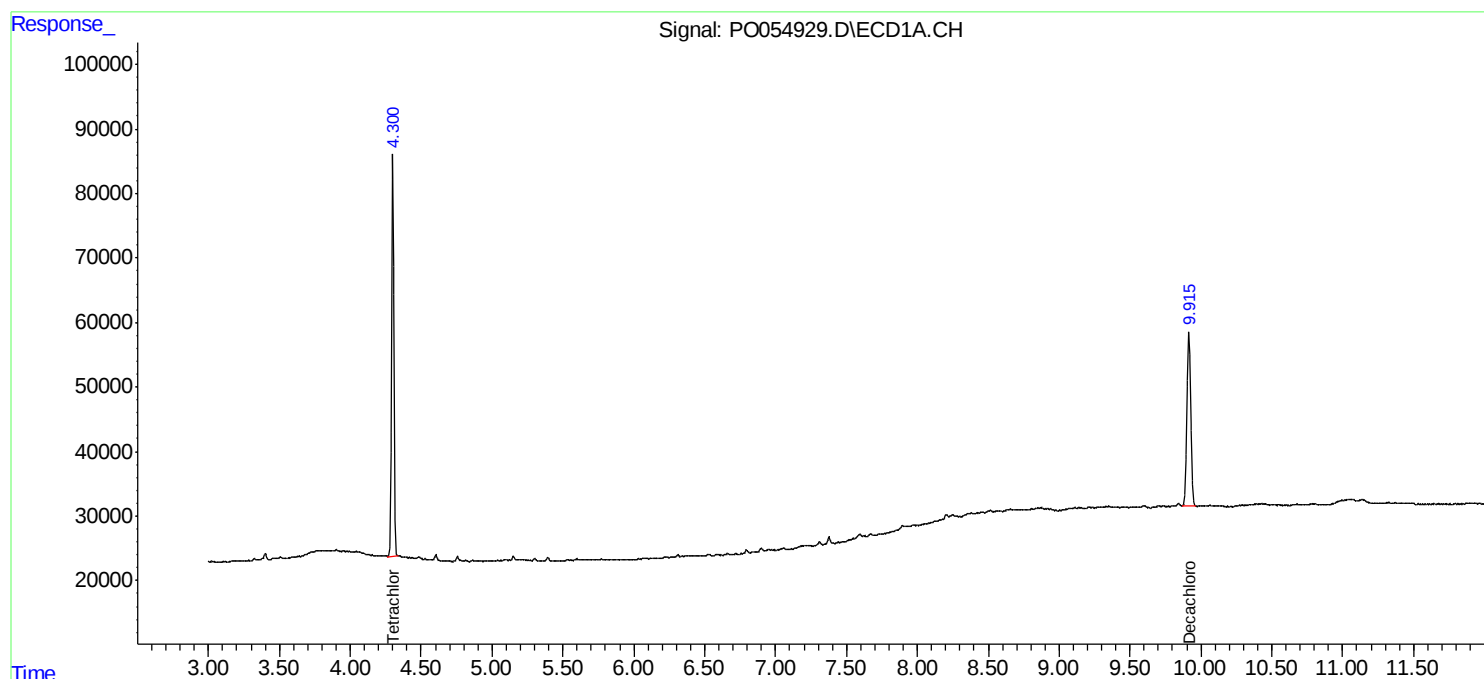

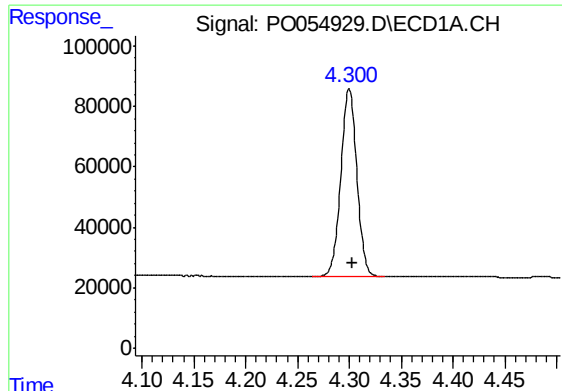


#1 Tetrachloro-m-xylene

R.T.: 4.300 min
Delta R.T.: -0.003 min
Response: 671829
Conc: 19.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
S10B(2-10)COMP


Manual Integrations
APPROVED

Sohil
4/5/2019 11:31:18 AM

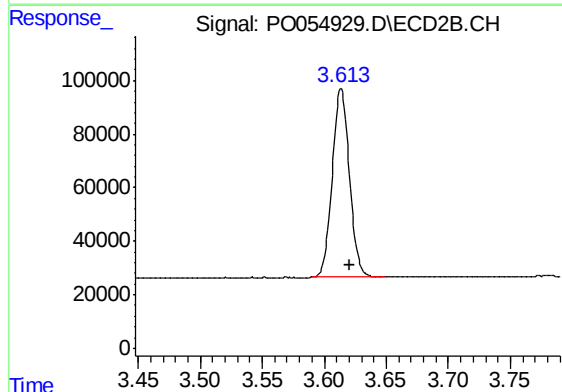


#1 Tetrachloro-m-xylene

R.T.: 3.614 min
Delta R.T.: -0.007 min
Response: 678482
Conc: 21.26 ng/ml

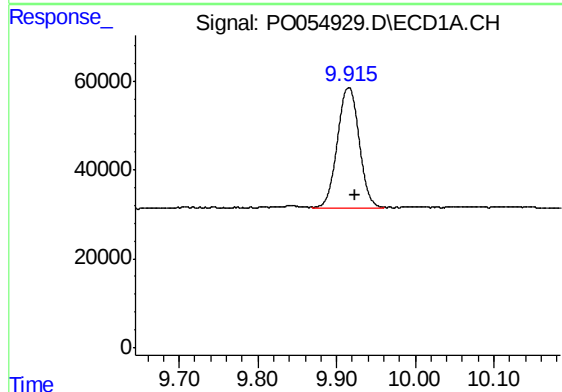

#2 Decachlorobiphenyl

R.T.: 9.915 min
Delta R.T.: -0.008 min
Response: 515954
Conc: 10.47 ng/ml m

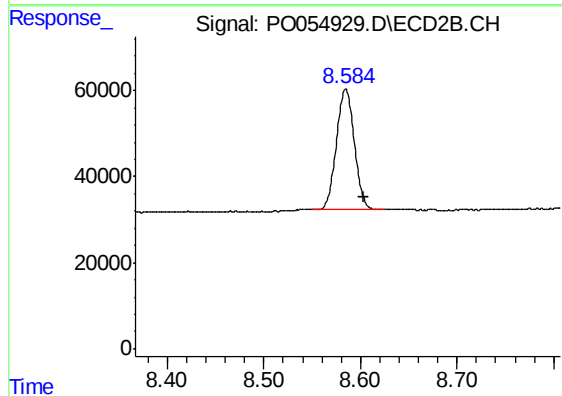

#2 Decachlorobiphenyl

R.T.: 8.585 min
Delta R.T.: -0.019 min
Response: 363253
Conc: 11.41 ng/ml