

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040419\
 Data File : P0054935.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Apr 2019 20:26
 Operator : SM/SJ
 Sample : K2227-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-PILE-1-C

Manual Integrations
 APPROVED

Sohil
 4/8/2019 8:34:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:51:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.300	3.613	1040361	991135	29.977	31.058
2) SA Decachlor...	9.916	8.583	991498	644955	20.112m	20.251

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040419\
Data File : P0054935.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Apr 2019 20:26
Operator : SM/SJ
Sample : K2227-05
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE-1-C


Manual Integrations
APPROVED

Sohil
4/8/2019 8:34:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:51:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

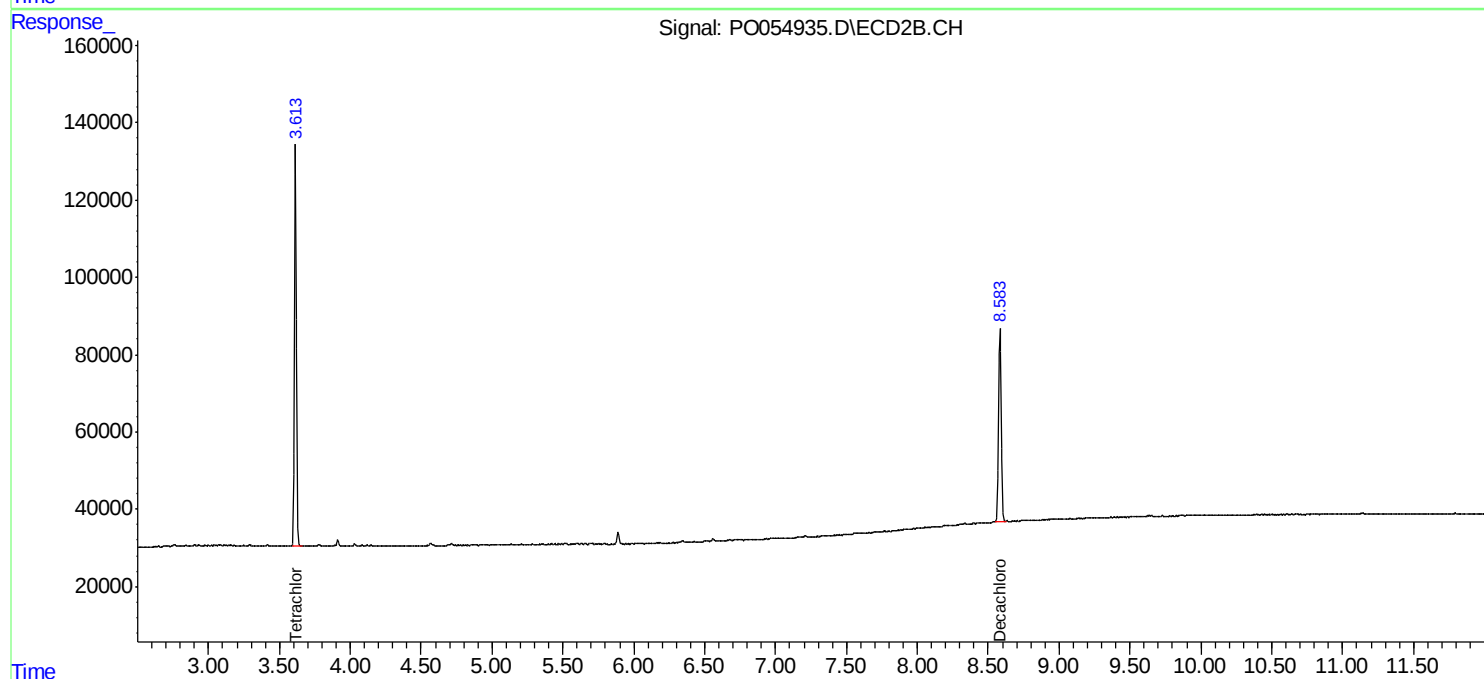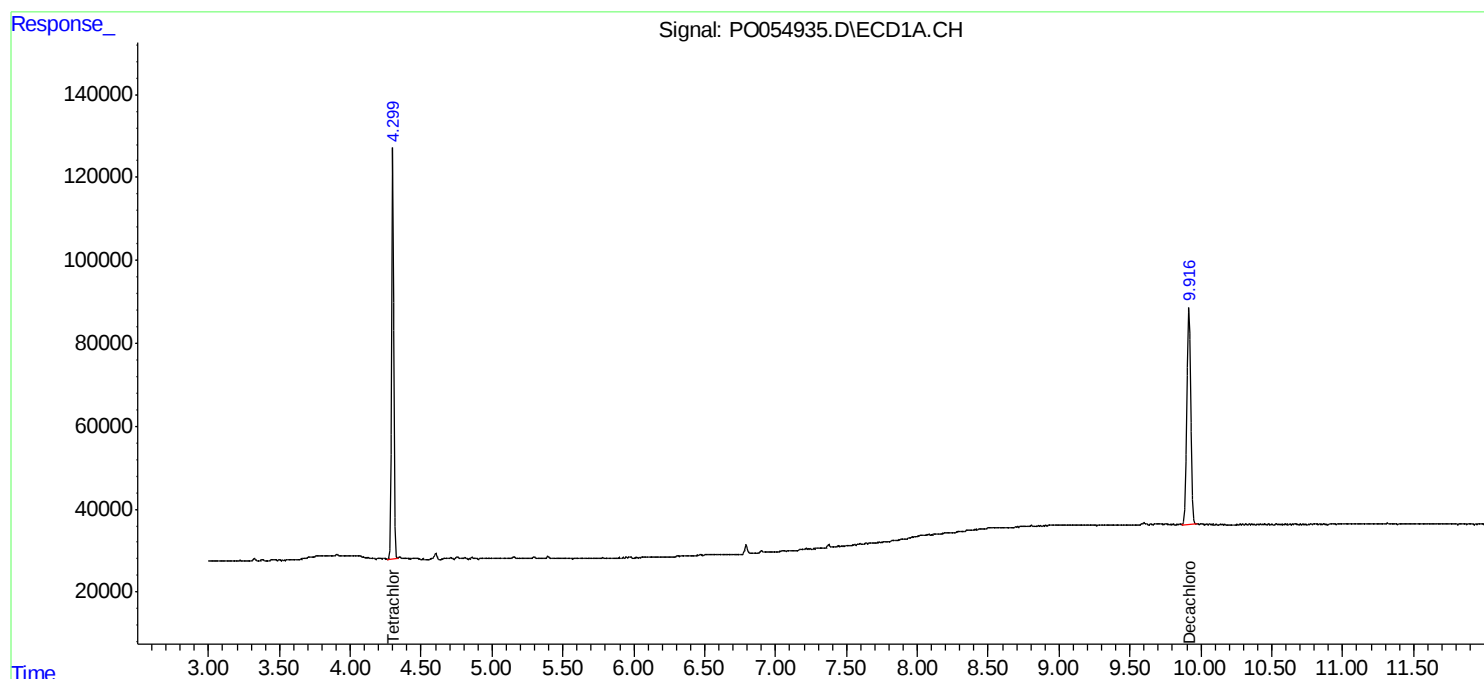

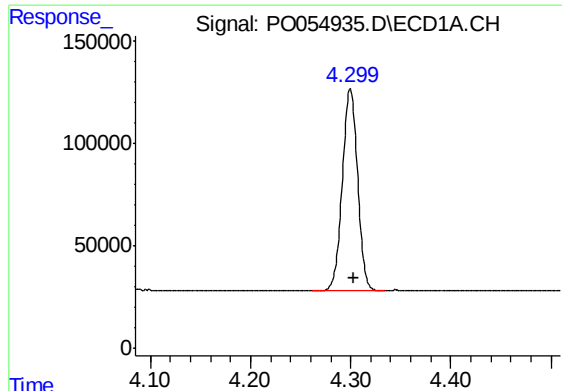


#1 Tetrachloro-m-xylene

R.T.: 4.300 min
Delta R.T.: -0.003 min
Response: 1040361
Conc: 29.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE-1-C


Manual Integrations
APPROVED

Sohil
4/8/2019 8:34:50 AM

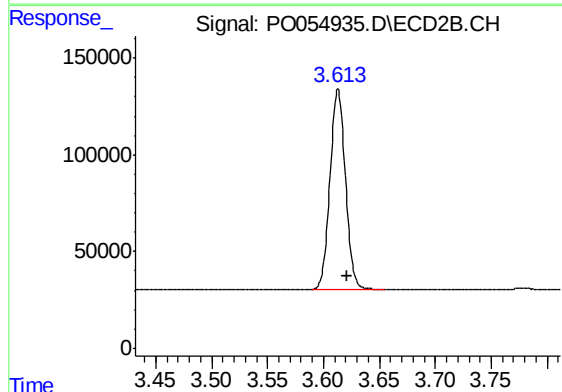


#1 Tetrachloro-m-xylene

R.T.: 3.613 min
Delta R.T.: -0.008 min
Response: 991135
Conc: 31.06 ng/ml

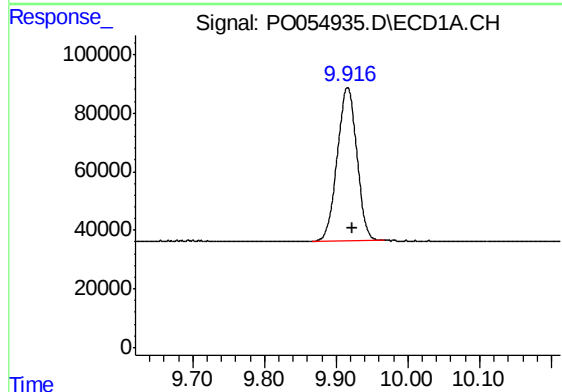

#2 Decachlorobiphenyl

R.T.: 9.916 min
Delta R.T.: -0.008 min
Response: 991498
Conc: 20.11 ng/ml m

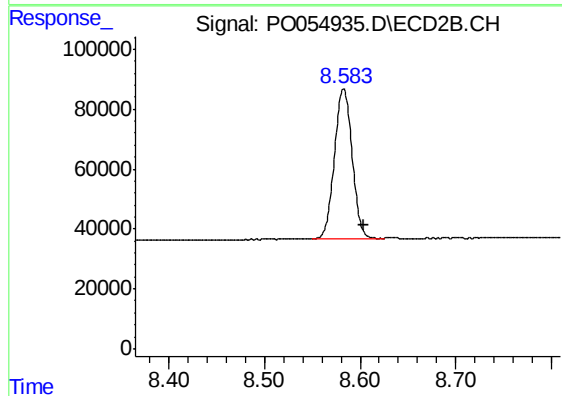

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: -0.021 min
Response: 644955
Conc: 20.25 ng/ml