

Data Path : P:\HPCHEM1\ECD 0\Data\P0040518\
 Data File : P0043645.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2018 21:58
 Operator : SM/UA
 Sample : J2265-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PF-3

Manual Integrations
 APPROVED

ugo
 4/6/2018 3:14:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 02:08:59 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 04 15:17:57 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.065	3.324	4452721	5859503	25.047	21.808
2) SA Decachlor...	9.403	8.083	2604326	3252037	14.452m	13.871

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0040518\
Data File : P0043645.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2018 21:58
Operator : SM/UA
Sample : J2265-02
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PF-3


Manual Integrations
APPROVED

ugo
4/6/2018 3:14:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 02:08:59 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 04 15:17:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

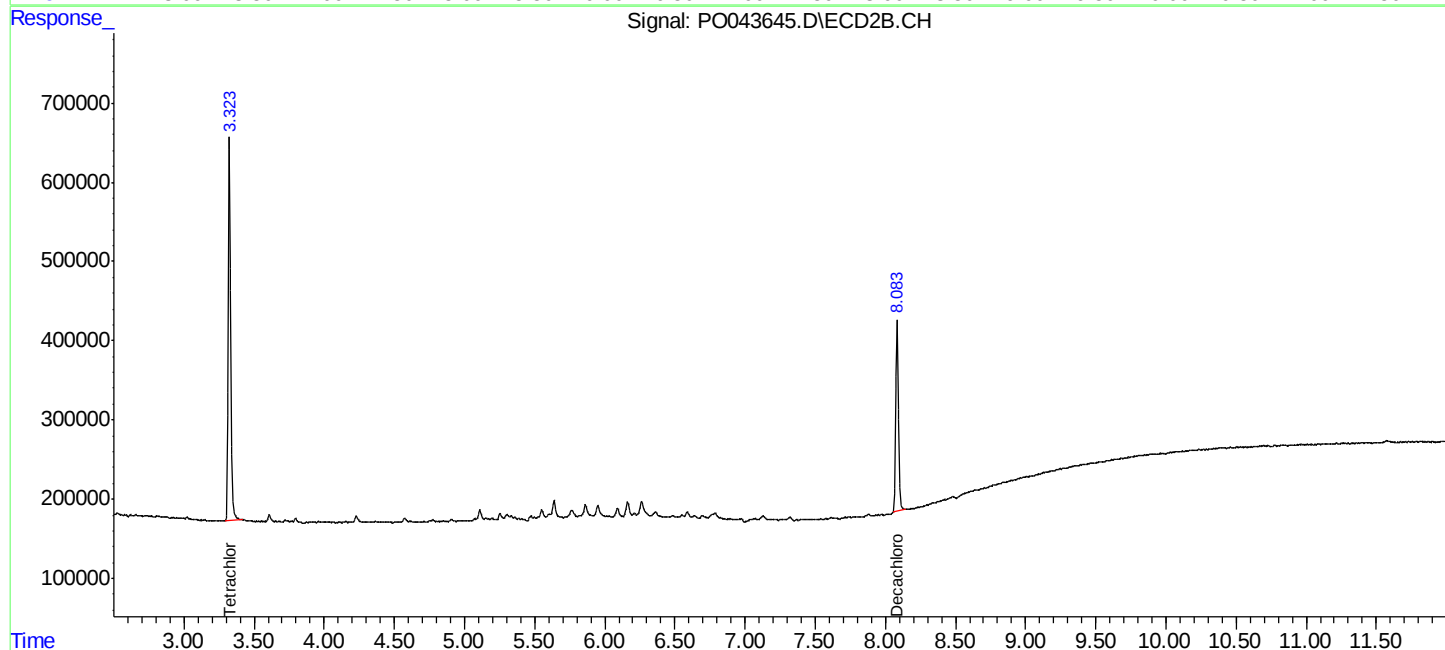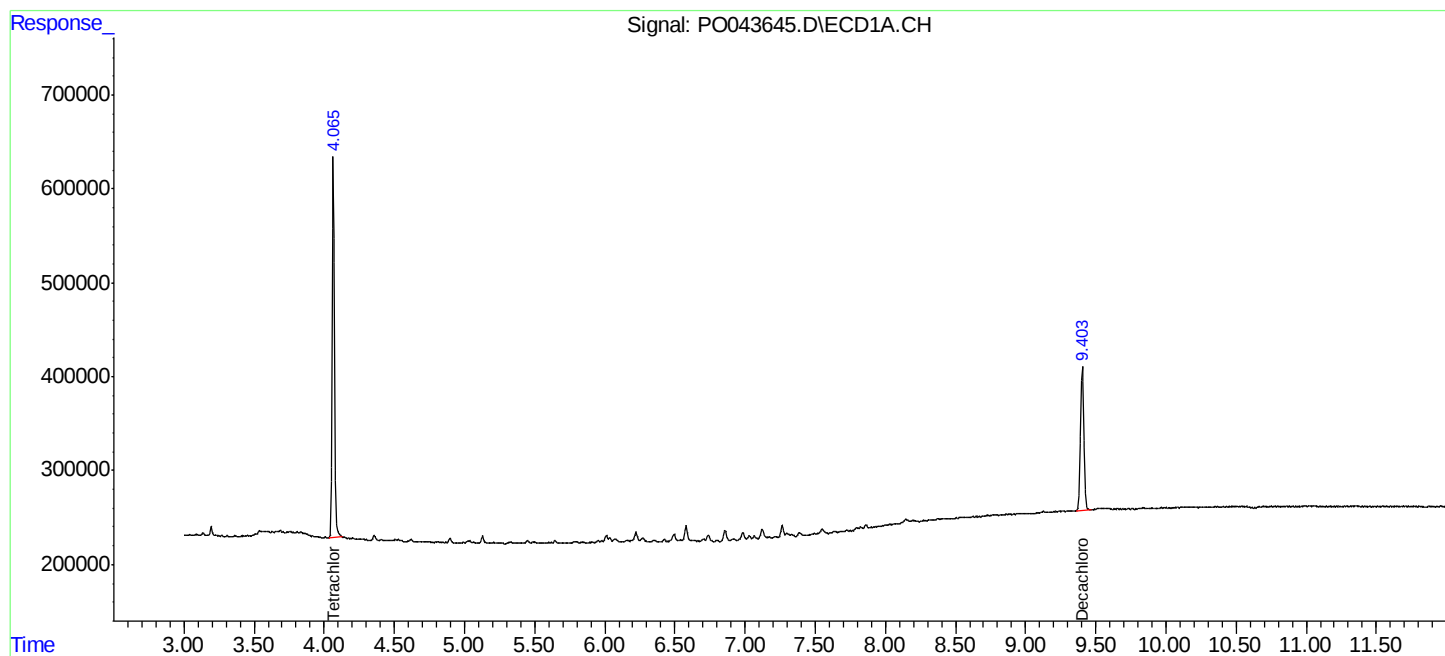

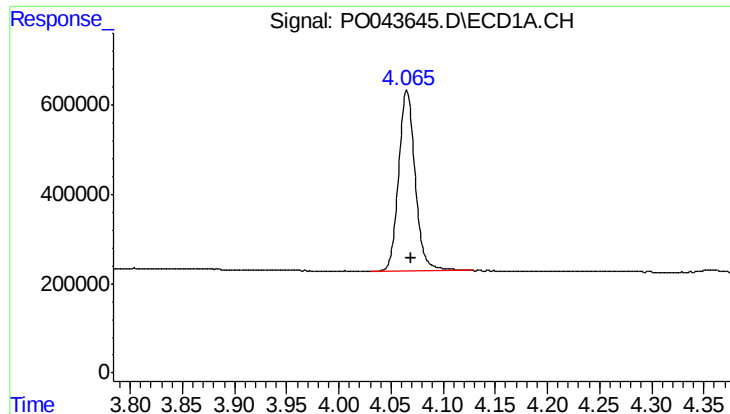


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: -0.004 min
Response: 4452721
Conc: 25.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
PF-3


Manual Integrations
APPROVED

ugo
4/6/2018 3:14:42 PM

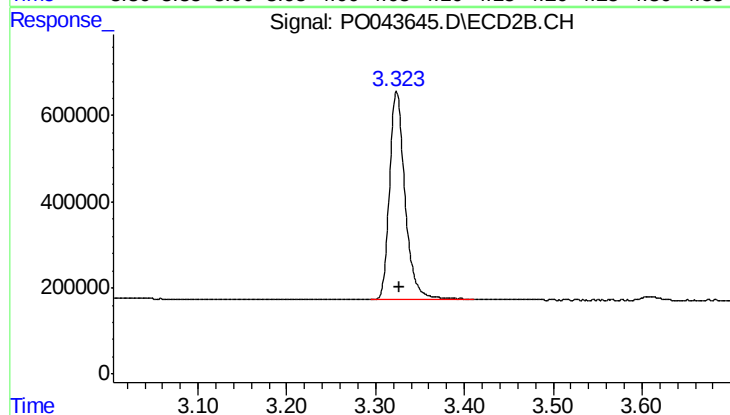


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: -0.003 min
Response: 5859503
Conc: 21.81 ng/ml

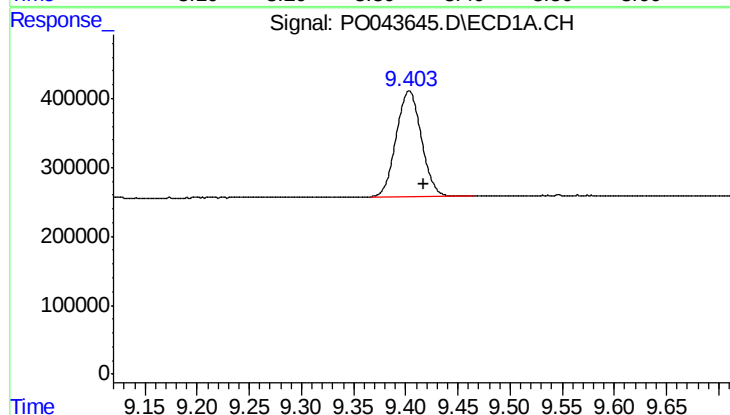

#2 Decachlorobiphenyl

R.T.: 9.403 min
Delta R.T.: -0.014 min
Response: 2604326
Conc: 14.45 ng/ml m

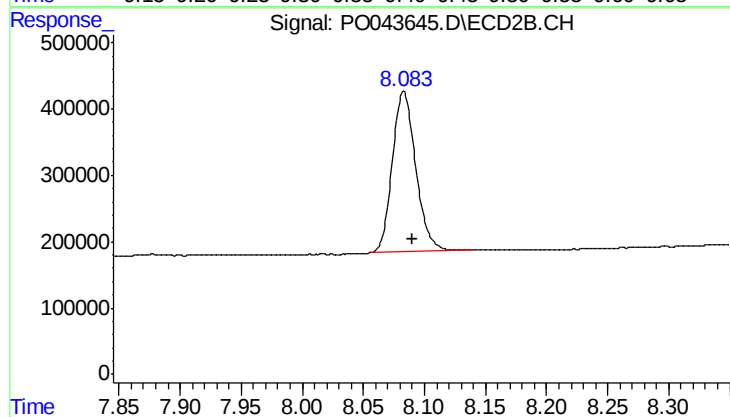

#2 Decachlorobiphenyl

R.T.: 8.083 min
Delta R.T.: -0.007 min
Response: 3252037
Conc: 13.87 ng/ml