

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040519\
 Data File : P0054999.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2019 23:13
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1232 LOD 40 PPB
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

Sohil
 4/8/2019 5:24:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 04:03:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.296	3.609	798270	691121	23.001	21.657
2)	SA Decachlor...	9.911	8.577	1000406	700424	20.293	21.993
Target Compounds							
11)	L3 AR-1232-1	4.667	3.982	53553	43041	62.202	57.396
12)	L3 AR-1232-2	5.192	4.705	28926	44858	59.138	52.094
13)	L3 AR-1232-3	5.480	4.880	56326	25315	57.634	52.243
14)	L3 AR-1232-4	5.640	4.962	29517	20693	57.667m	47.095
15)	L3 AR-1232-5	5.729	5.131	21380	25346	51.394m	52.114m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040519\
Data File : PO054999.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2019 23:13
Operator : SM/SJ
Sample : K1560-07
Misc : AR1232 LOD 40 PPB
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:24:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 04:03:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

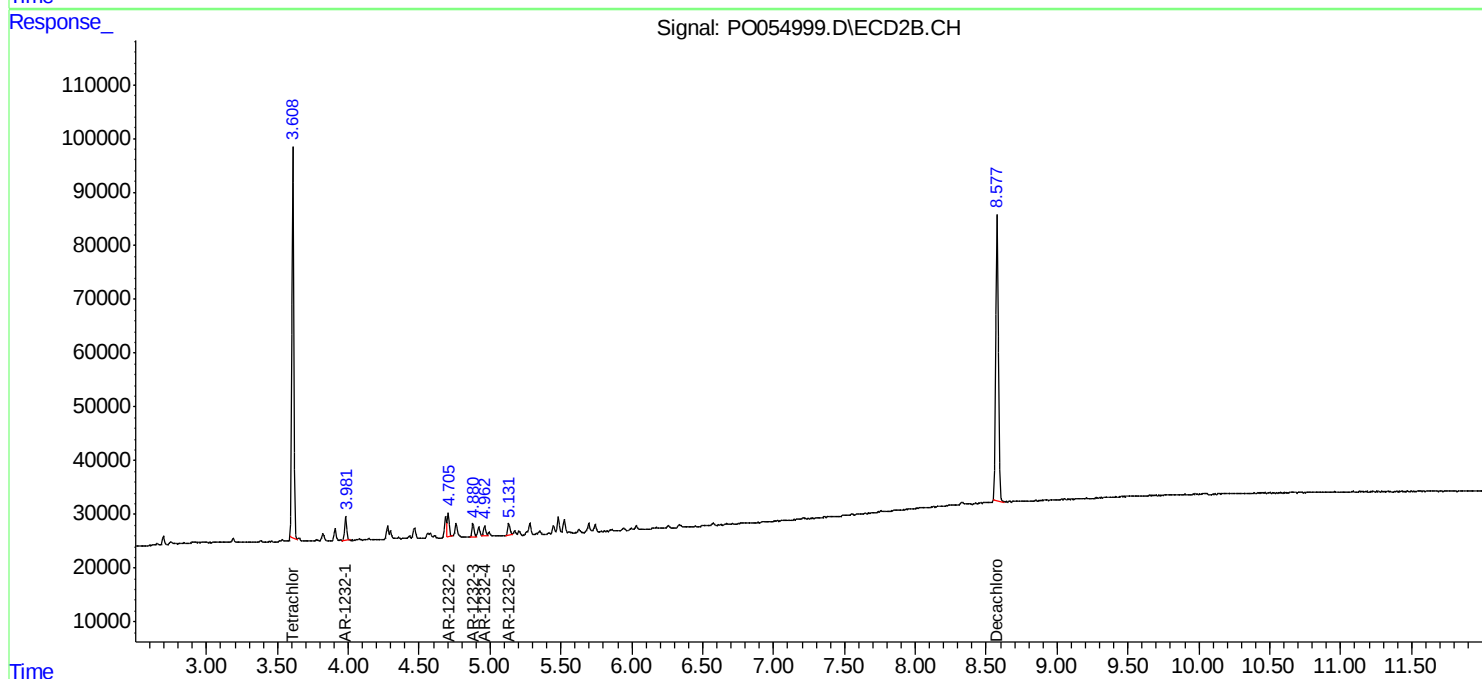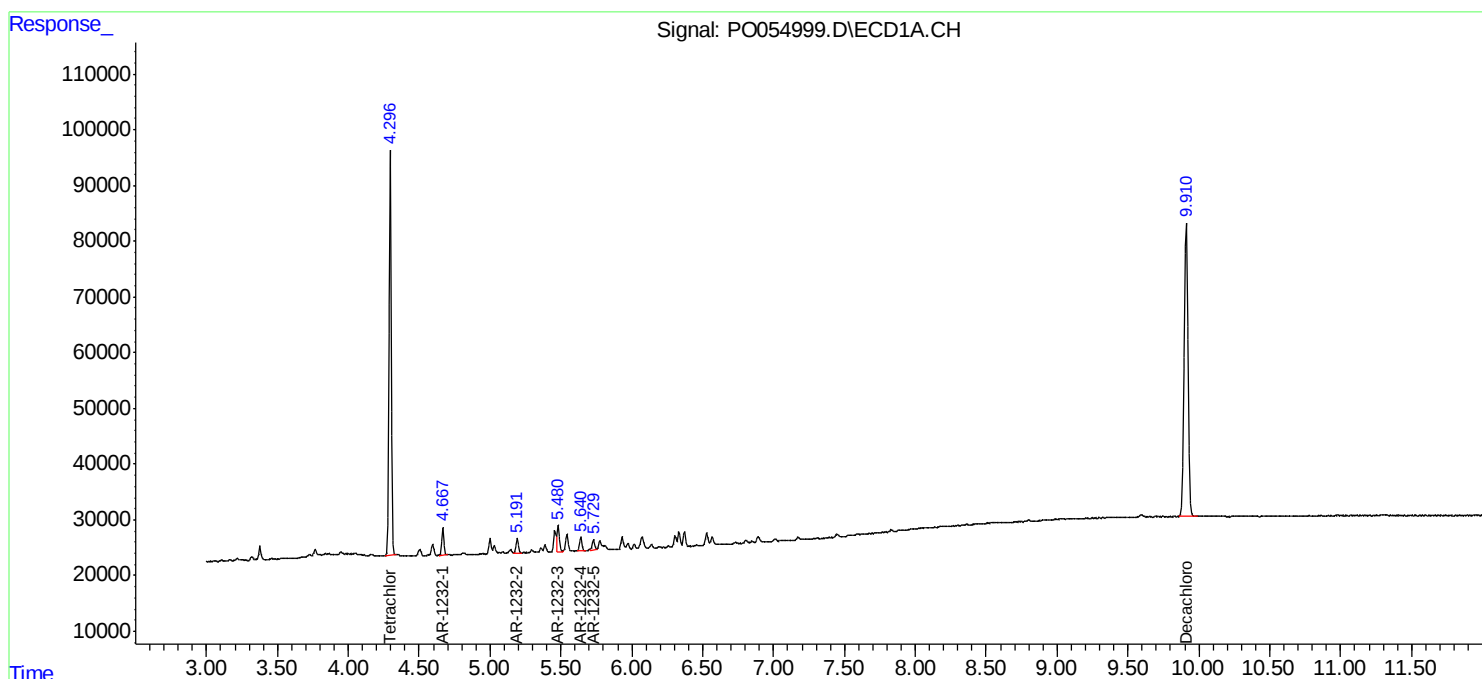

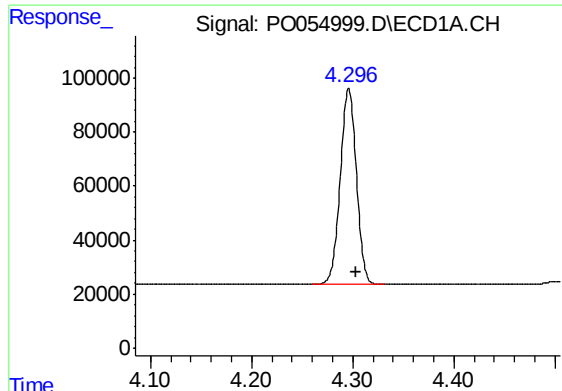


#1 Tetrachloro-m-xylene

R.T.: 4.296 min
Delta R.T.: -0.007 min
Response: 798270
Conc: 23.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:24:48 PM

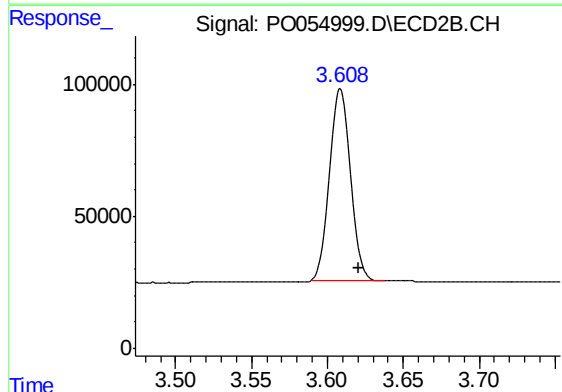


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.012 min
Response: 691121
Conc: 21.66 ng/ml

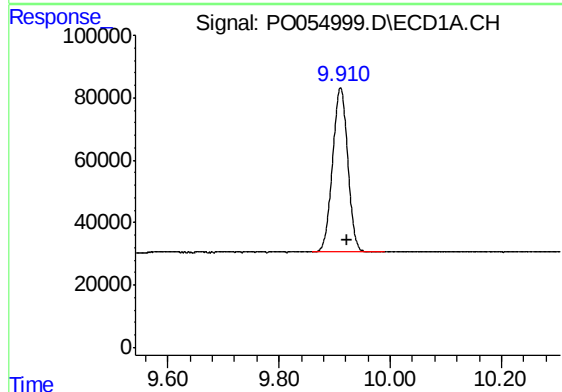


#2 Decachlorobiphenyl

R.T.: 9.911 min
Delta R.T.: -0.012 min
Response: 1000406
Conc: 20.29 ng/ml

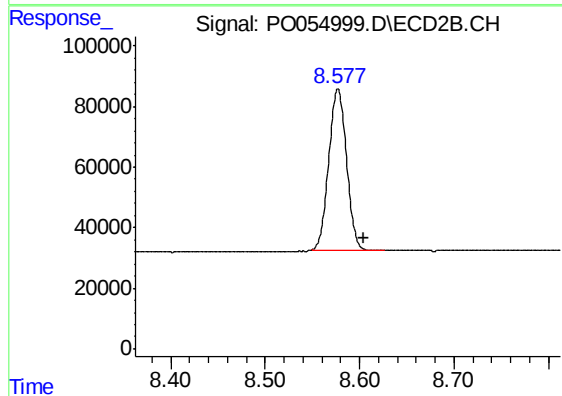

#2 Decachlorobiphenyl

R.T.: 8.577 min
Delta R.T.: -0.027 min
Response: 700424
Conc: 21.99 ng/ml

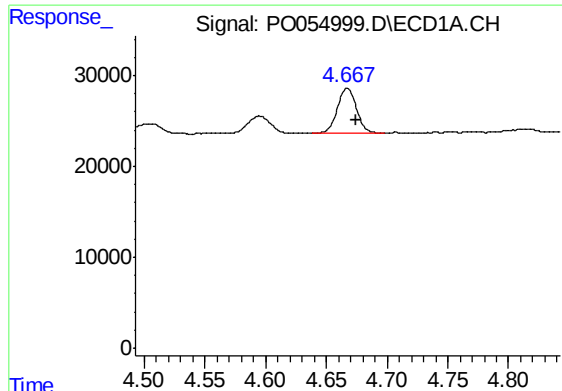


#11 AR-1232-1

R.T.: 4.667 min
Delta R.T.: -0.008 min
Response: 53553
Conc: 62.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:24:48 PM

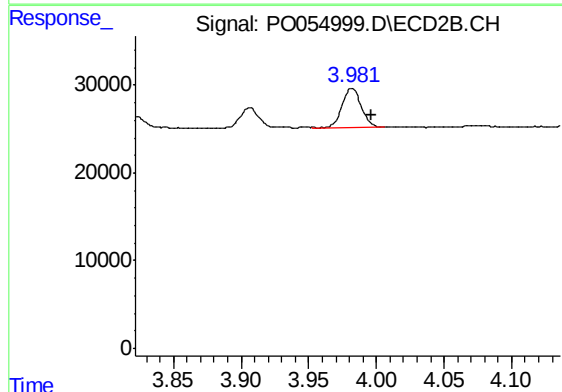


#11 AR-1232-1

R.T.: 3.982 min
Delta R.T.: -0.015 min
Response: 43041
Conc: 57.40 ng/ml

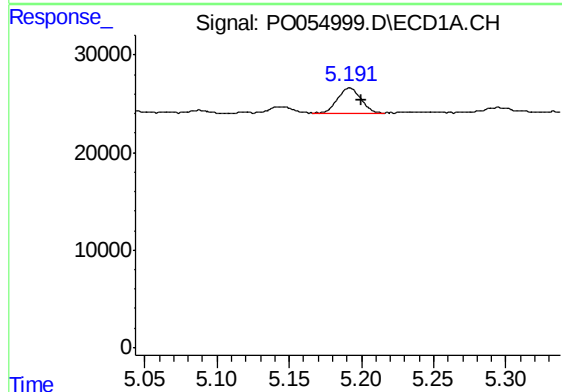


#12 AR-1232-2

R.T.: 5.192 min
Delta R.T.: -0.008 min
Response: 28926
Conc: 59.14 ng/ml

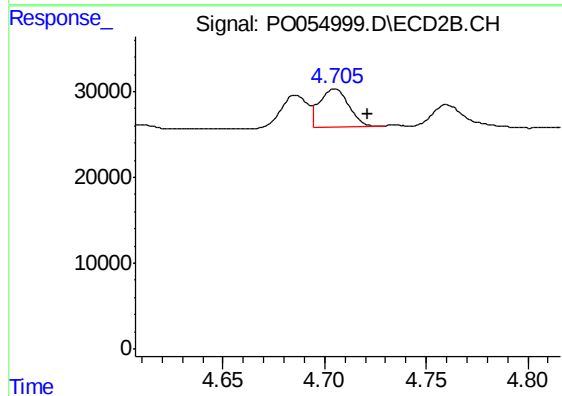

#12 AR-1232-2

R.T.: 4.705 min
Delta R.T.: -0.016 min
Response: 44858
Conc: 52.09 ng/ml

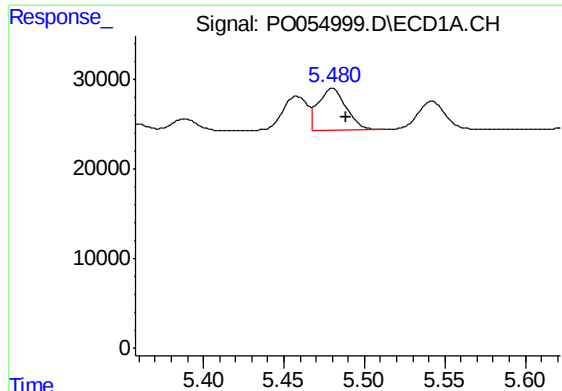


#13 AR-1232-3

R.T.: 5.480 min
Delta R.T.: -0.008 min
Response: 56326
Conc: 57.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:24:48 PM

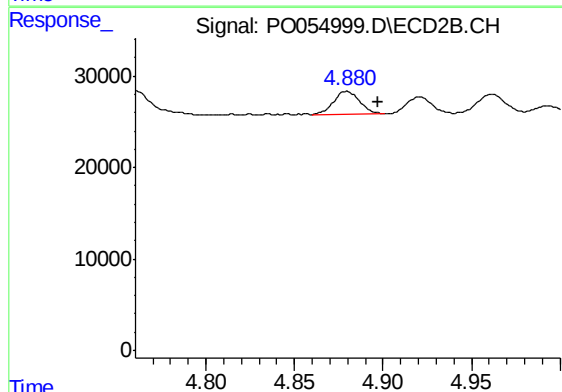


#13 AR-1232-3

R.T.: 4.880 min
Delta R.T.: -0.017 min
Response: 25315
Conc: 52.24 ng/ml

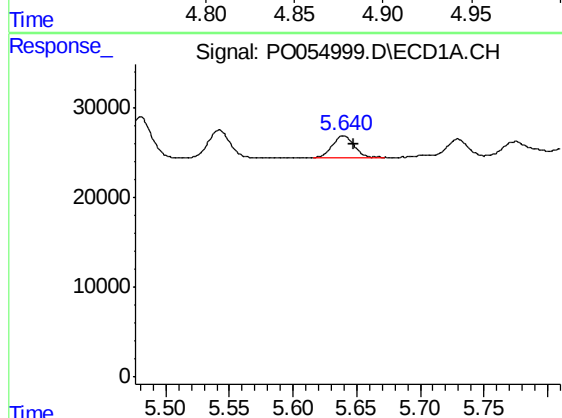


#14 AR-1232-4

R.T.: 5.640 min
Delta R.T.: -0.008 min
Response: 29517
Conc: 57.67 ng/ml m

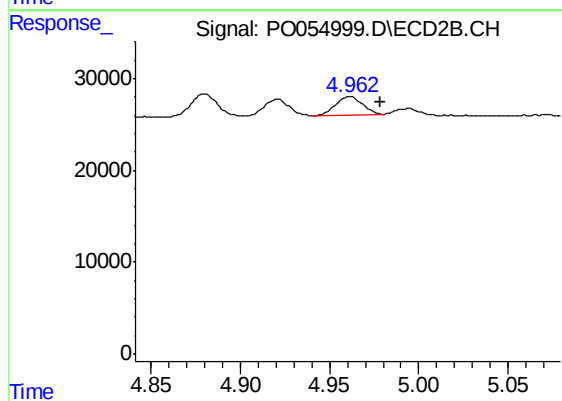

#14 AR-1232-4

R.T.: 4.962 min
Delta R.T.: -0.017 min
Response: 20693
Conc: 47.09 ng/ml

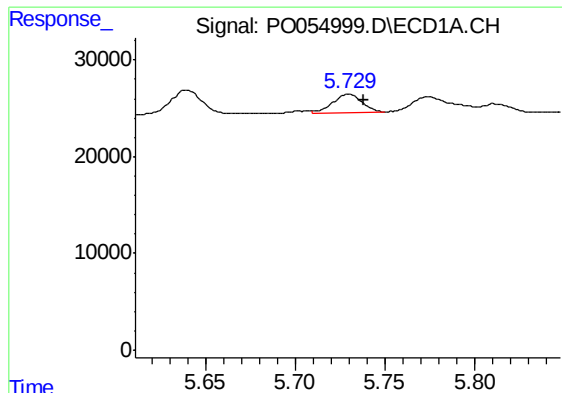


#15 AR-1232-5

R.T.: 5.729 min
Delta R.T.: -0.009 min
Response: 21380
Conc: 51.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

Sohil
4/8/2019 5:24:48 PM

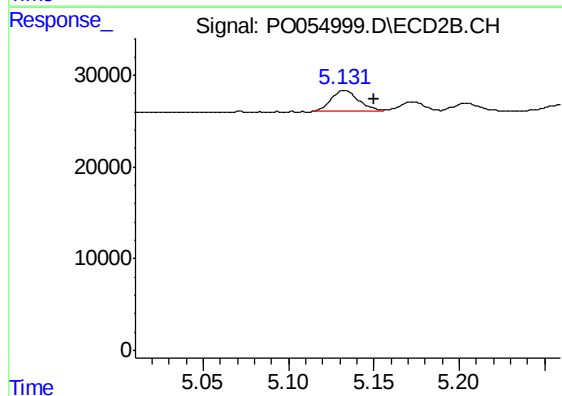

#15 AR-1232-5

R.T.: 5.131 min
Delta R.T.: -0.019 min
Response: 25346
Conc: 52.11 ng/ml m