

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040519\
 Data File : P0055005.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2019 00:55
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1248 LOD 40PPB
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

Sohil
 4/8/2019 5:25:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 04:04:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.297	3.610	904631	819398	26.066	25.676
2)	SA Decachlor...	9.911	8.578	1049554	740187	21.290	23.241
Target Compounds							
21)	L5 AR-1248-1	5.458	4.686	63290	53731	63.311	61.212m
22)	L5 AR-1248-2	5.729	4.921	96498	75816	66.445	62.733
23)	L5 AR-1248-3	5.931	4.962	103601	78131	64.865	62.616
24)	L5 AR-1248-4	6.334	5.132	116435	95590	61.982	62.765m
25)	L5 AR-1248-5	6.372	5.523	111320	88764	62.093	59.538m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040519\
Data File : PO055005.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2019 00:55
Operator : SM/SJ
Sample : K1560-07
Misc : AR1248 LOD 40PPB
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 04:04:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

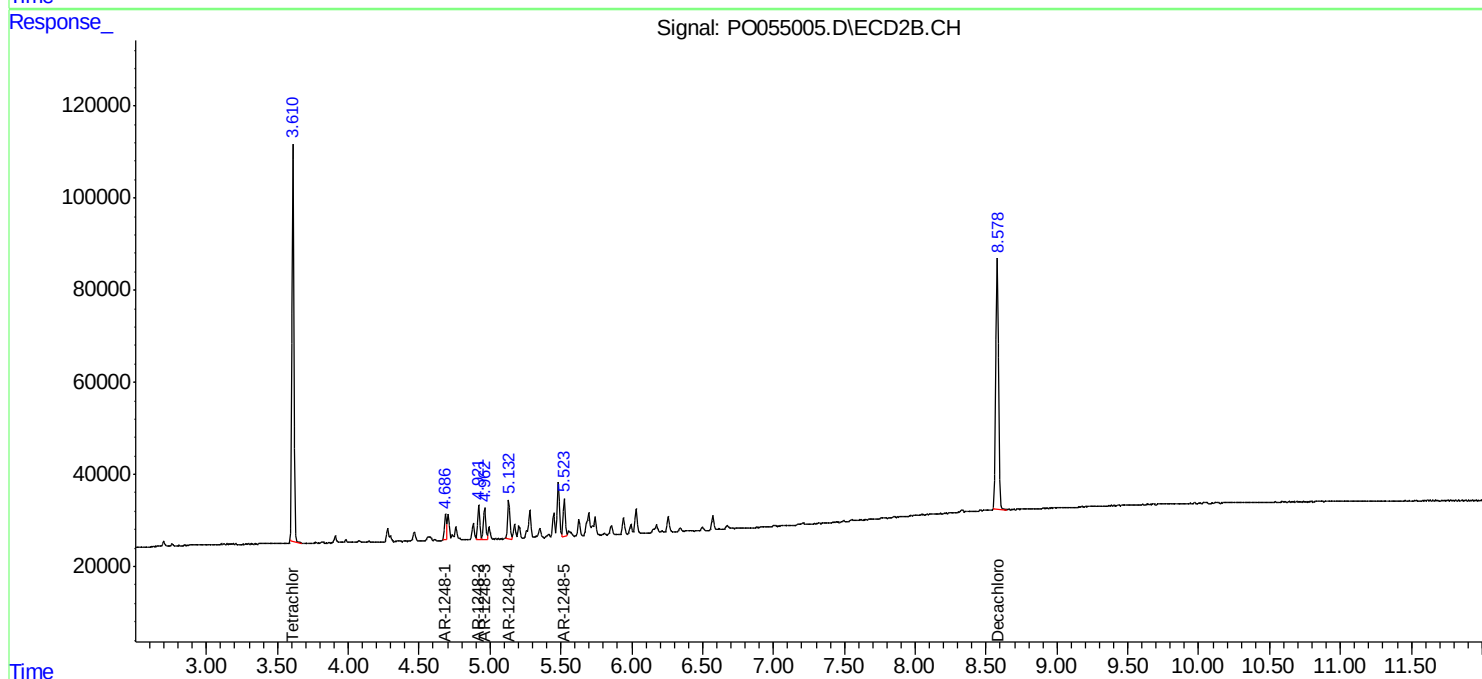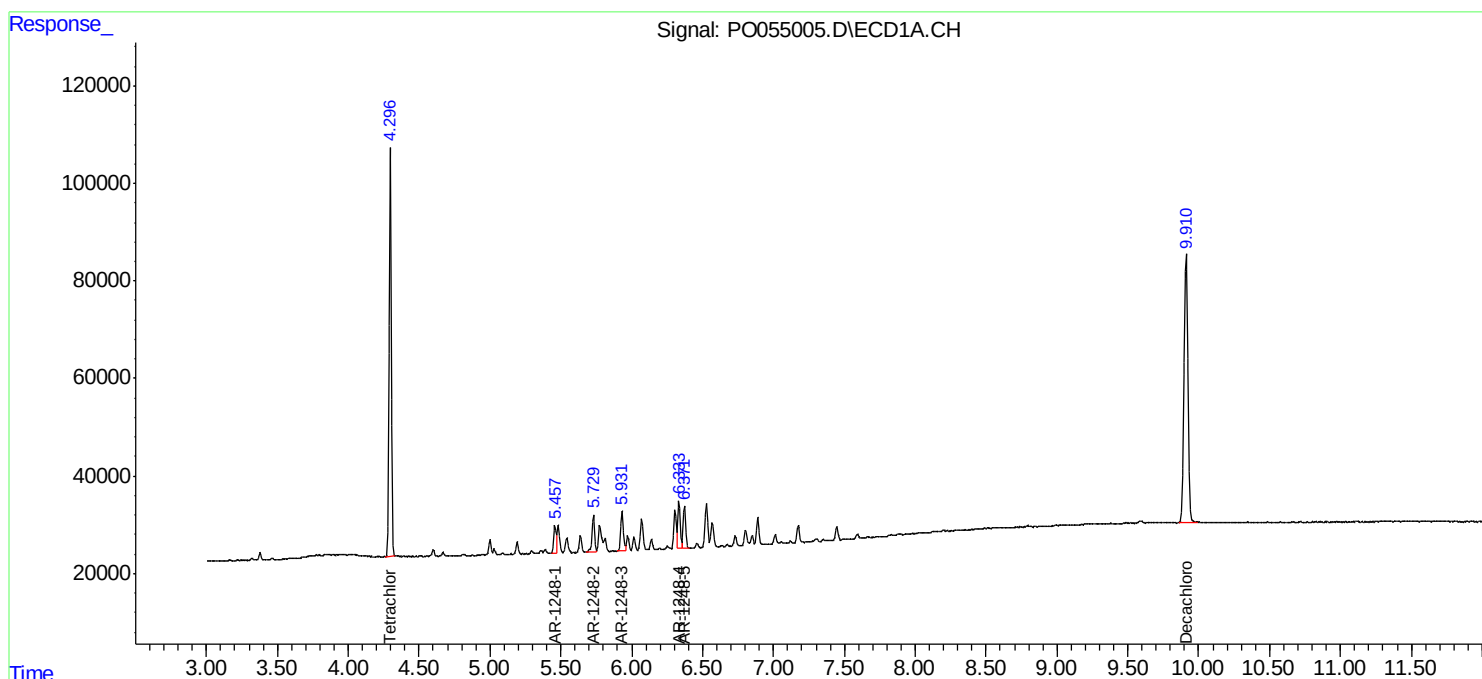

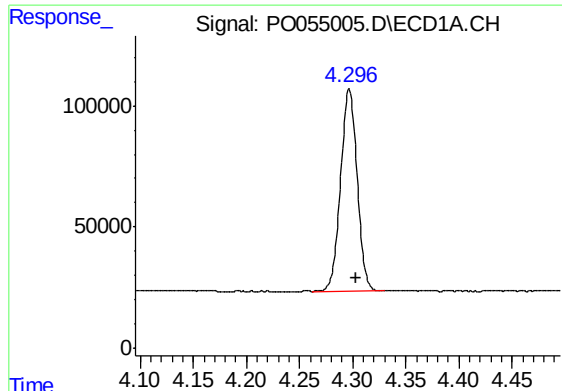


#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: -0.006 min
Response: 904631
Conc: 26.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:13 PM

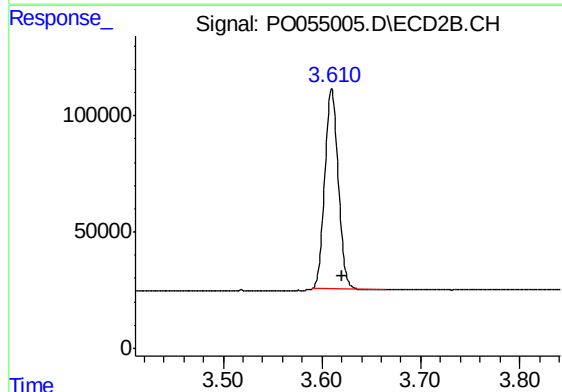


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.011 min
Response: 819398
Conc: 25.68 ng/ml

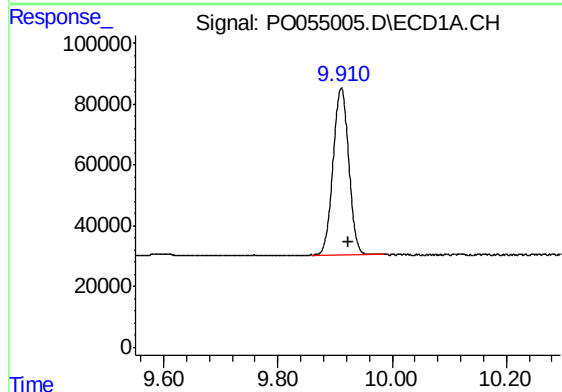


#2 Decachlorobiphenyl

R.T.: 9.911 min
Delta R.T.: -0.012 min
Response: 1049554
Conc: 21.29 ng/ml

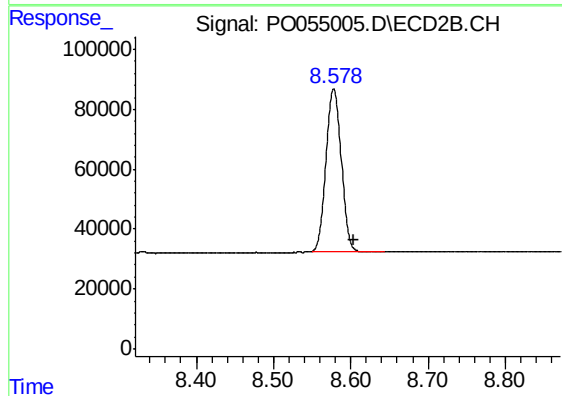

#2 Decachlorobiphenyl

R.T.: 8.578 min
Delta R.T.: -0.026 min
Response: 740187
Conc: 23.24 ng/ml

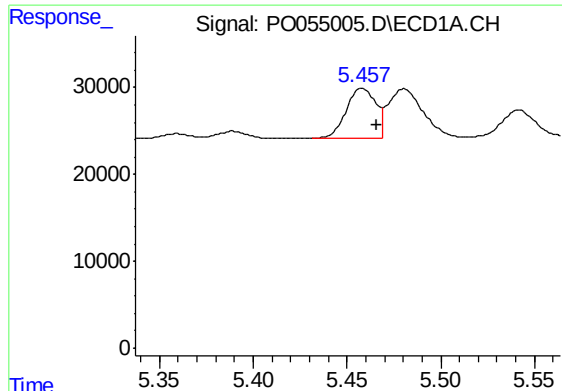


#21 AR-1248-1

R.T.: 5.458 min
Delta R.T.: -0.008 min
Response: 63290
Conc: 63.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:13 PM

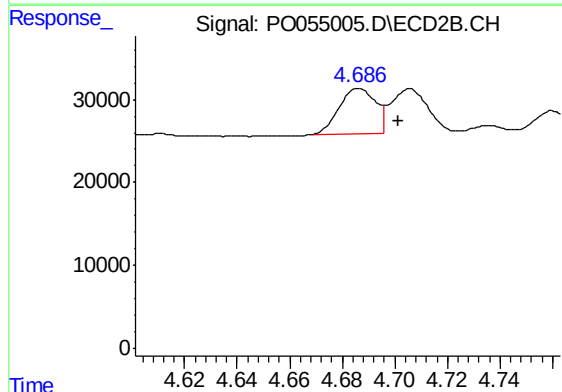


#21 AR-1248-1

R.T.: 4.686 min
Delta R.T.: -0.015 min
Response: 53731
Conc: 61.21 ng/ml m

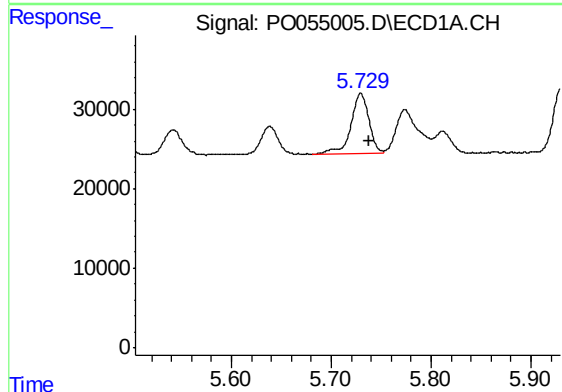


#22 AR-1248-2

R.T.: 5.729 min
Delta R.T.: -0.008 min
Response: 96498
Conc: 66.44 ng/ml

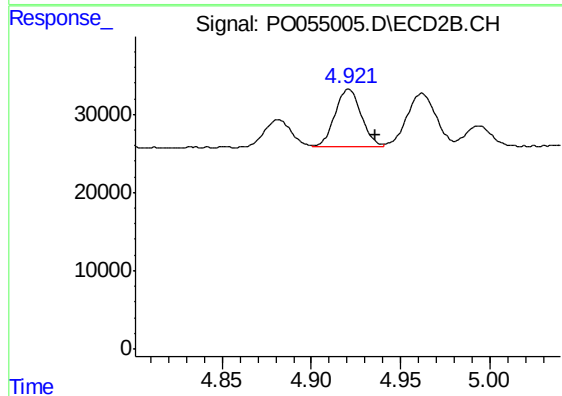

#22 AR-1248-2

R.T.: 4.921 min
Delta R.T.: -0.015 min
Response: 75816
Conc: 62.73 ng/ml

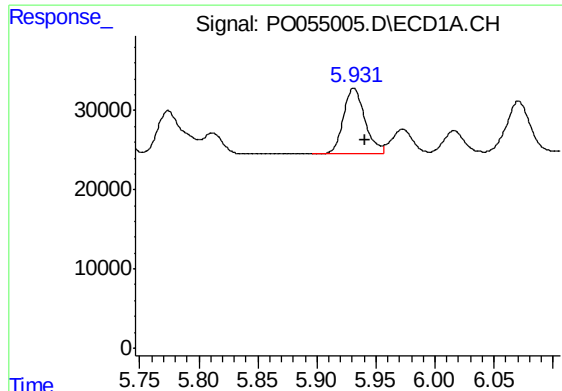


#23 AR-1248-3

R.T.: 5.931 min
Delta R.T.: -0.009 min
Response: 103601
Conc: 64.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:13 PM

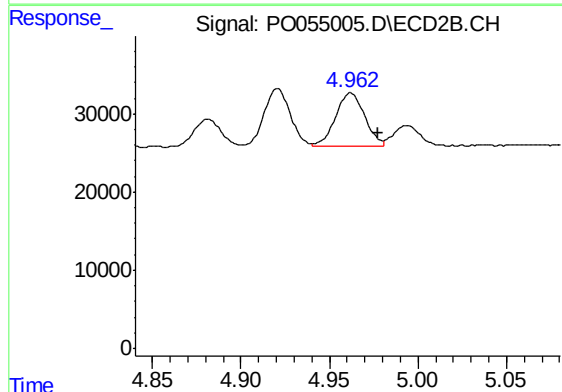


#23 AR-1248-3

R.T.: 4.962 min
Delta R.T.: -0.015 min
Response: 78131
Conc: 62.62 ng/ml

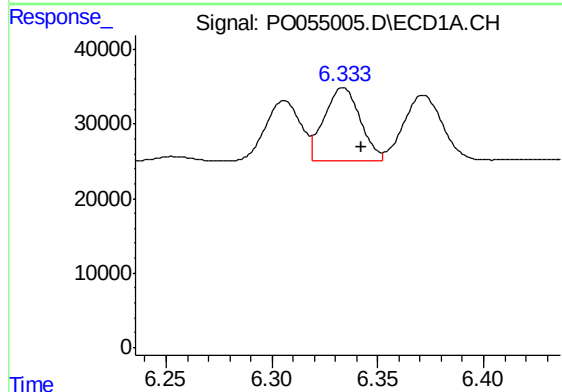


#24 AR-1248-4

R.T.: 6.334 min
Delta R.T.: -0.008 min
Response: 116435
Conc: 61.98 ng/ml

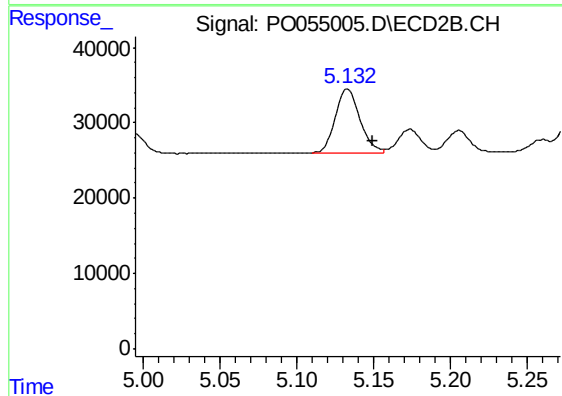

#24 AR-1248-4

R.T.: 5.132 min
Delta R.T.: -0.017 min
Response: 95590
Conc: 62.76 ng/ml m

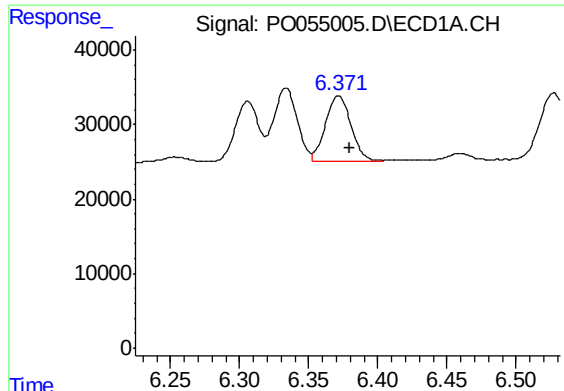


#25 AR-1248-5

R.T.: 6.372 min
Delta R.T.: -0.009 min
Response: 111320
Conc: 62.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:13 PM

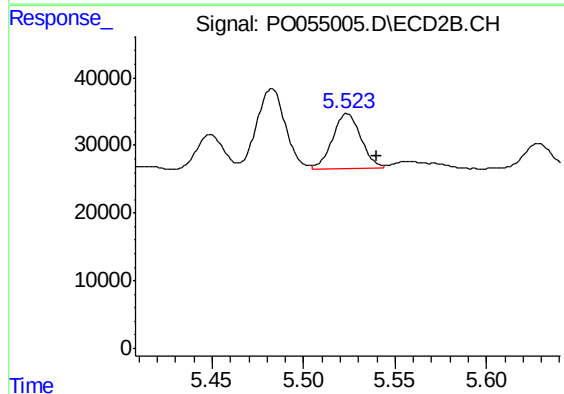

#25 AR-1248-5

R.T.: 5.523 min
Delta R.T.: -0.017 min
Response: 88764
Conc: 59.54 ng/ml m