

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040519\
 Data File : P0055007.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2019 1:29
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

Sohil
 4/8/2019 5:25:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 04:05:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.297	3.610	969392	871363	27.932	27.305
2)	SA Decachlor...	9.911	8.578	1131255	791887	22.947	24.864
Target Compounds							
26)	L6 AR-1254-1	6.307	5.483	80083	89665	44.167	41.028
27)	L6 AR-1254-2	6.524	5.629	122611	80178	42.950	41.351
28)	L6 AR-1254-3	6.889	6.031	126816	121123	40.327	37.784
29)	L6 AR-1254-4	7.174	6.257	91929	76038	37.578	38.836m
30)	L6 AR-1254-5	7.591	6.673	80637	101099	30.085	35.169

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040519\
Data File : PO055007.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2019 1:29
Operator : SM/SJ
Sample : K1560-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 04:05:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

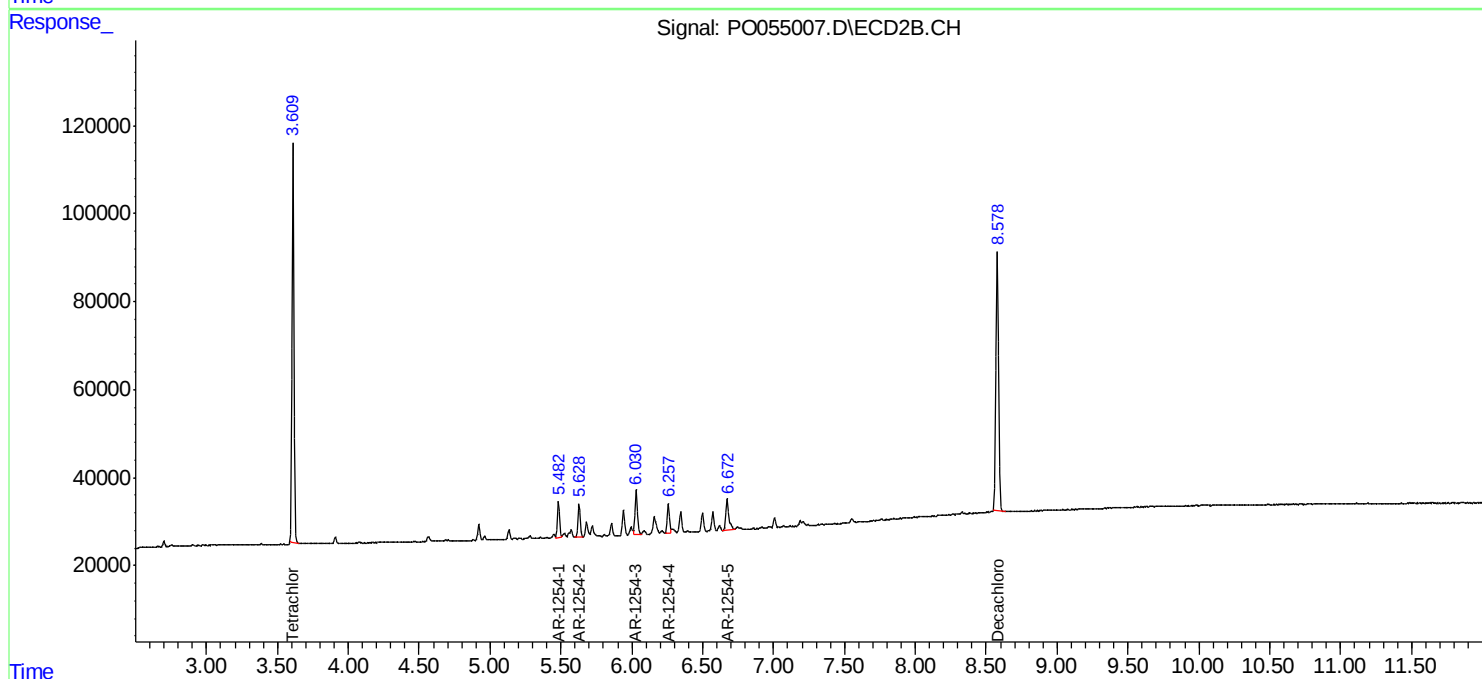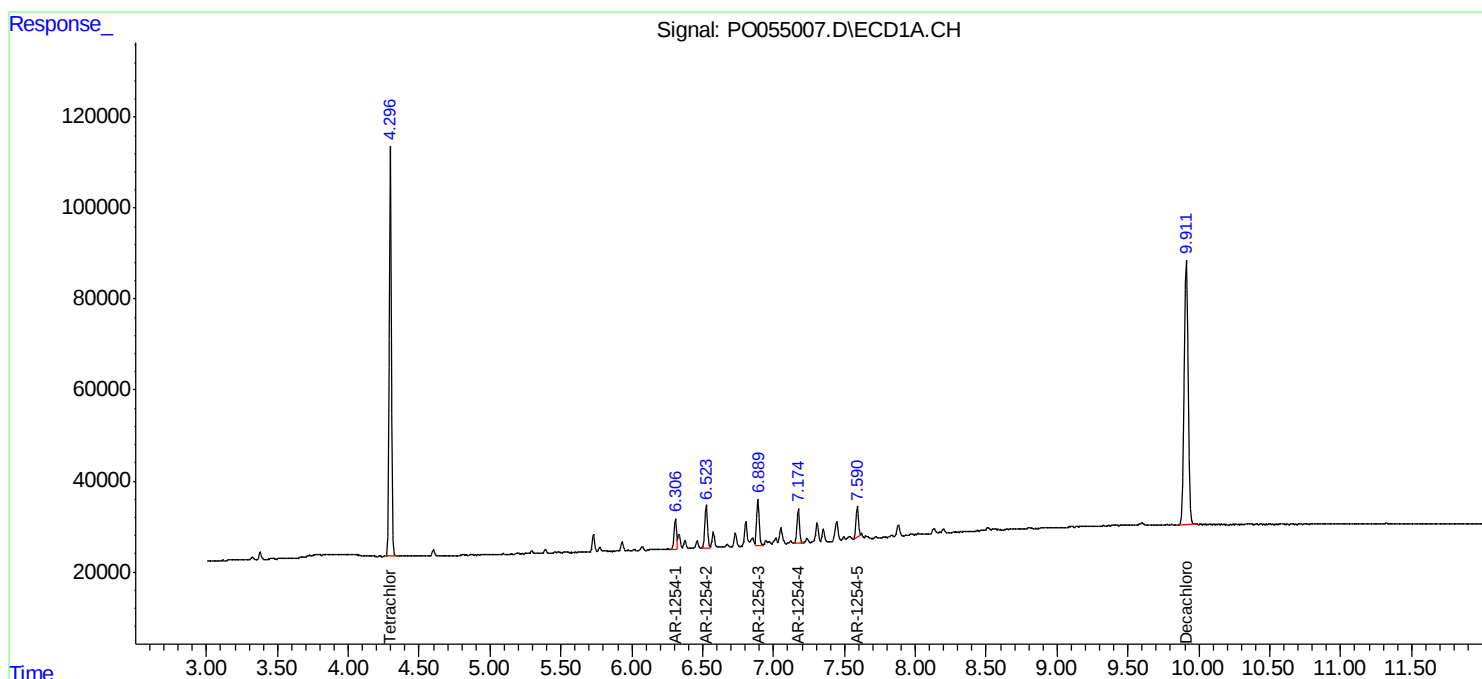

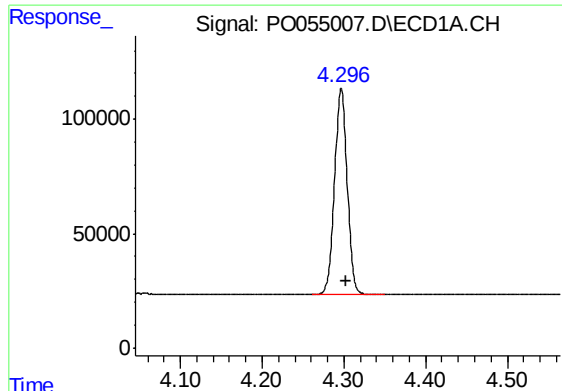


#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: -0.006 min
Response: 969392
Conc: 27.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:19 PM

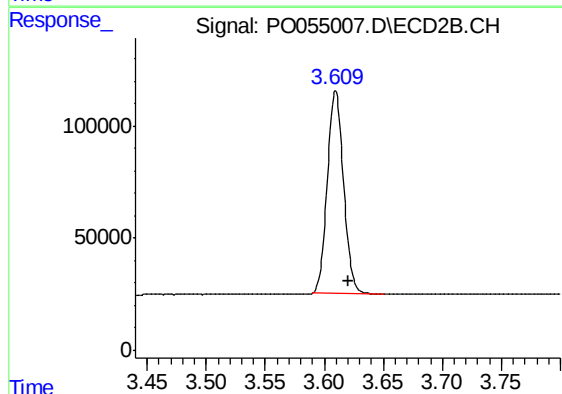


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.011 min
Response: 871363
Conc: 27.30 ng/ml

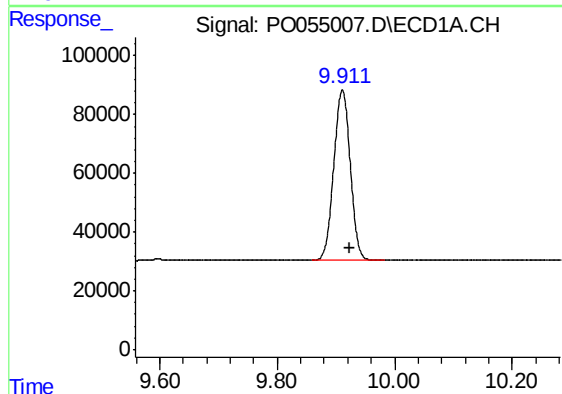


#2 Decachlorobiphenyl

R.T.: 9.911 min
Delta R.T.: -0.012 min
Response: 1131255
Conc: 22.95 ng/ml

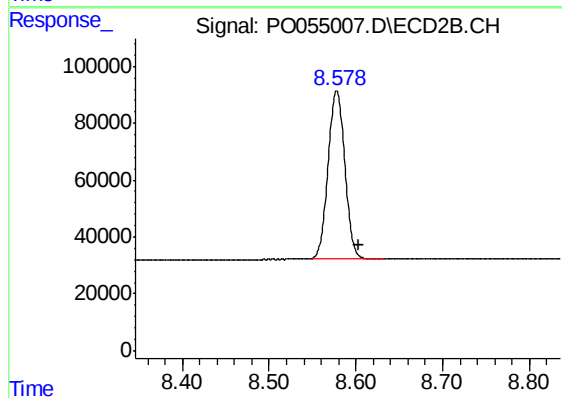

#2 Decachlorobiphenyl

R.T.: 8.578 min
Delta R.T.: -0.026 min
Response: 791887
Conc: 24.86 ng/ml

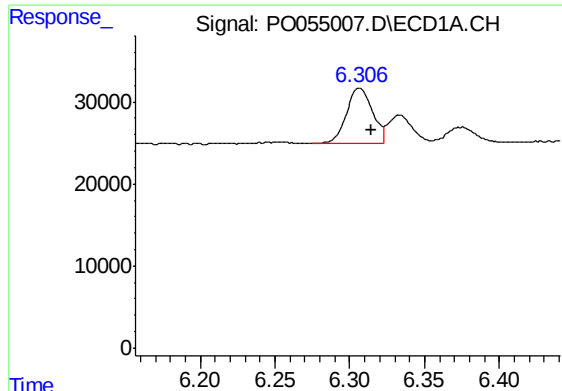


#26 AR-1254-1

R.T.: 6.307 min
Delta R.T.: -0.008 min
Response: 80083
Conc: 44.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:19 PM

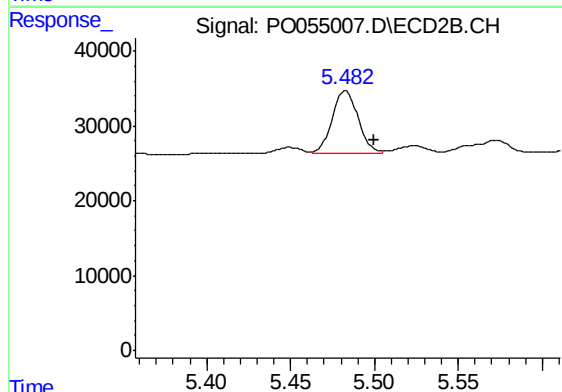


#26 AR-1254-1

R.T.: 5.483 min
Delta R.T.: -0.017 min
Response: 89665
Conc: 41.03 ng/ml

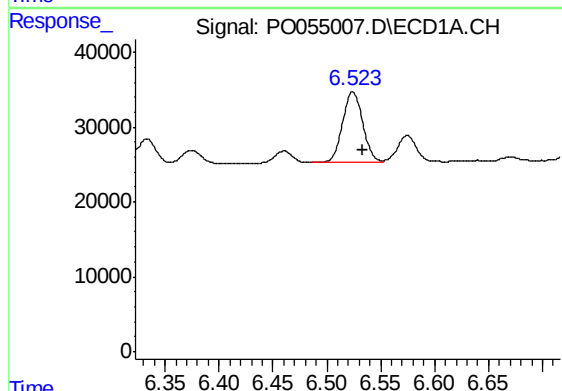


#27 AR-1254-2

R.T.: 6.524 min
Delta R.T.: -0.009 min
Response: 122611
Conc: 42.95 ng/ml

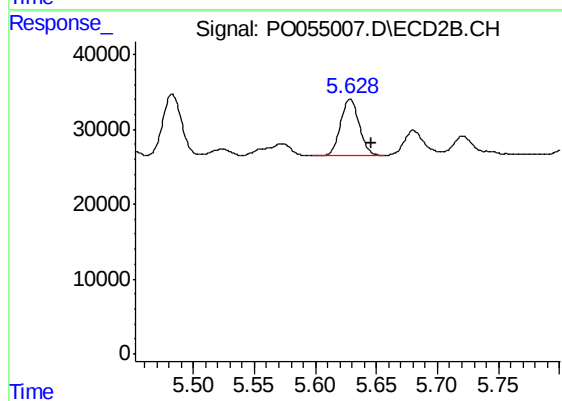

#27 AR-1254-2

R.T.: 5.629 min
Delta R.T.: -0.017 min
Response: 80178
Conc: 41.35 ng/ml

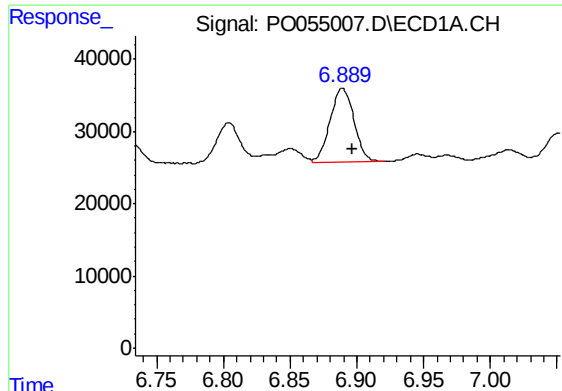


#28 AR-1254-3

R.T.: 6.889 min
Delta R.T.: -0.008 min
Response: 126816
Conc: 40.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:19 PM

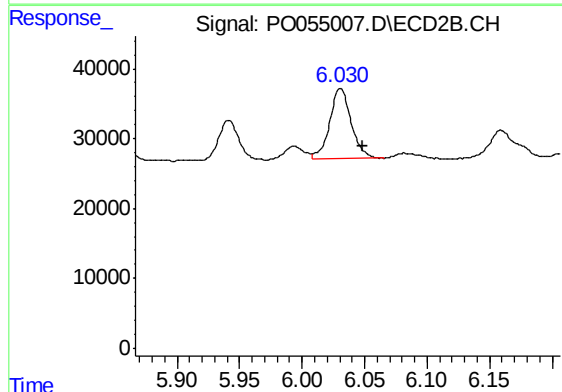


#28 AR-1254-3

R.T.: 6.031 min
Delta R.T.: -0.018 min
Response: 121123
Conc: 37.78 ng/ml

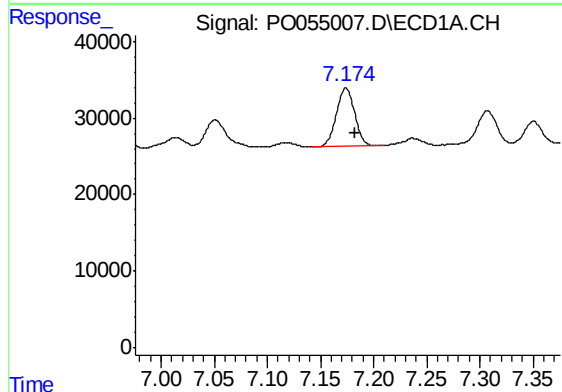


#29 AR-1254-4

R.T.: 7.174 min
Delta R.T.: -0.008 min
Response: 91929
Conc: 37.58 ng/ml

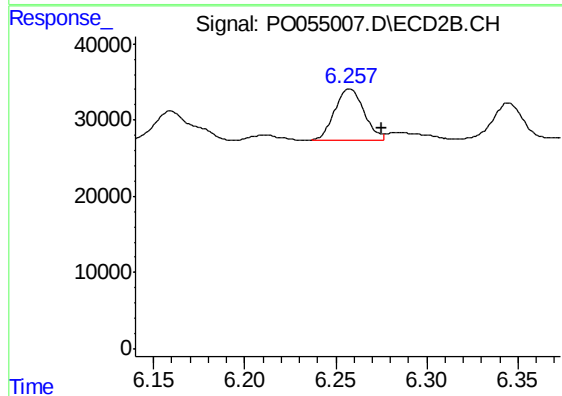

#29 AR-1254-4

R.T.: 6.257 min
Delta R.T.: -0.019 min
Response: 76038
Conc: 38.84 ng/ml m

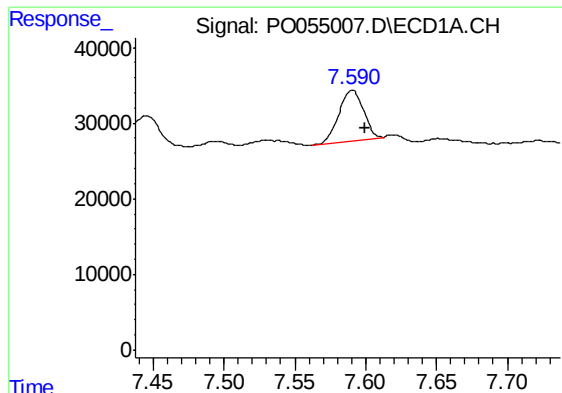


#30 AR-1254-5

R.T.: 7.591 min
Delta R.T.: -0.009 min
Response: 80637
Conc: 30.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:19 PM

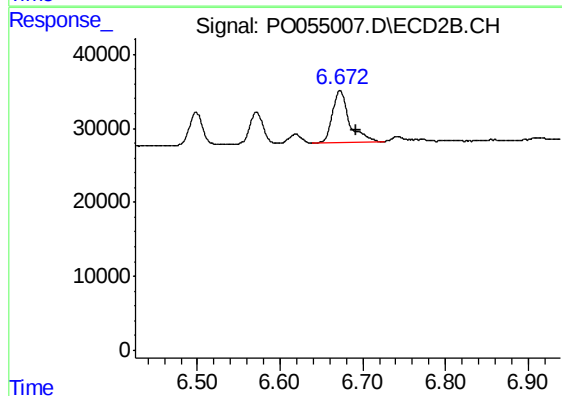

#30 AR-1254-5

R.T.: 6.673 min
Delta R.T.: -0.020 min
Response: 101099
Conc: 35.17 ng/ml